
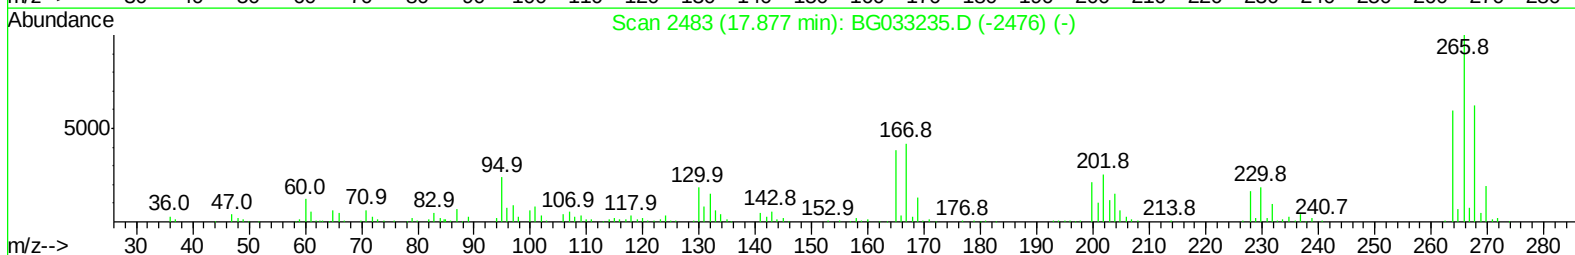
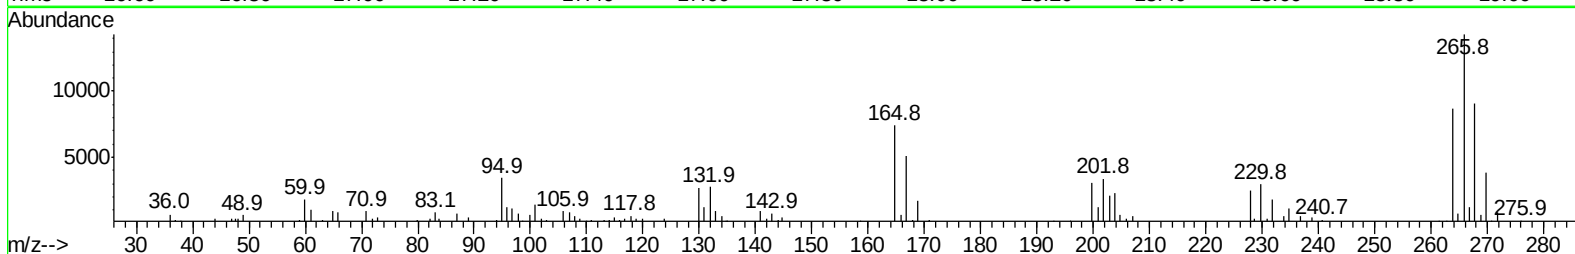


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033628.D
Acq On : 6 Apr 2018 14:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:31:39 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

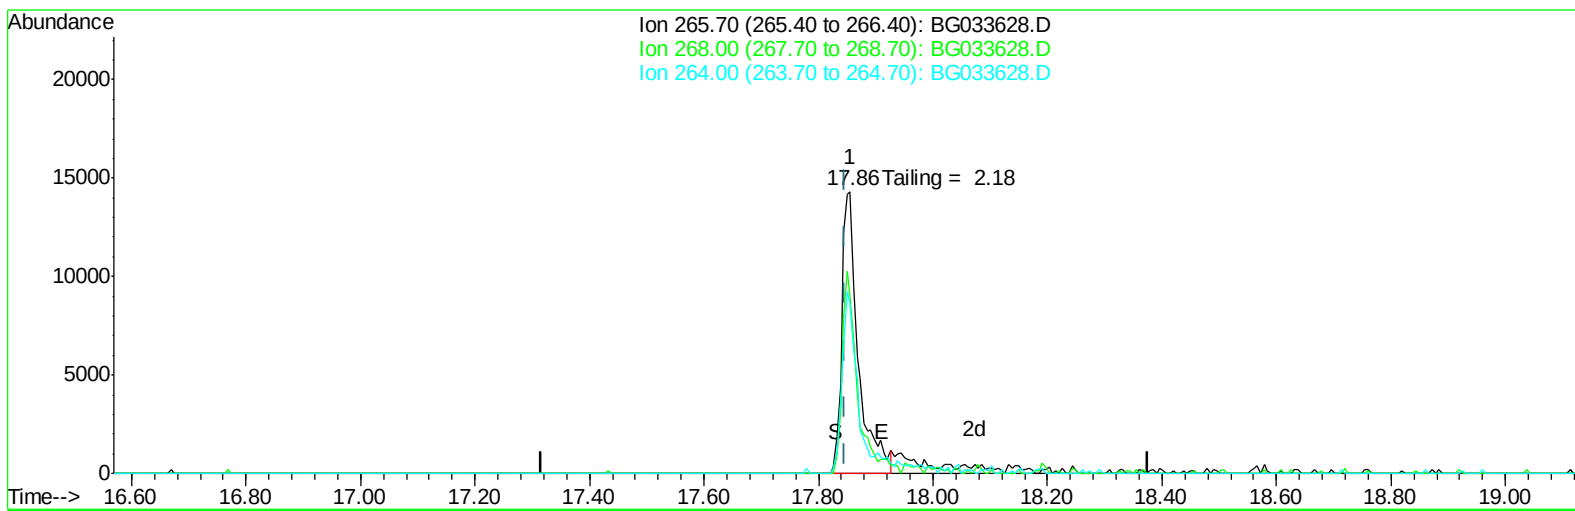

TIC: BG033628.D

(69) Pentachlorophenol (C)




17.856min (+0.008) 0.00ng

response 28547

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.12
264.00	62.00	65.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033628.D
Acq On : 6 Apr 2018 14:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:31:39 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

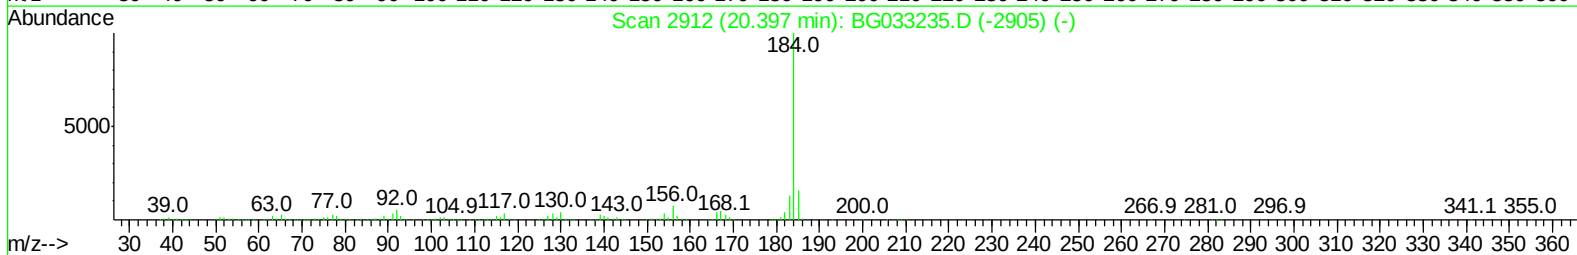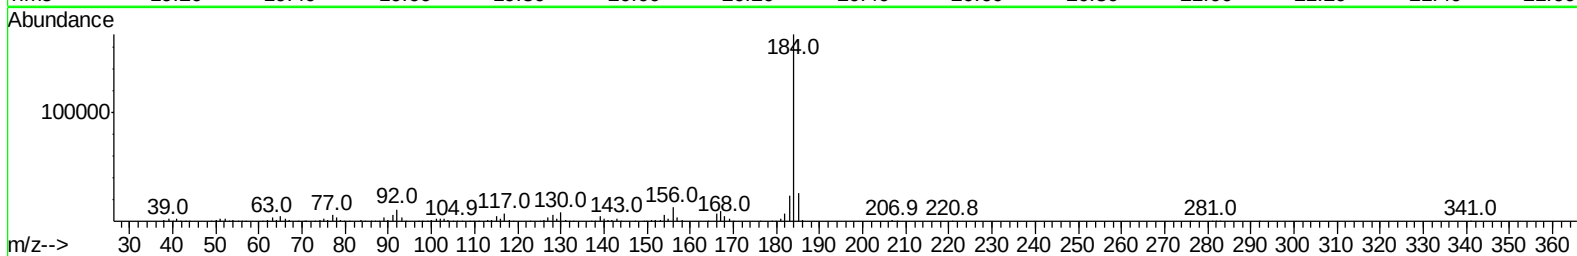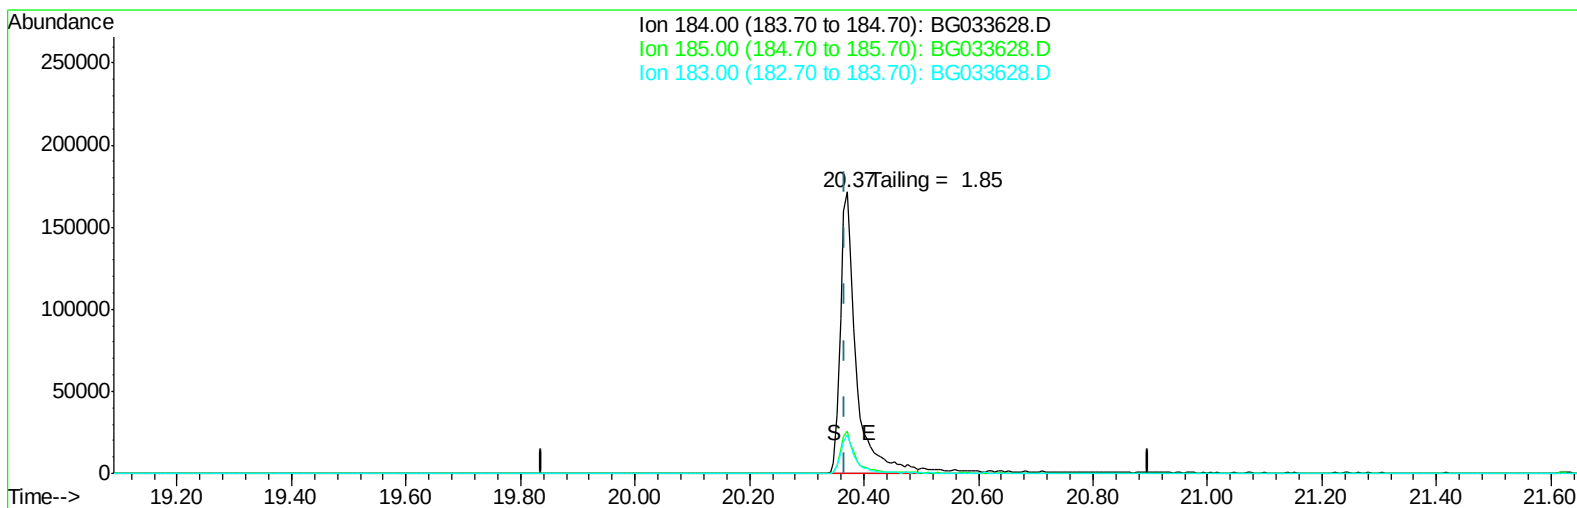

TIC: BG033628.D

(76) Benzidine

20.370min (+0.003) 139839.52ng

response 329925

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.21
183.00	13.30	13.47
0.00	0.00	0.00