
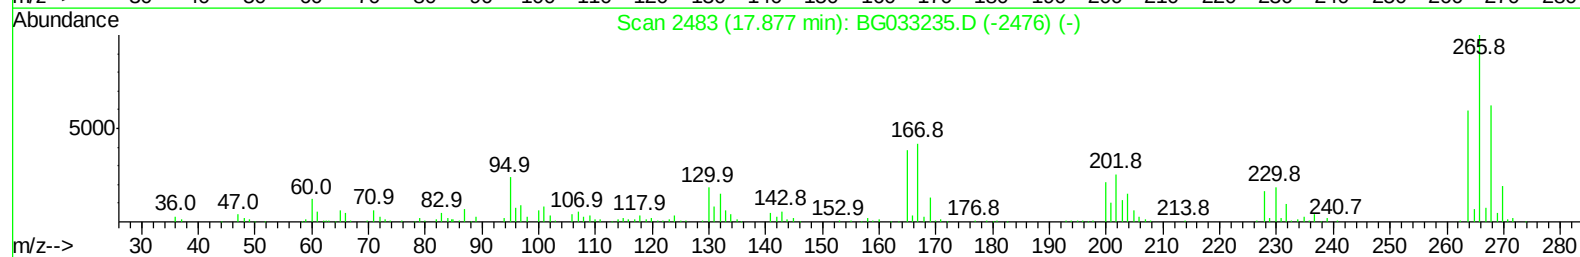
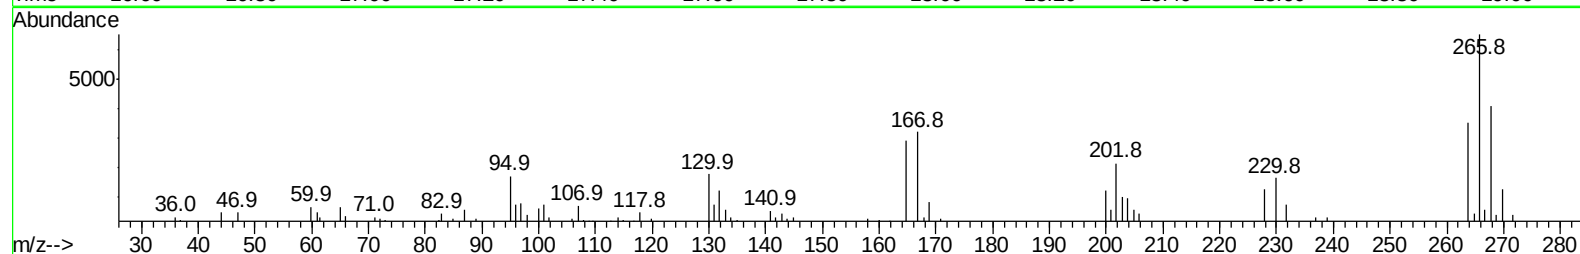


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033646.D
Acq On : 7 Apr 2018 2:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:35:08 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

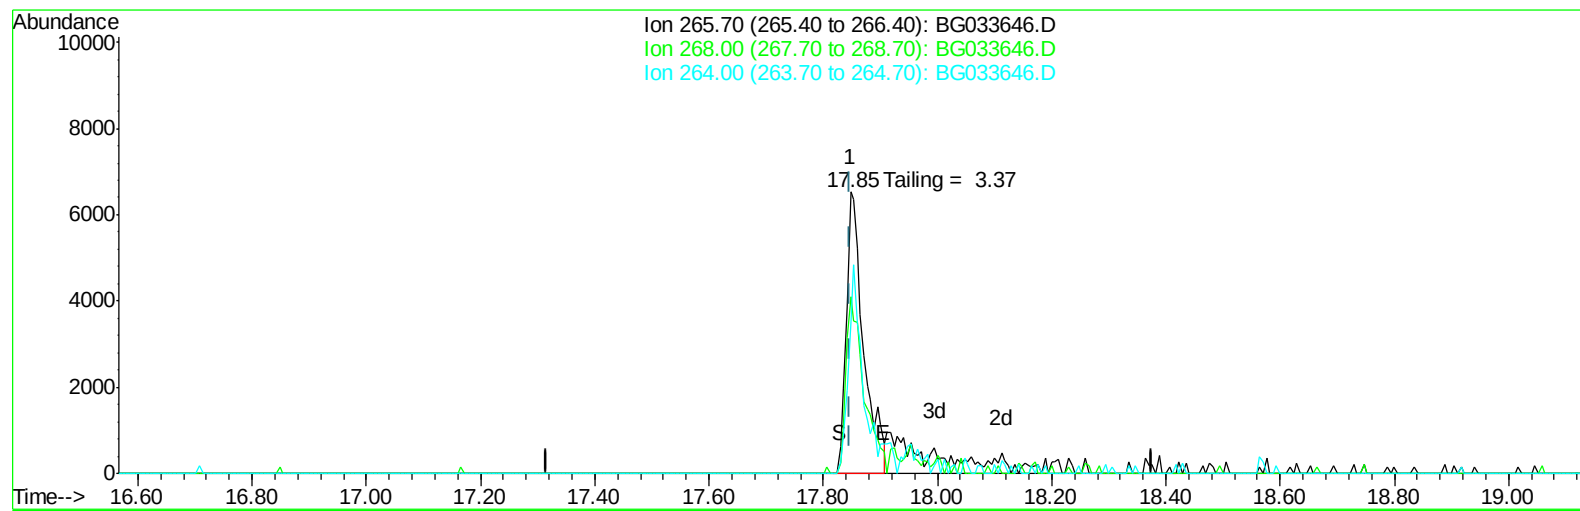

TIC: BG033646.D

(69) Pentachlorophenol (C)




17.848min (+0.000) 4501.27ng

response 13785

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.11
264.00	62.00	54.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033646.D
Acq On : 7 Apr 2018 2:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:35:08 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

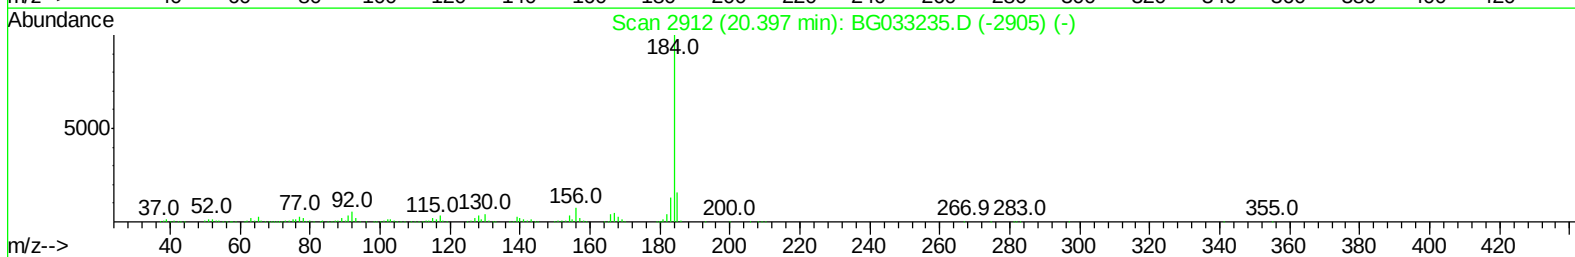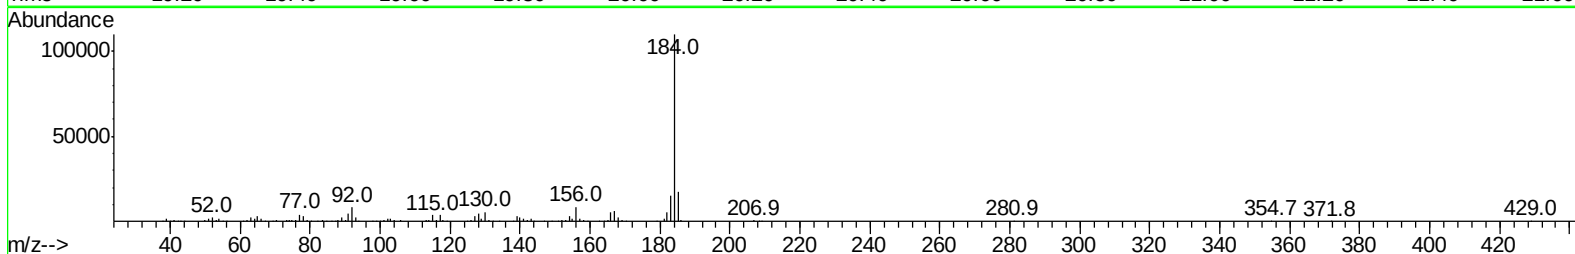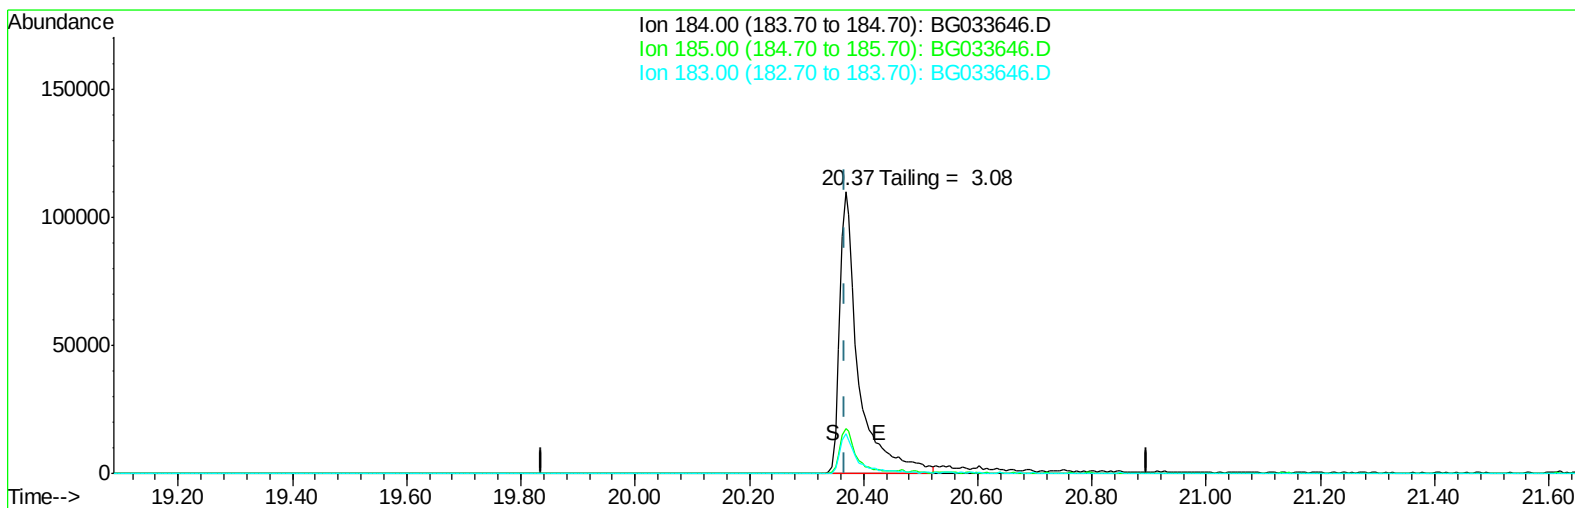

TIC: BG033646.D

(76) Benzidine

20.368min (+0.000) 0.00ng

response 251581

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.01
183.00	13.30	13.92
0.00	0.00	0.00