
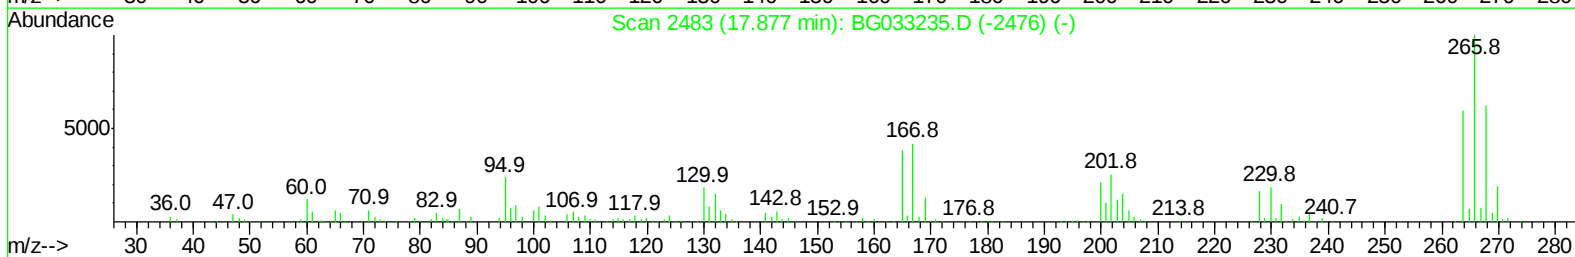
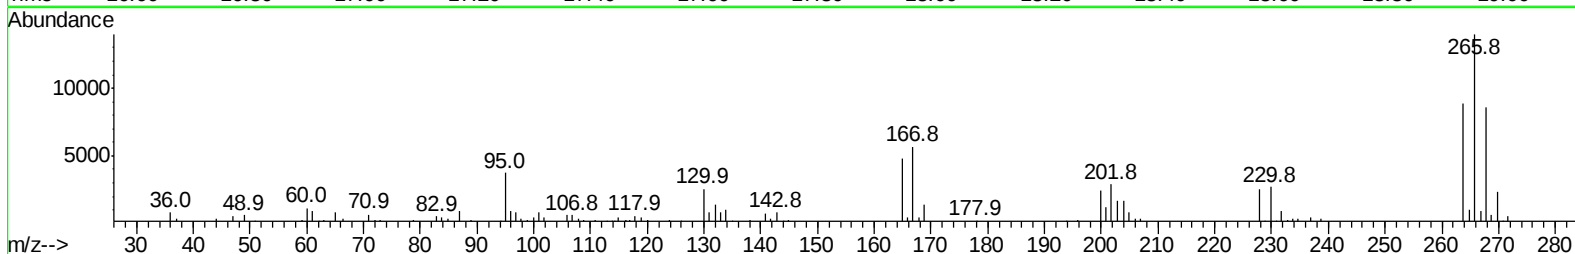


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033665.D
Acq On : 7 Apr 2018 15:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:36:16 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

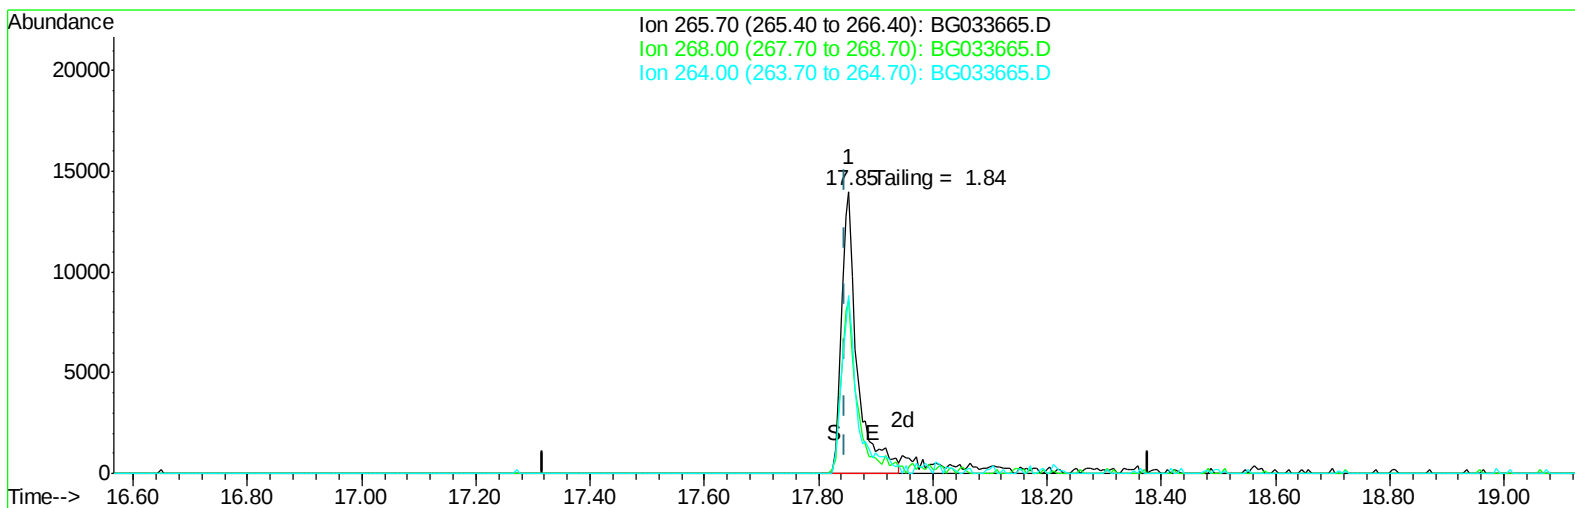

TIC: BG033665.D

(69) Pentachlorophenol (C)




17.853min (+0.005) 12594.41ng

response 26999

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.78
264.00	62.00	63.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033665.D
Acq On : 7 Apr 2018 15:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 04:36:16 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

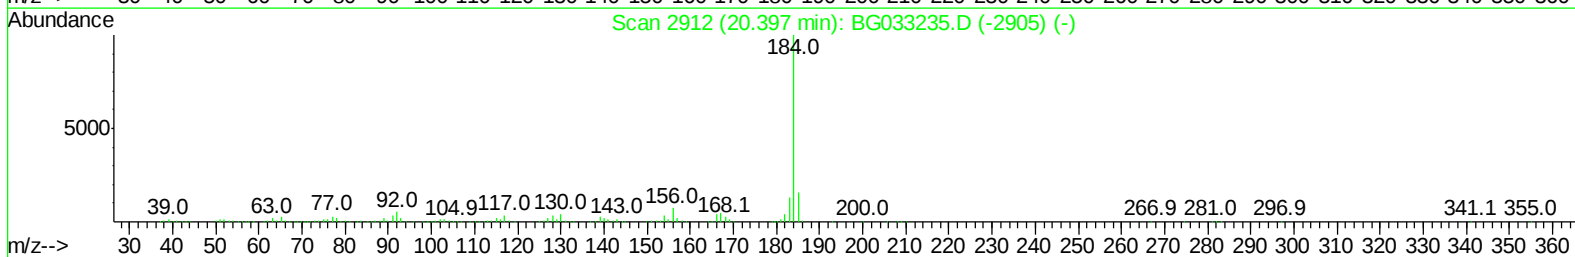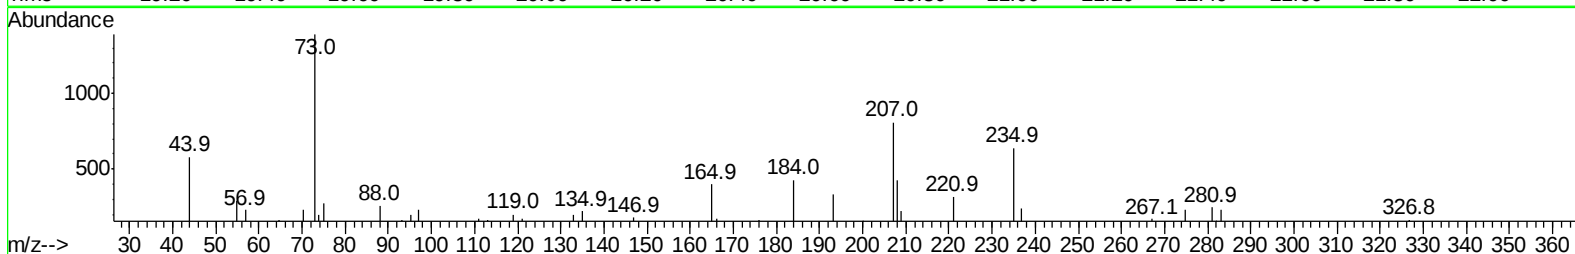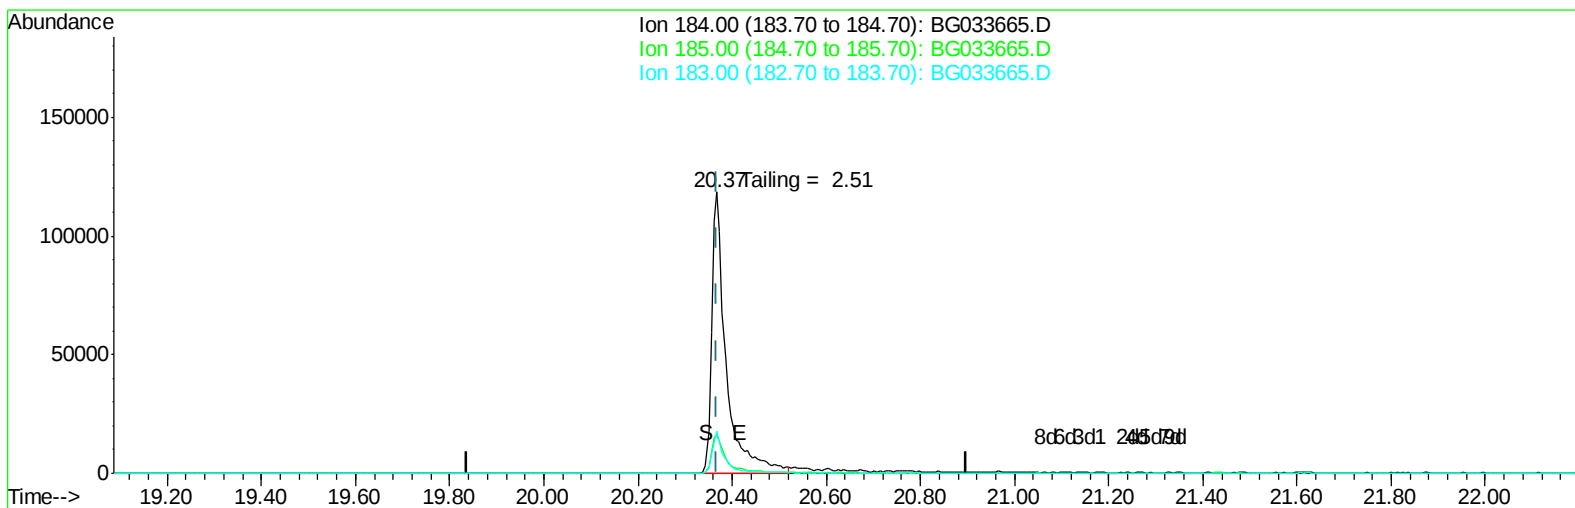

TIC: BG033665.D

(76) Benzidine

21.184min (+0.816) 157.80ng

response 291

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00