

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
 Data File : BG033641.D
 Acq On : 6 Apr 2018 23:12
 Operator : SJ/JU
 Sample : J2232-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CV-RB26667RT

Quant Time: Apr 07 01:29:49 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 05 17:36:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	35150	20.00	ng	0.00
21) Naphthalene-d8	11.74	136	165450	20.00	ng	0.00
38) Acenaphthene-d10	15.48	164	128571	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	310572	20.00	ng	0.00
75) Chrysene-d12	22.56	240	313381	20.00	ng	0.00
86) Perylene-d12	26.33	264	289644	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	325112	173.44	ng	0.00
7) Phenol-d6	7.97	99	447630	138.98	ng	0.00
23) Nitrobenzene-d5	10.06	82	351934	97.73	ng	0.00
41) 2,4,6-Tribromophenol	16.95	330	234766	122.09	ng	0.00
44) 2-Fluorobiphenyl	14.11	172	889906	99.92	ng	0.00
78) Terphenyl-d14	20.73	244	1504298	102.66	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
Data File : BG033641.D
Acq On : 6 Apr 2018 23:12
Operator : SJ/JU
Sample : J2232-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CV-RB26667RT

Quant Time: Apr 07 01:29:49 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

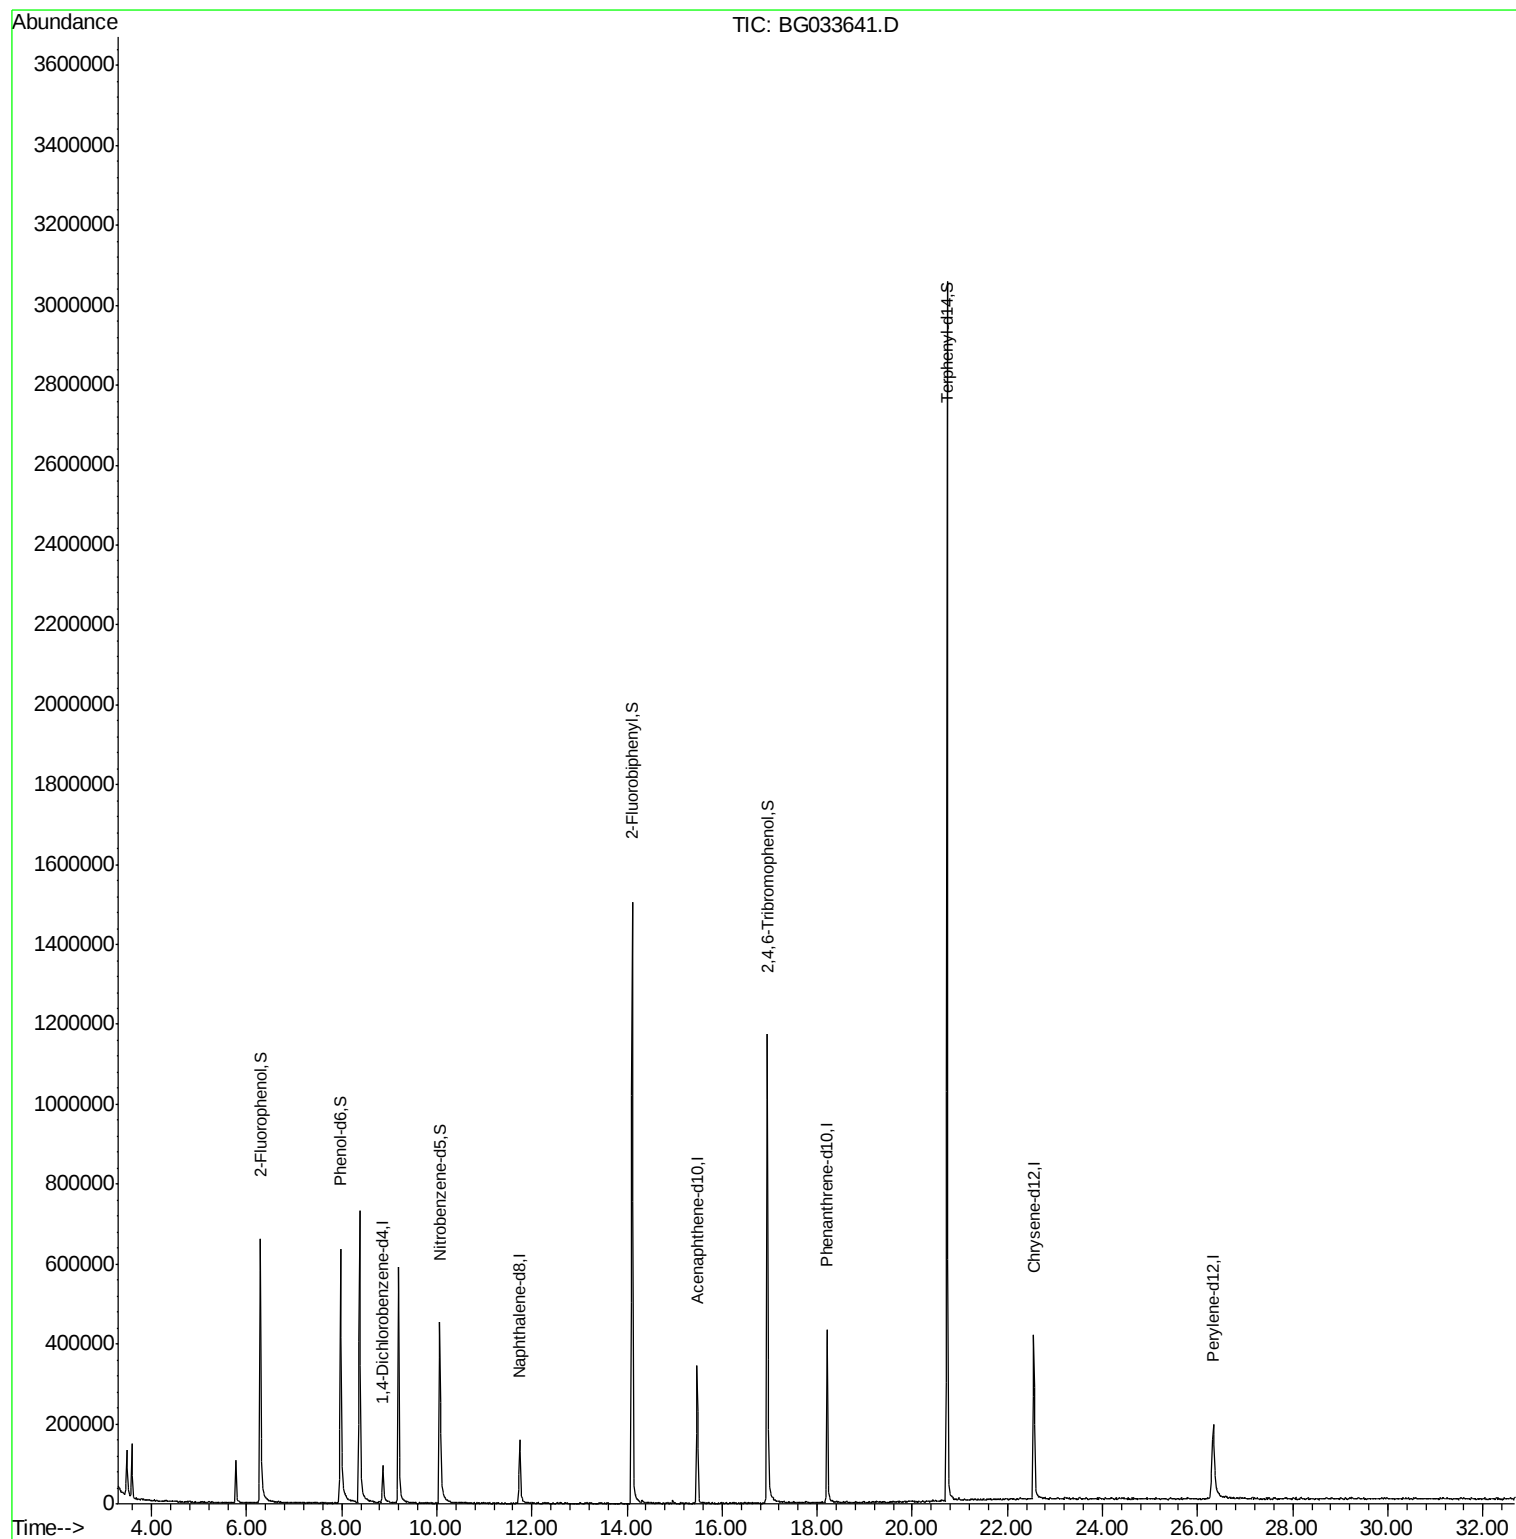

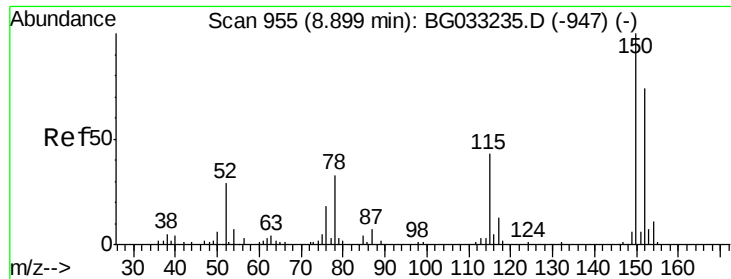

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.87 min Scan# 949

Delta R.T. 0.00 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12

Instrument :

BNA_G

ClientSampleId :

CV-RB26667RT


Tot Ion:152 Resp: 35150

Ion Ratio Lower Upper

152 100

150 142.1 126.6 189.8




115 62.6 53.0 79.4

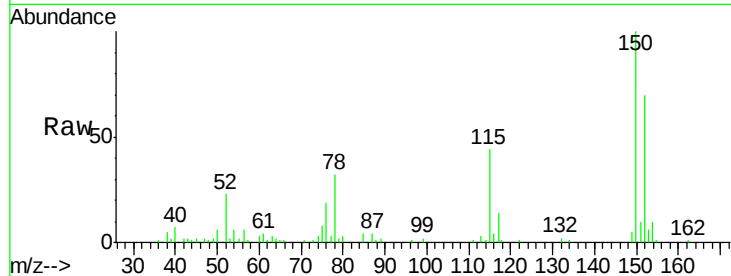

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

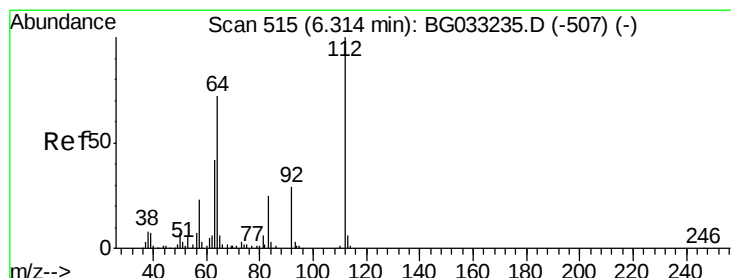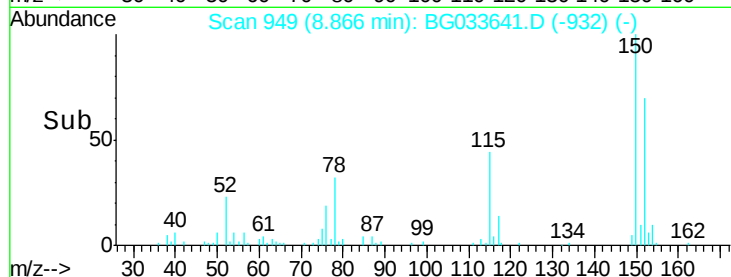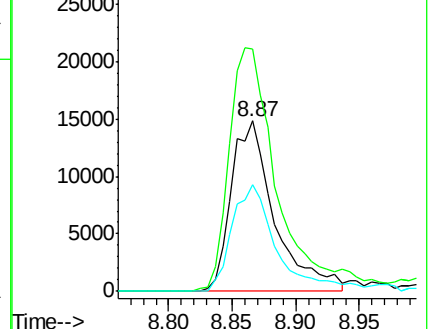

#5

2-Fluorophenol

Concen: 173.435 ng

RT: 6.29 min Scan# 510

Delta R.T. -0.00 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12


Tgt Ion:112 Resp: 325112

Ion Ratio Lower Upper

112 100

64 72.5 56.3 84.5



63 41.5 30.1 45.1

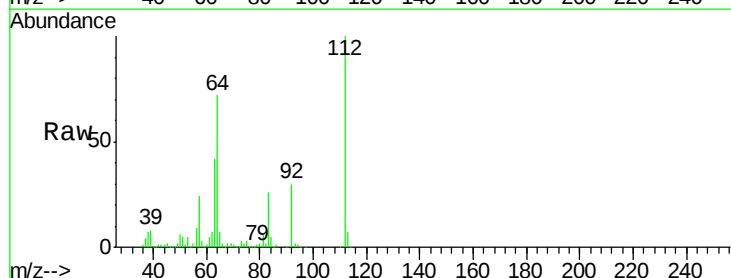


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

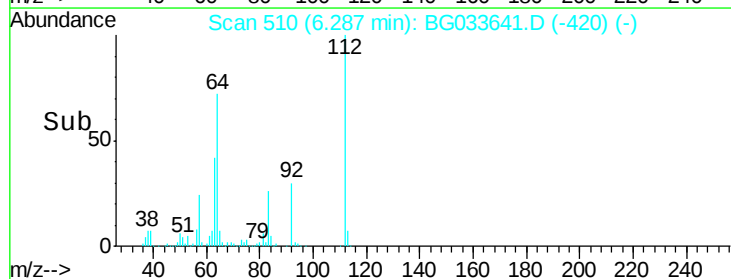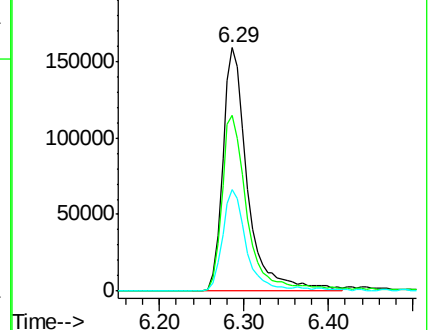

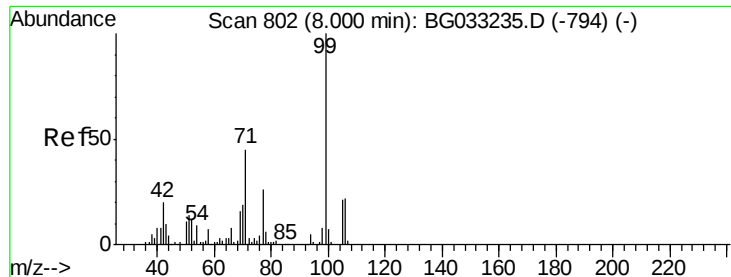

#7

Phenol-d6

Concen: 138.979 ng

RT: 7.97 min Scan# 797

Delta R.T. 0.00 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12

Instrument :

BNA_G

ClientSampleId :

CV-RB26667RT


Tot Ion: 99 Resp: 447630

Ion Ratio Lower Upper




99 100

42 21.9 14.1 21.1#

71 40.2 26.1 39.1#

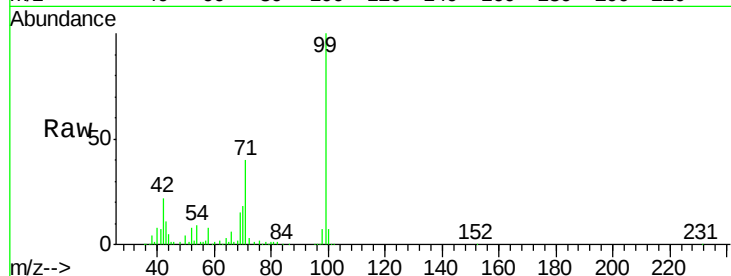

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

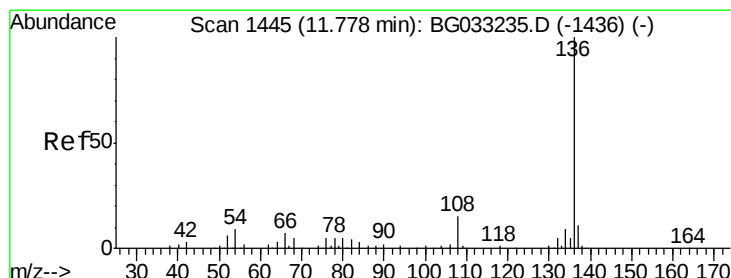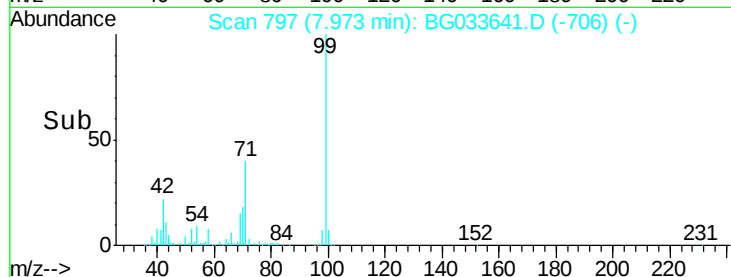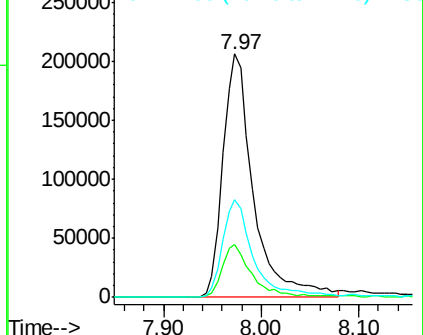

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.74 min Scan# 1439

Delta R.T. 0.00 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12

Tgt Ion: 136 Resp: 165450


Ion Ratio Lower Upper

136 100



137 10.8 9.2 13.8


54 11.2 10.3 15.5

68 5.4 4.5 6.7

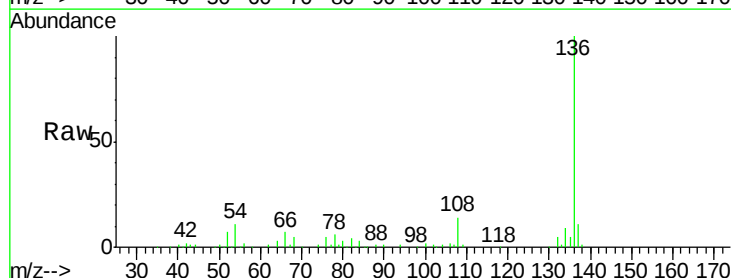

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



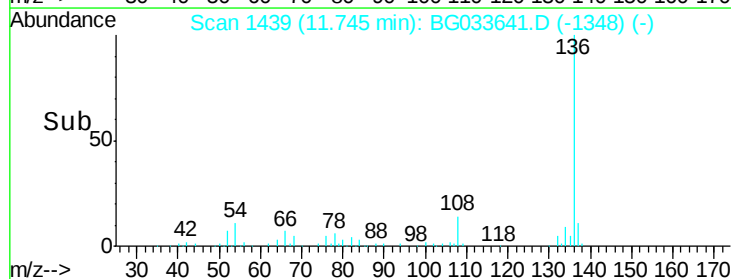
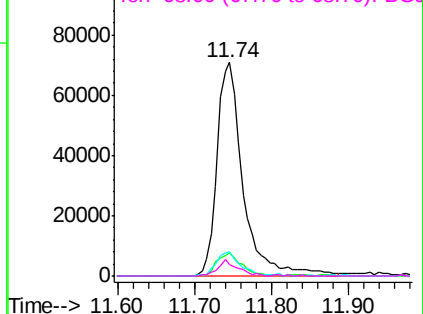


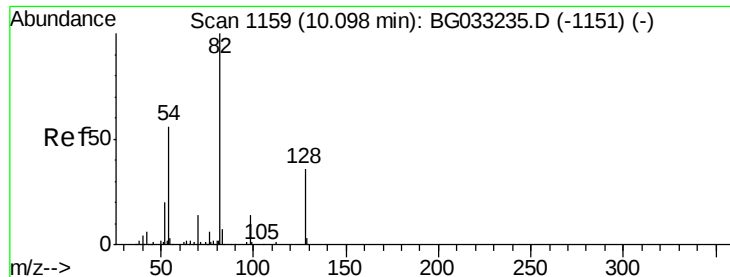

#23
 Nitrobenzene-d5
 Concen: 97.729 ng
 RT: 10.06 min Scan# 1152
 Delta R.T. -0.00 min
 Lab File: BG033641.D
 Acq: 6 Apr 2018 23:12




Instrument :
 BNA_G
 ClientSampleId :
 CV-RB26667RT


Tot Ion	82	Resp	351934
Ion	Ratio	Lower	Upper
82	100		
128	37.0	29.7	44.5
54	58.2	43.1	64.7

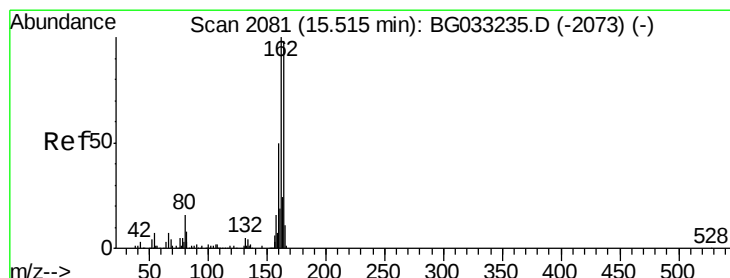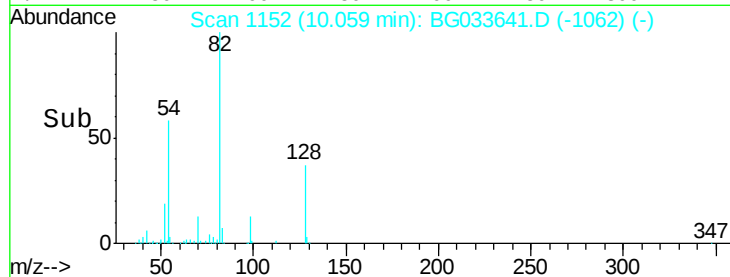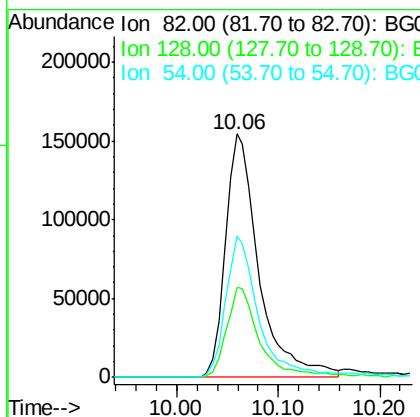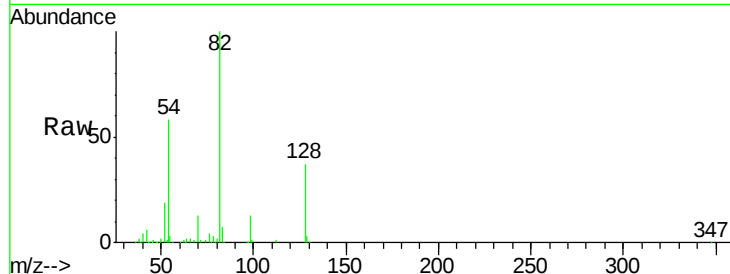

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.48 min Scan# 2074
 Delta R.T. -0.00 min
 Lab File: BG033641.D
 Acq: 6 Apr 2018 23:12

Tgt Ion	164	Resp	128571
Ion	Ratio	Lower	Upper
164	100		
162	103.1	78.8	118.2
160	48.0	35.4	53.0


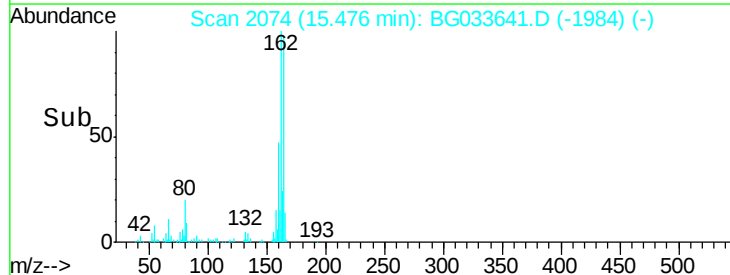
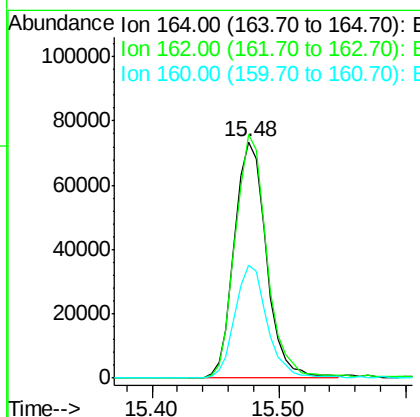
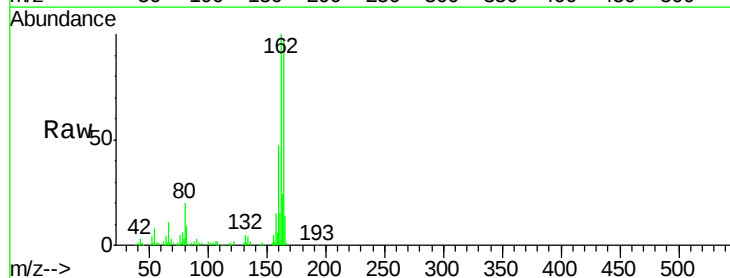


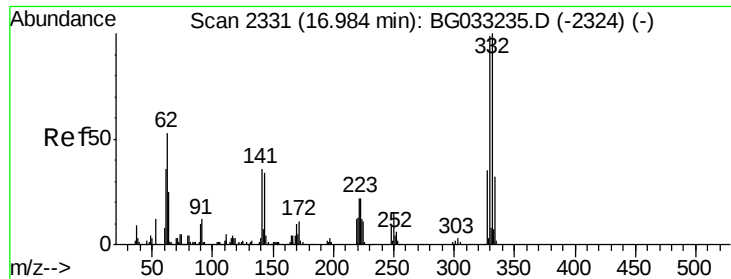

#41
 2,4,6-Tribromophenol
 Concen: 122.088 ng
 RT: 16.95 min Scan# 2325
 Delta R.T. -0.00 min
 Lab File: BG033641.D
 Acq: 6 Apr 2018 23:12




Instrument :
 BNA_G
 ClientSampleId :
 CV-RB26667RT


Tot Ion:330 Resp: 234766
 Ion Ratio Lower Upper
 330 100
 332 94.3 77.0 115.6
 141 38.3 25.2 37.8#

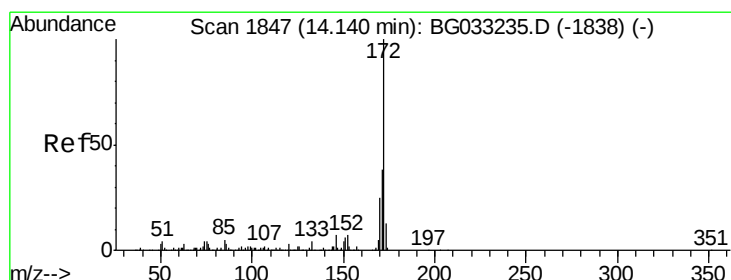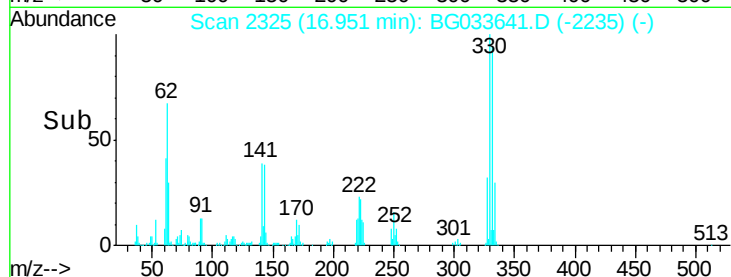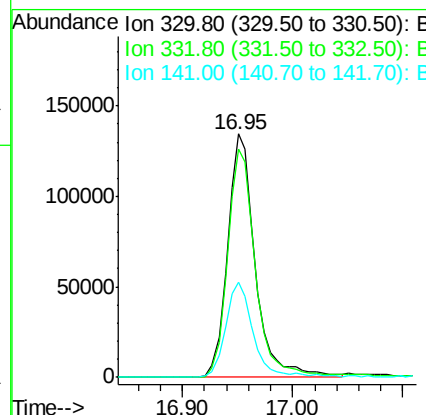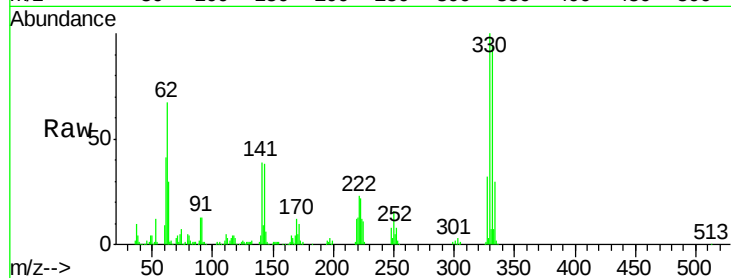

#44
 2-Fluorobiphenyl
 Concen: 99.921 ng
 RT: 14.11 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BG033641.D
 Acq: 6 Apr 2018 23:12

Tgt Ion:172 Resp: 889906
 Ion Ratio Lower Upper
 172 100
 171 37.4 30.0 45.0
 170 25.7 19.5 29.3


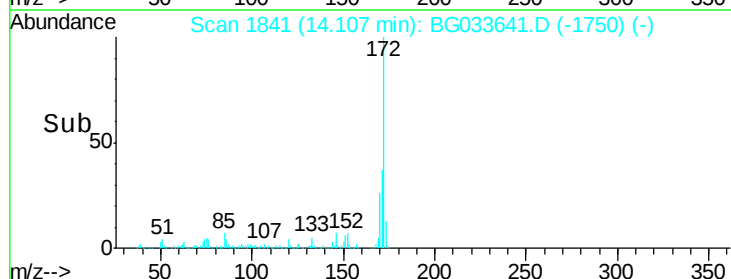
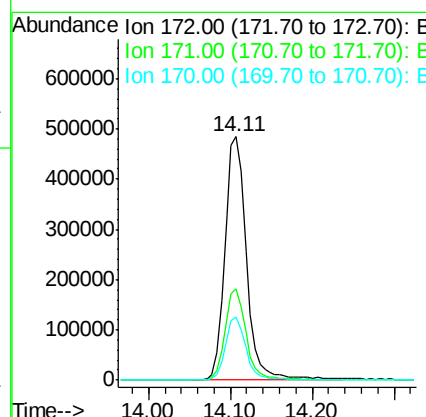
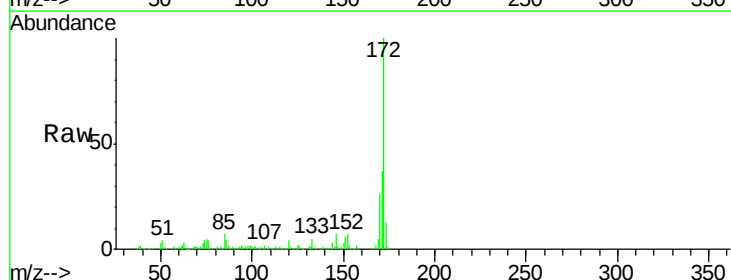


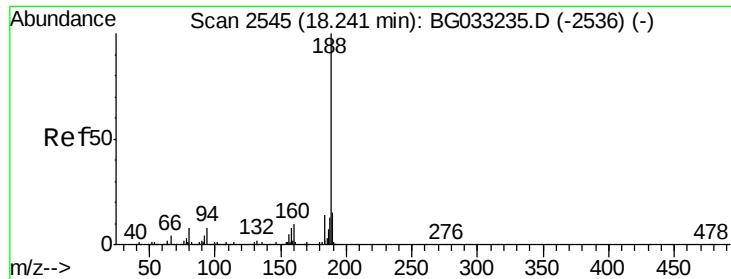

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.21 min Scan# 2539
Delta R.T. -0.00 min
Lab File: BG033641.D
Acq: 6 Apr 2018 23:12




Instrument :
BNA_G
ClientSampleId :
CV-RB26667RT


Tot Ion:188 Resp: 310572
Ion Ratio Lower Upper
188 100
94 7.5 6.9 10.3
80 9.3 7.7 11.5

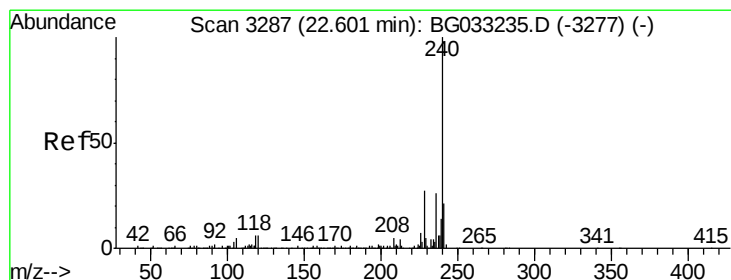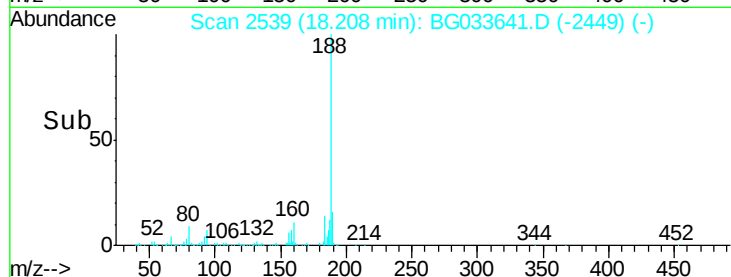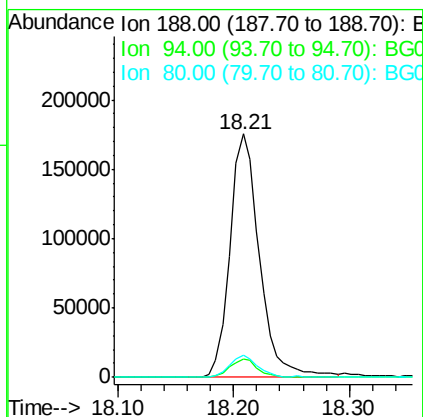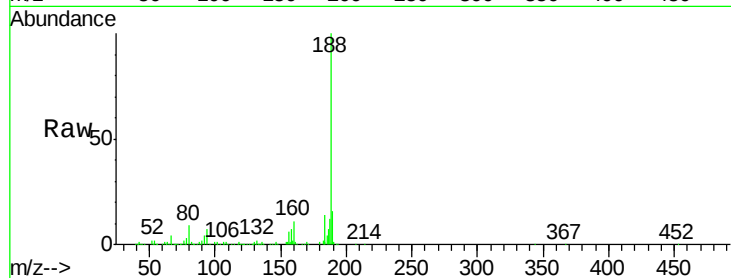

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.56 min Scan# 3279
Delta R.T. -0.00 min
Lab File: BG033641.D
Acq: 6 Apr 2018 23:12

Tgt Ion:240 Resp: 313381
Ion Ratio Lower Upper
240 100
120 8.2 6.8 10.2
236 27.0 20.9 31.3

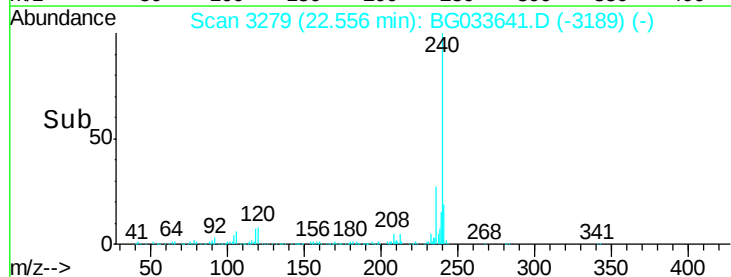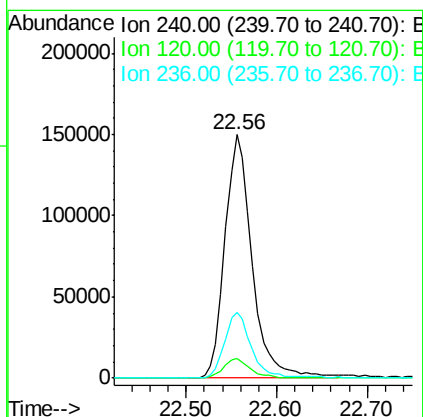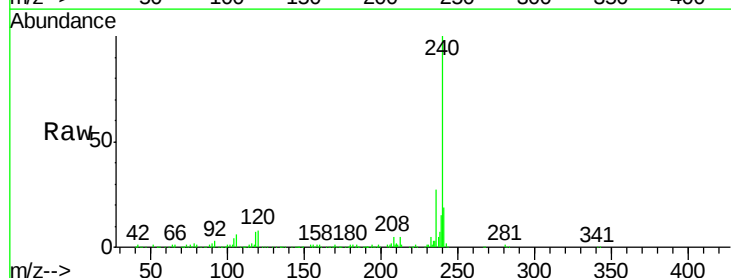

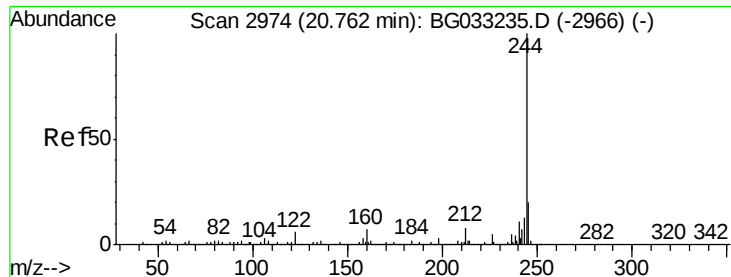

#78

Terphenyl-d14

Concen: 102.658 ng

RT: 20.73 min Scan# 2968

Delta R.T. 0.00 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12

Instrument :

BNA_G

ClientSampled :

CV-RB26667RT


Tot Ion:244 Resp: 1504298

Ion Ratio Lower Upper

244 100

212 9.0 5.8 8.8#



122 8.2 7.0 10.4

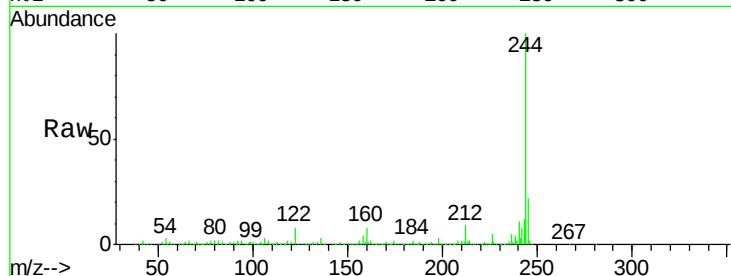

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

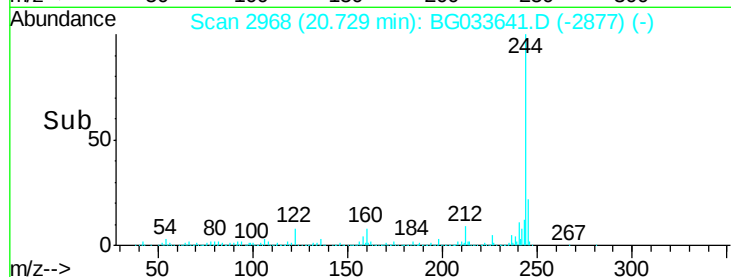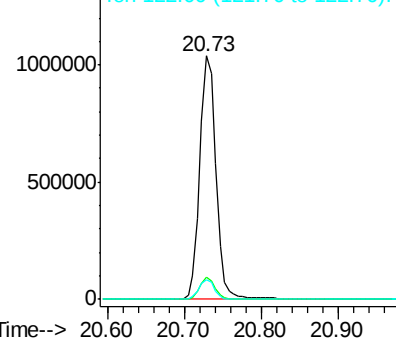

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.33 min Scan# 3921

Delta R.T. 0.01 min

Lab File: BG033641.D

Acq: 6 Apr 2018 23:12


Tgt Ion:264 Resp: 289644

Ion Ratio Lower Upper

264 100

260 24.4 17.4 26.0

265 23.9 17.7 26.5

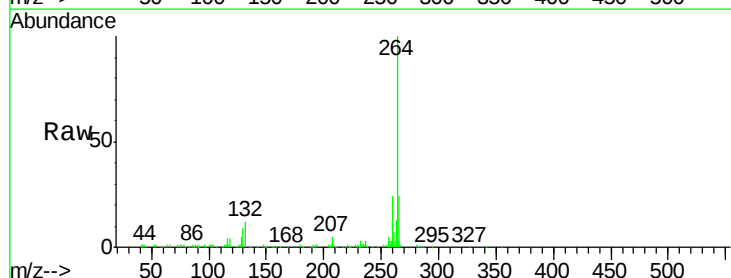

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

