


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
 Data File : BG033628.D
 Acq On : 6 Apr 2018 14:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 05 17:36:07 2018

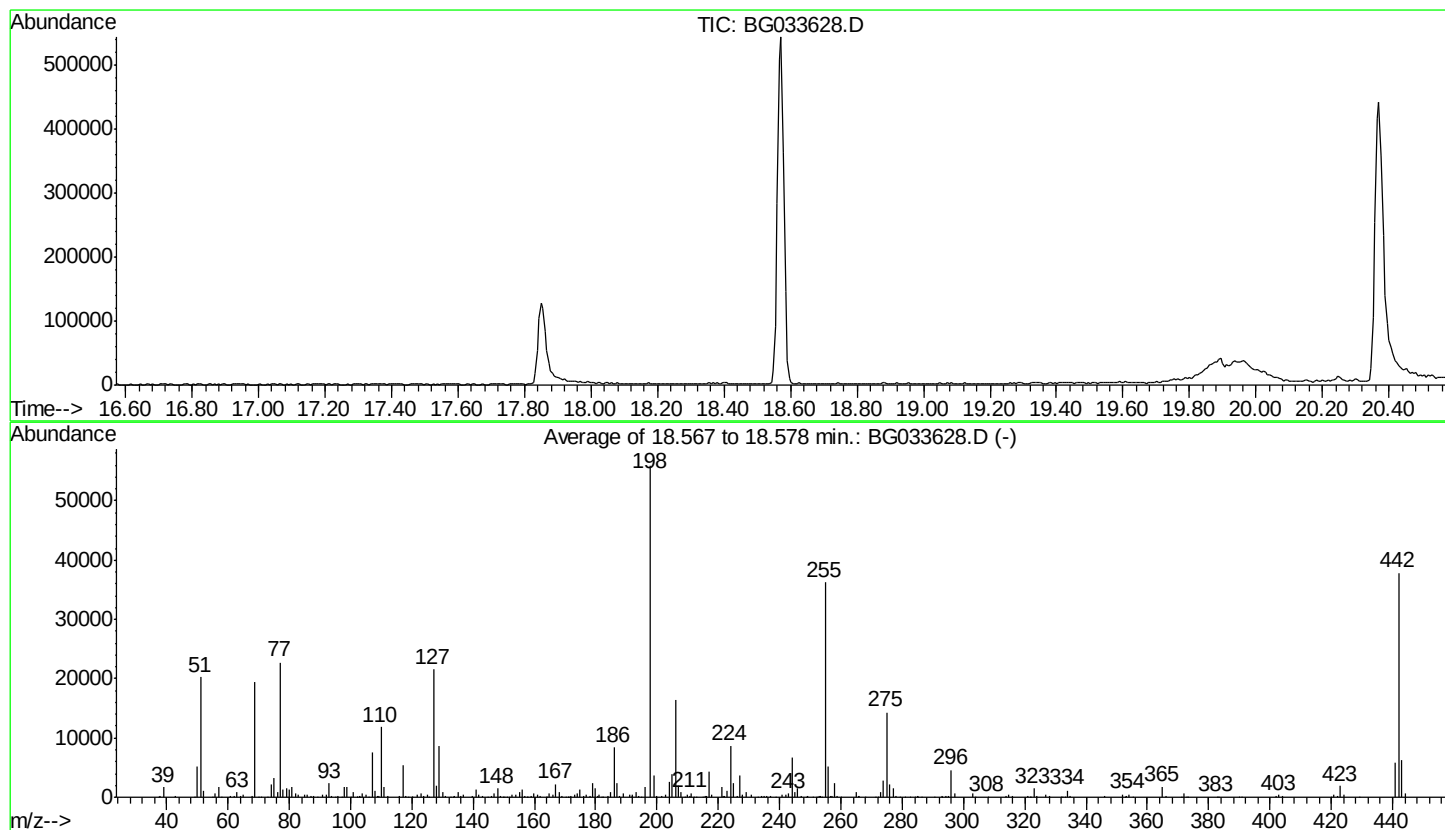

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	20253	PASS
68	69	0.00	2	0.9	176	PASS
69	198	0.00	100	34.8	19473	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	38.6	21591	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55941	PASS
199	198	5	9	6.5	3658	PASS
275	198	10	60	25.5	14281	PASS
365	198	1	100	3.2	1815	PASS
441	443	0.01	100	92.7	5802	PASS
442	198	50	100	67.7	37858	PASS
443	442	15	24	16.5	6261	PASS