


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040618\
 Data File : BG033665.D
 Acq On : 7 Apr 2018 15:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 05 17:36:07 2018

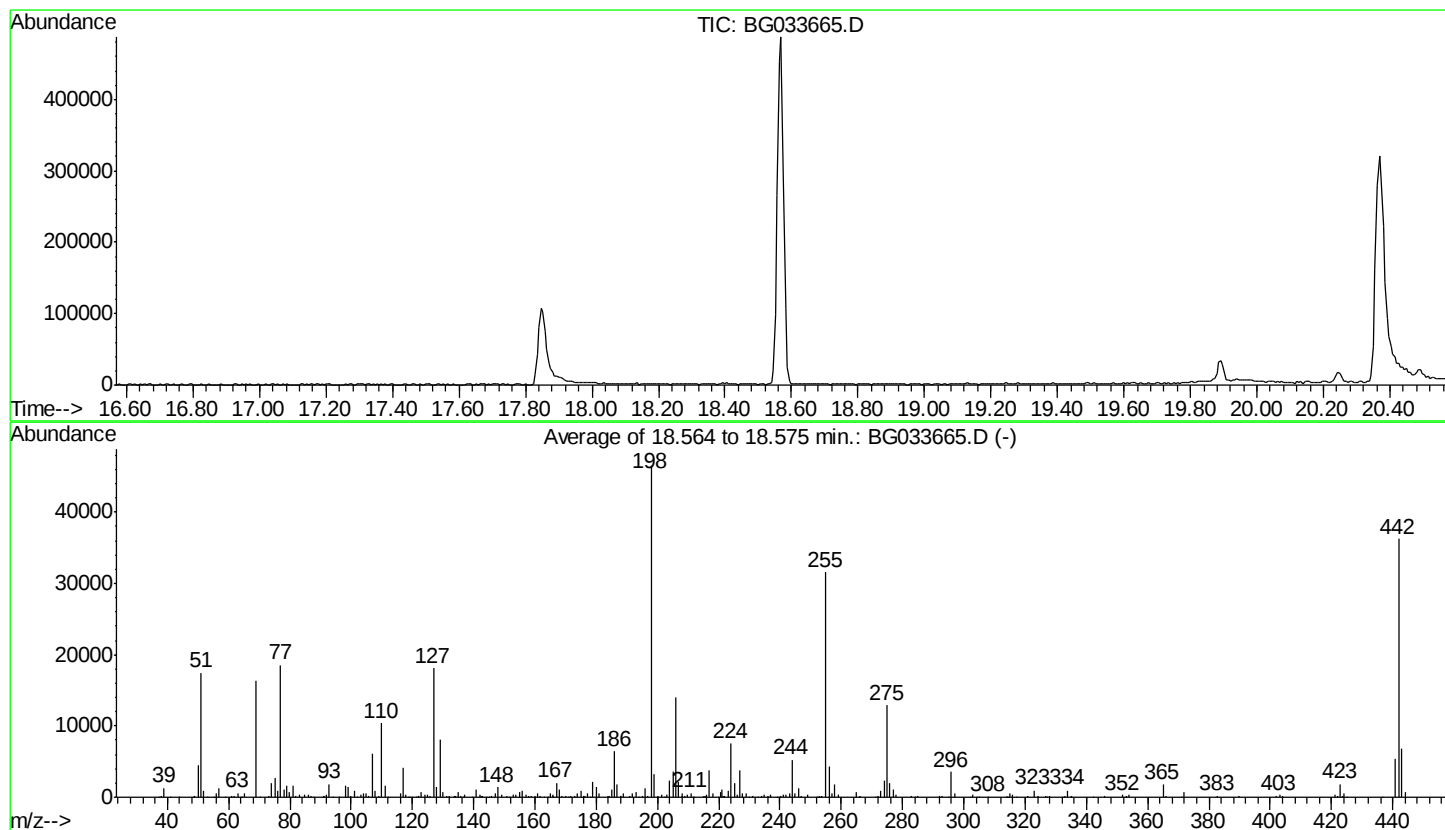

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	17474	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	16421	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	39.0	18129	PASS
197	198	0.00	2	0.5	230	PASS
198	198	100	100	100.0	46533	PASS
199	198	5	9	6.8	3150	PASS
275	198	10	60	27.6	12857	PASS
365	198	1	100	3.8	1791	PASS
441	443	0.01	100	78.3	5318	PASS
442	198	50	100	78.0	36277	PASS
443	442	15	24	18.7	6794	PASS