
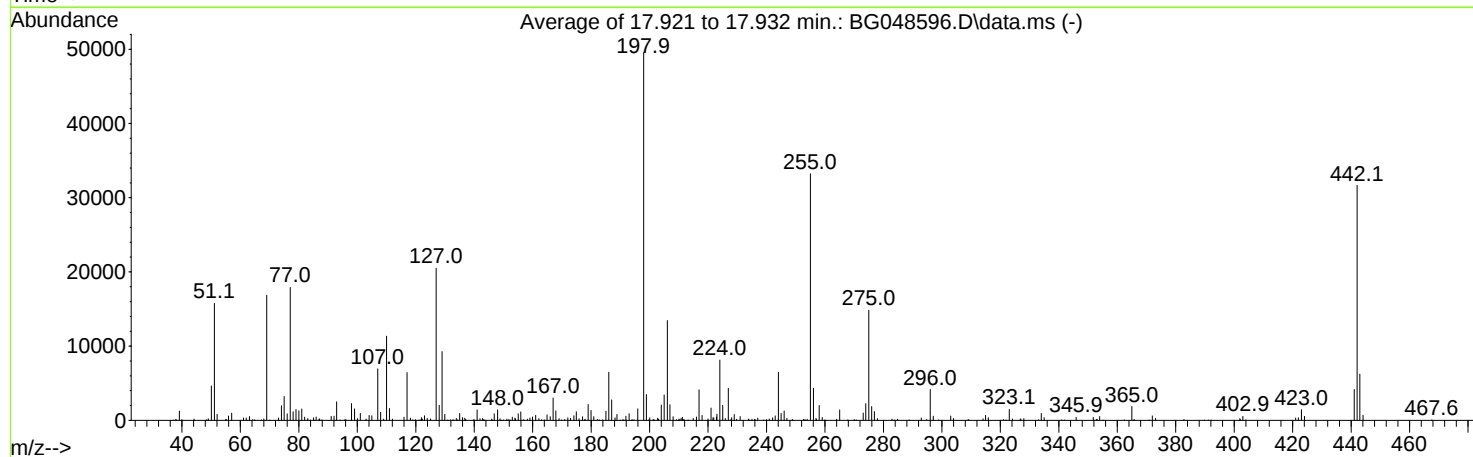


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040621\
 Data File : BG048596.D
 Acq On : 6 Apr 2021 9:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 10:20:56 2021

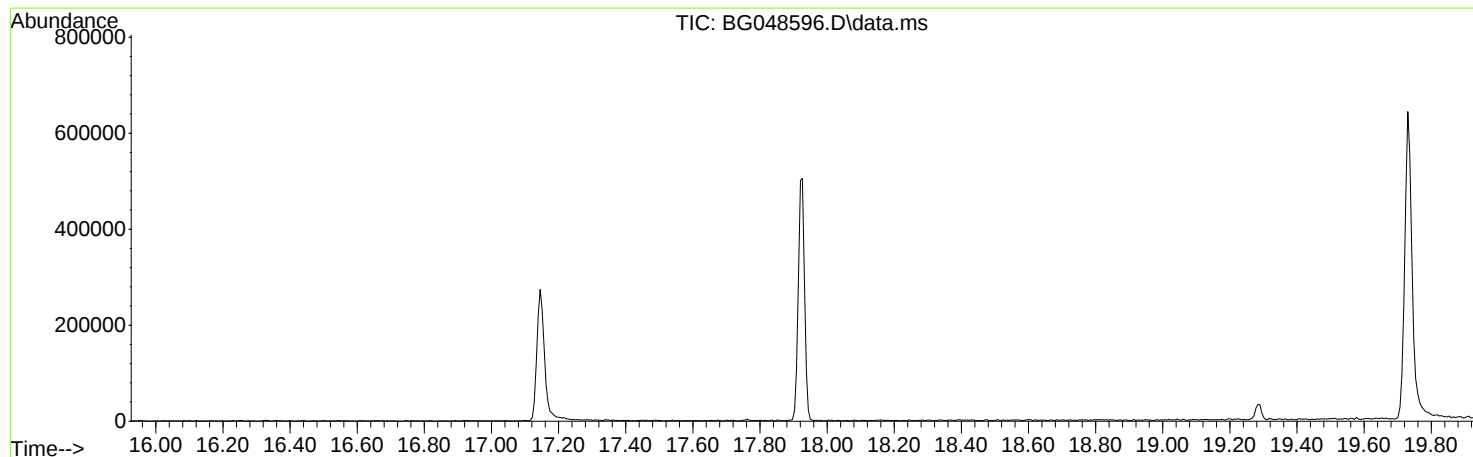

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	15768	PASS
68	69	0.00	2	1.1	186	PASS
69	198	0.00	100	34.0	16862	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	41.4	20504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49560	PASS
199	198	5	9	7.0	3481	PASS
275	198	10	60	29.9	14823	PASS
365	198	1	100	3.8	1866	PASS
441	198	0.01	100	8.4	4162	PASS
442	198	50	100	63.9	31667	PASS
443	442	15	24	19.7	6238	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2021	BNA_G	<u>BG048596.D</u>
Compound Name	Response	Retention Time
DDT	199631	20.97
DDD	3455	20.52
DDE	378	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3833	203464	1.88

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040621\
Data File : BG048596.D
Acq On : 6 Apr 2021 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:57:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 10:20:56 2021
Response via : Initial Calibration

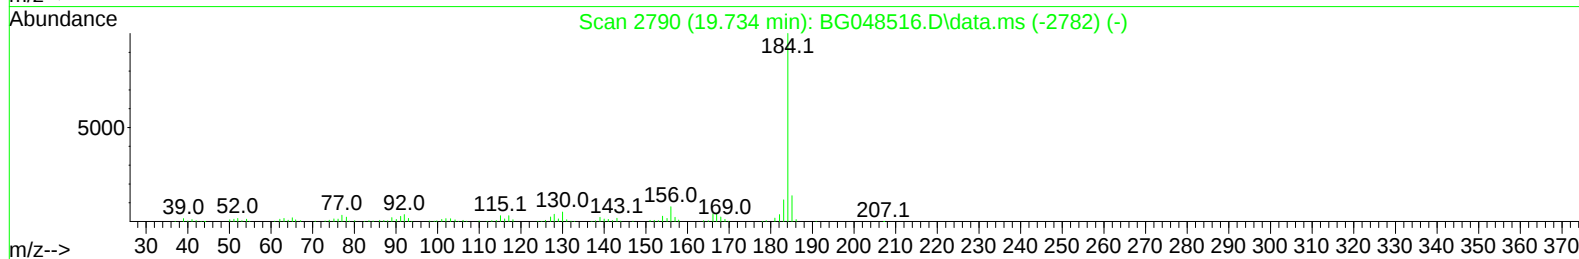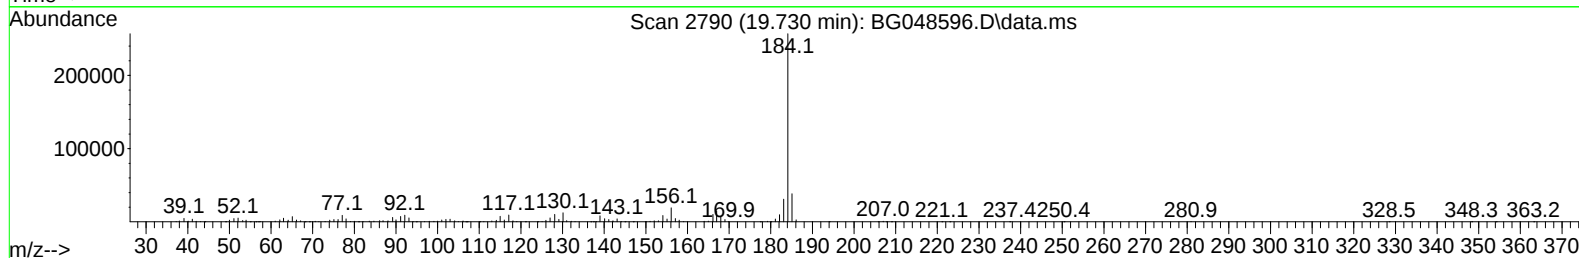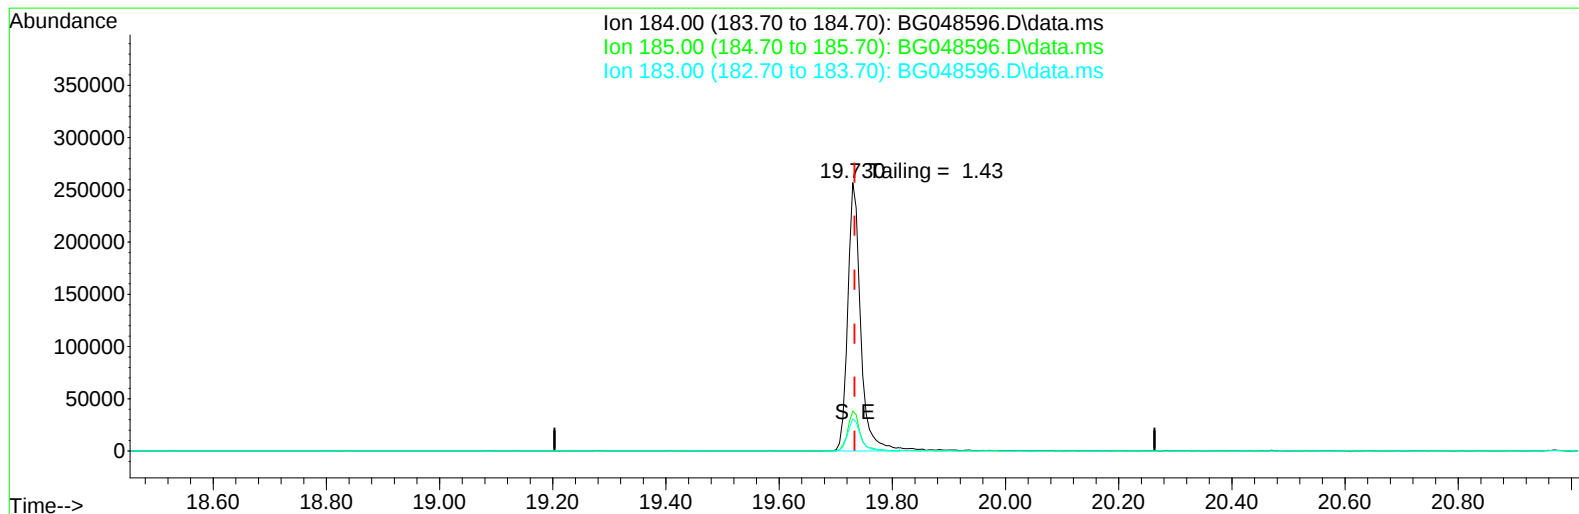

TIC: BG048596.D\data.ms

(77) Benzidine

19.730min (-0.003) 167801.47 ng

response 409123

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.91
183.00	11.50	12.05
0.00	0.00	0.00

