
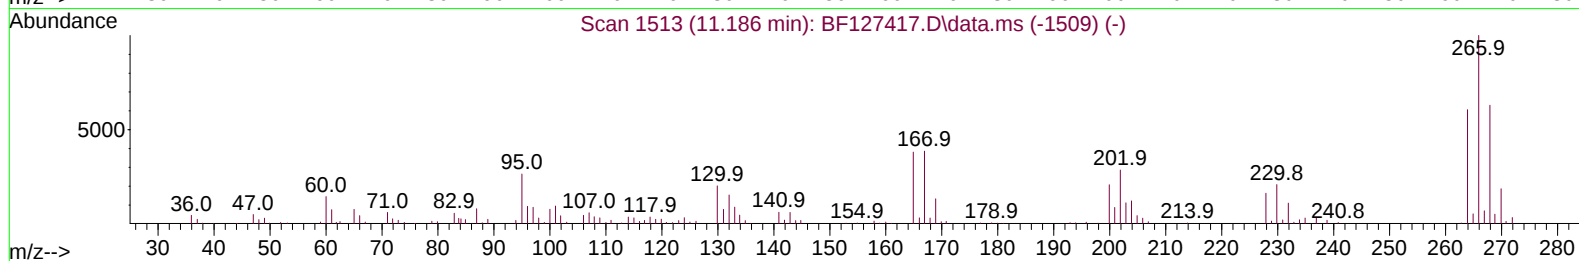
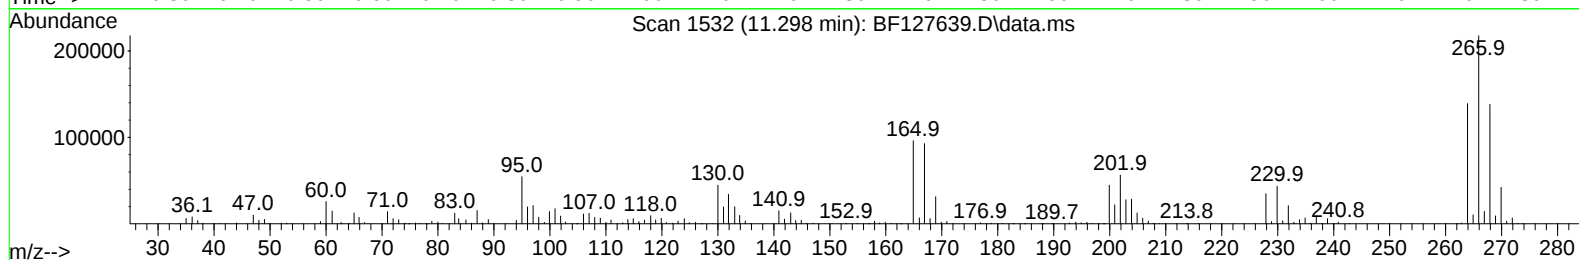


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127639.D
Acq On : 06 Apr 2022 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 13:06:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:06:44 2022
Response via : Initial Calibration

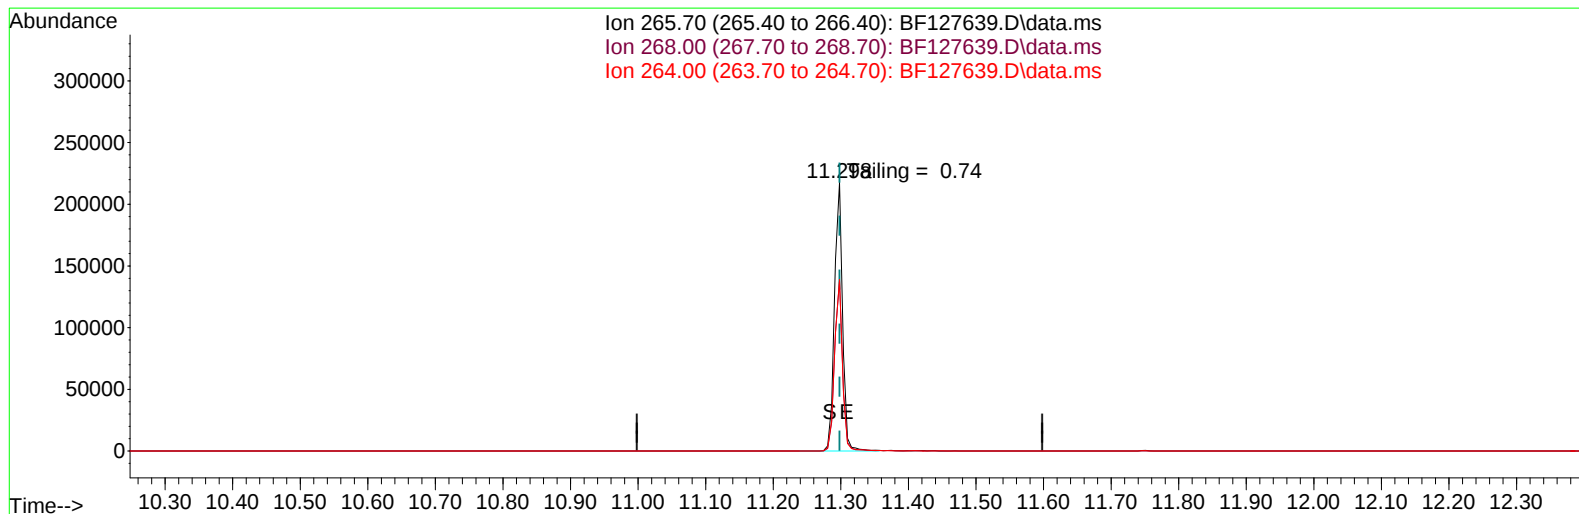

TIC: BF127639.D\data.ms

(70) Pentachlorophenol (C)

11.298min (0.000) 377428.56 ng

response 182284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	60.60	63.93
0.00	0.00	0.00