
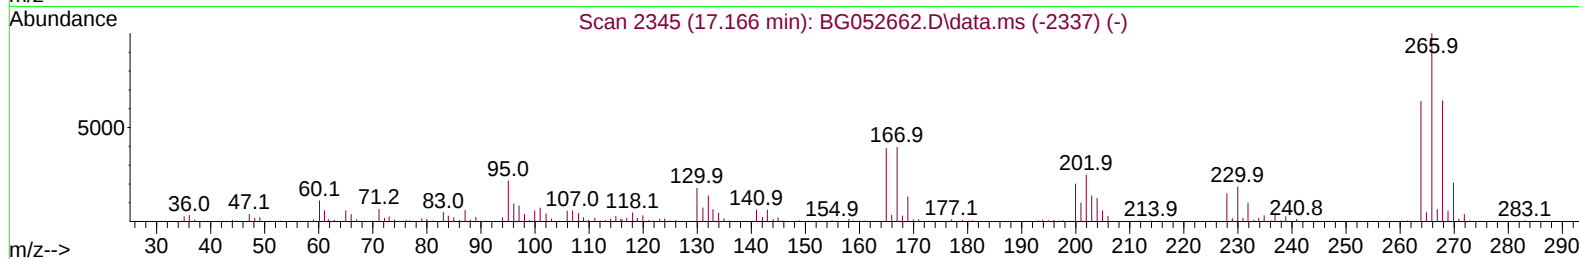
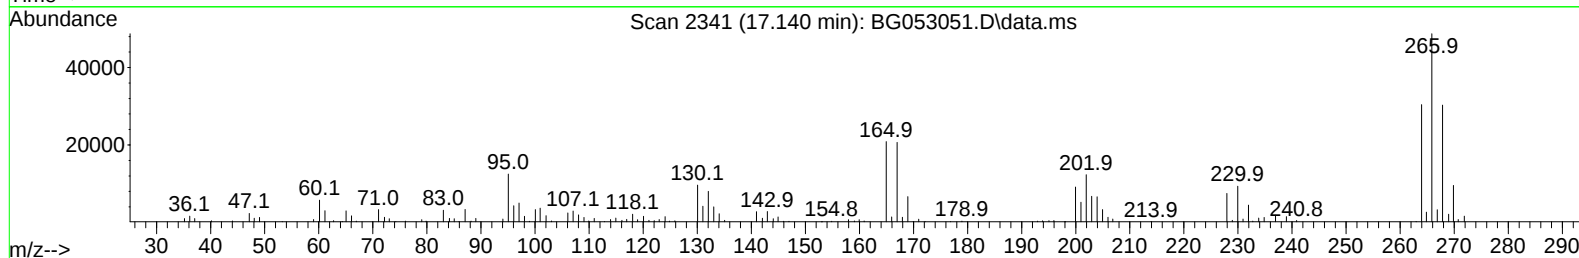


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040622\
Data File : BG053051.D
Acq On : 6 Apr 2022 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 14:43:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 14:35:39 2022
Response via : Initial Calibration

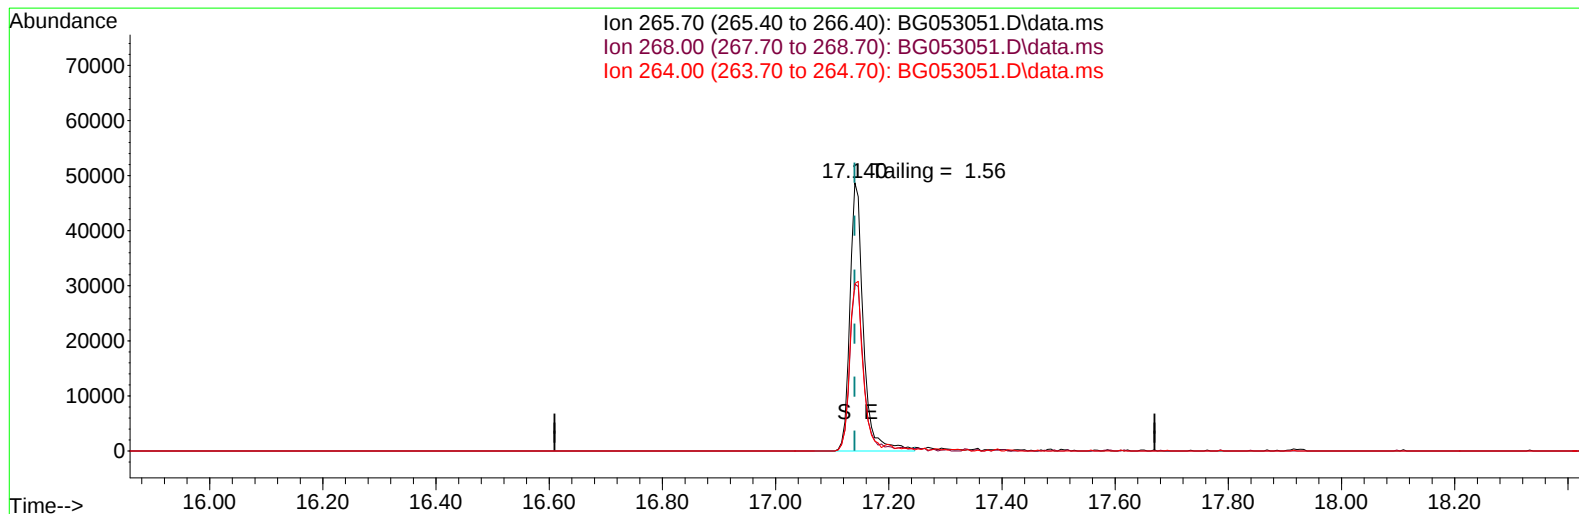

TIC: BG053051.D\data.ms

(70) Pentachlorophenol (C)




17.140min (+ 0.001) 155303.20 ng

response 81157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.19
264.00	56.60	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040622\
Data File : BG053051.D
Acq On : 6 Apr 2022 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 14:43:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 14:35:39 2022
Response via : Initial Calibration

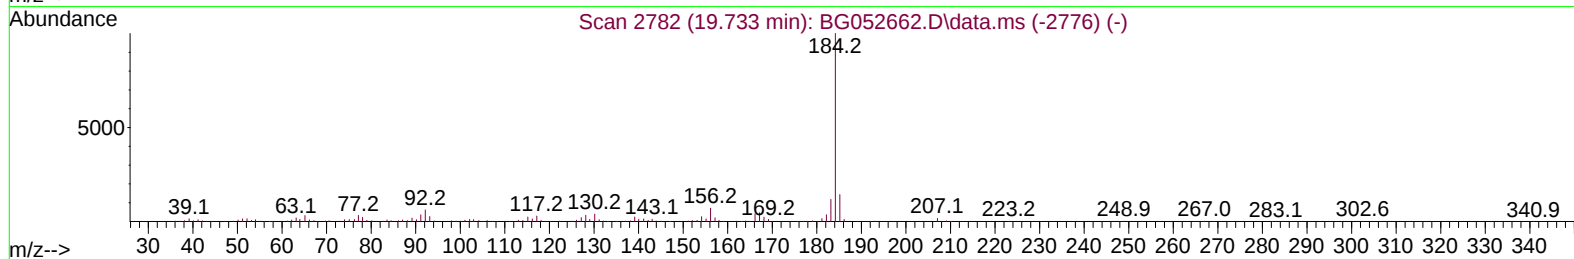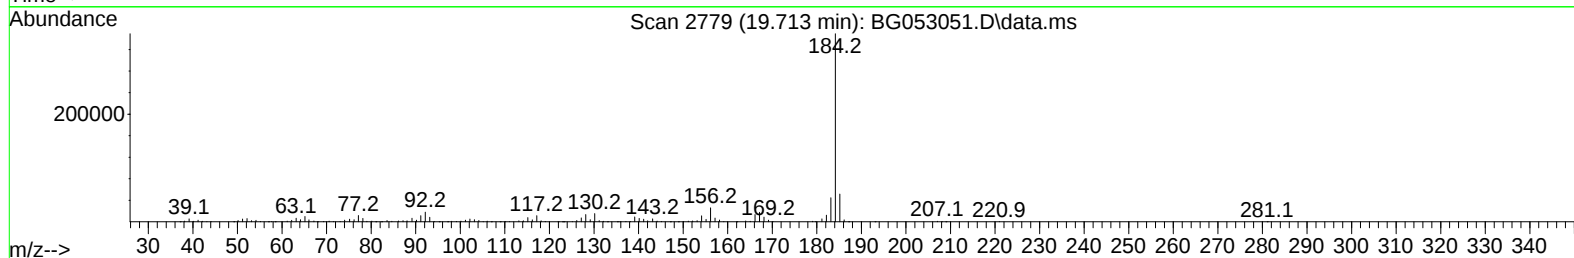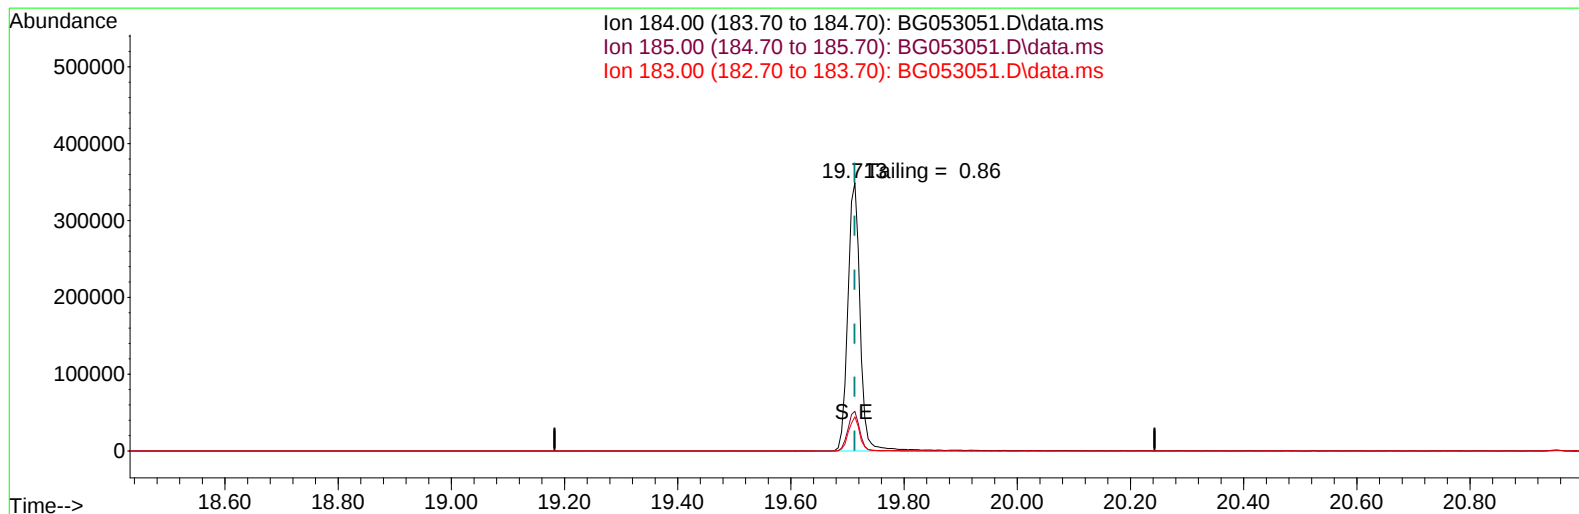

TIC: BG053051.D\data.ms

(77) Benzidine**19.713min (+ 0.001) 69801.02 ng****response 525690**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.79
183.00	11.80	12.79
0.00	0.00	0.00