
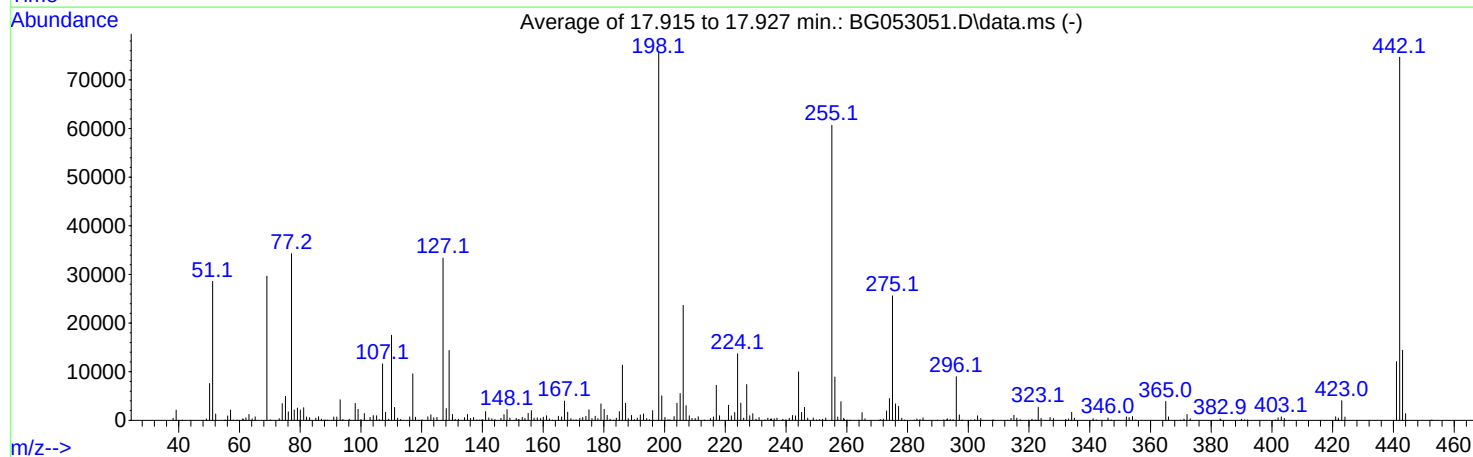


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040622\
 Data File : BG053051.D
 Acq On : 6 Apr 2022 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 14:35:39 2022

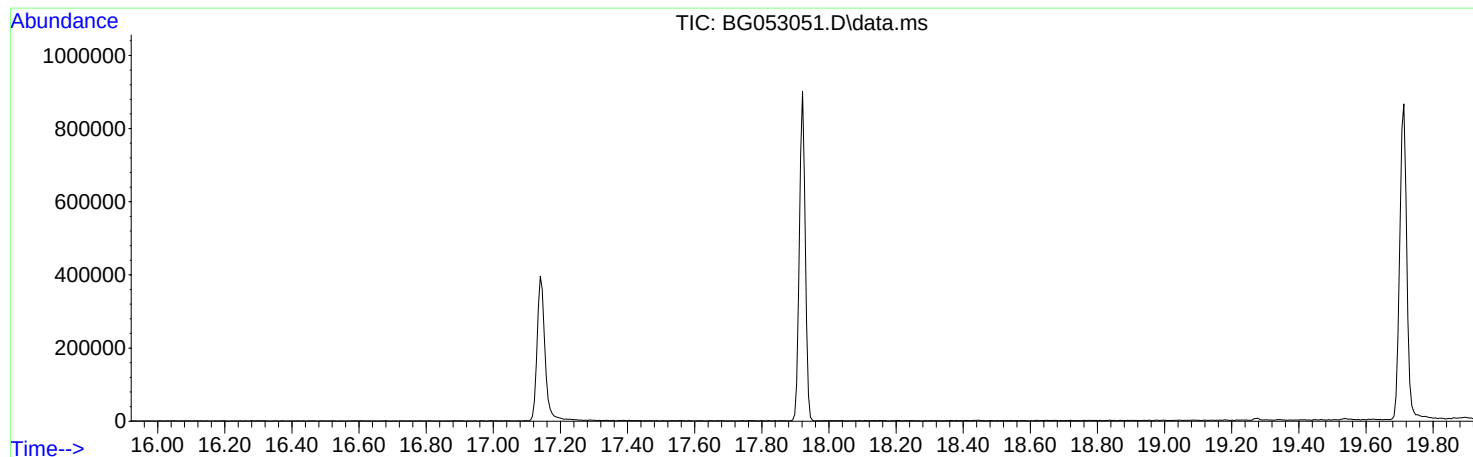




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	28576	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.2	29675	PASS
70	69	0.00	2	0.4	114	PASS
127	198	10	80	44.1	33357	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75640	PASS
199	198	5	9	6.6	5027	PASS
275	198	10	60	33.8	25597	PASS
365	198	1	100	5.1	3868	PASS
441	198	0.01	100	16.0	12081	PASS
442	442	50	100	100.0	74675	PASS
443	442	15	24	19.3	14417	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040622\
Data File : BG053051.D
Acq On : 6 Apr 2022 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 14:43:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 14:35:39 2022
Response via : Initial Calibration

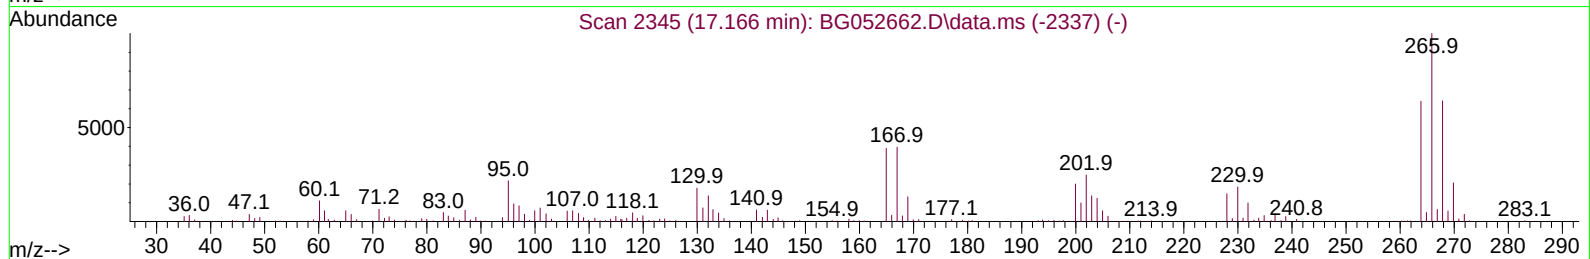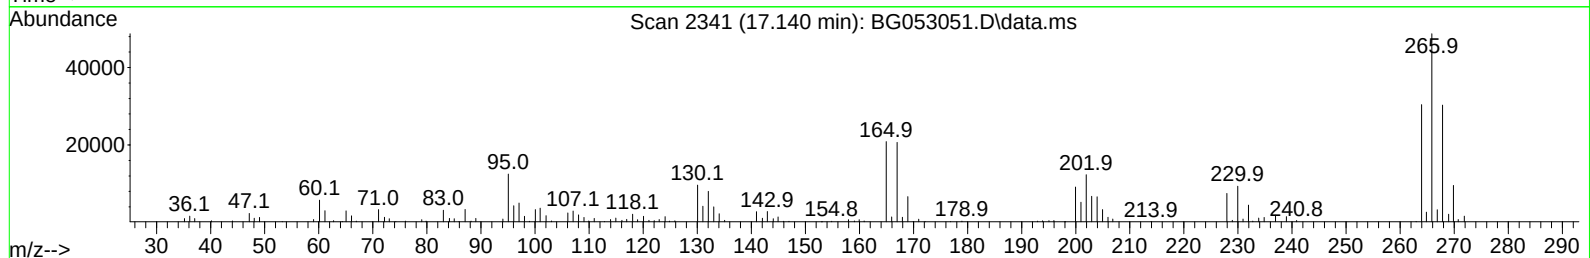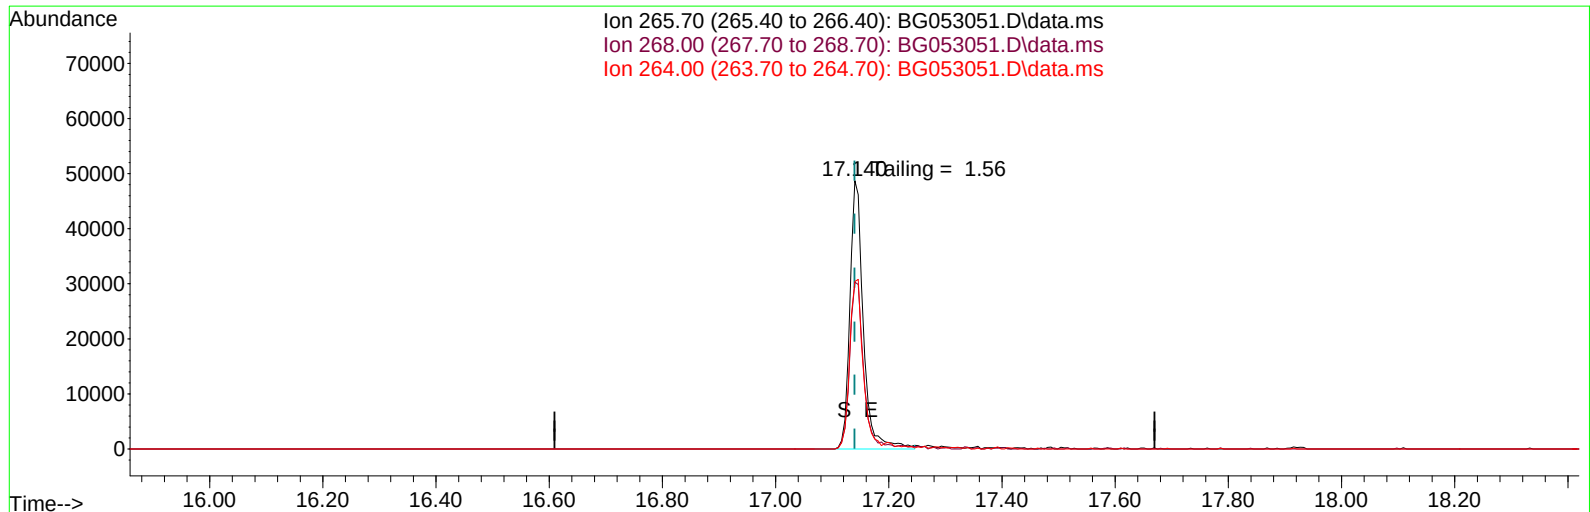

TIC: BG053051.D\data.ms

(70) Pentachlorophenol (C)

17.140min (+ 0.001) 155303.20 ng




response 81157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.19
264.00	56.60	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040622\
Data File : BG053051.D
Acq On : 6 Apr 2022 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 14:43:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 14:35:39 2022
Response via : Initial Calibration

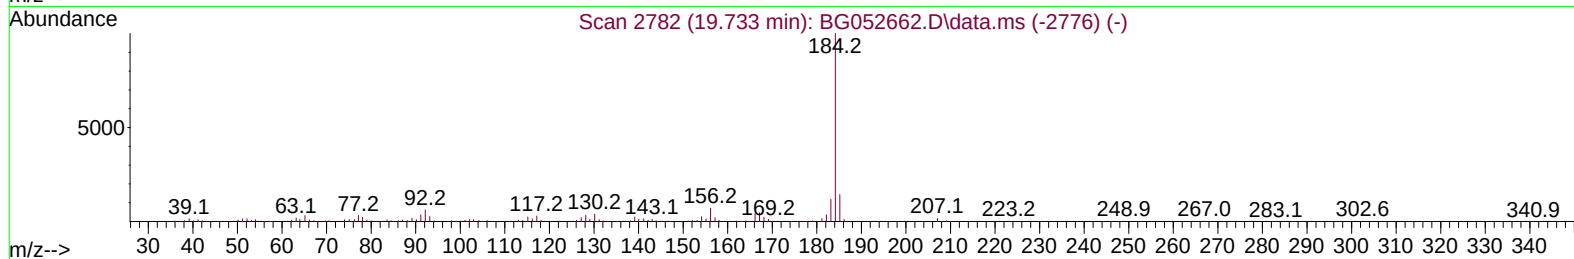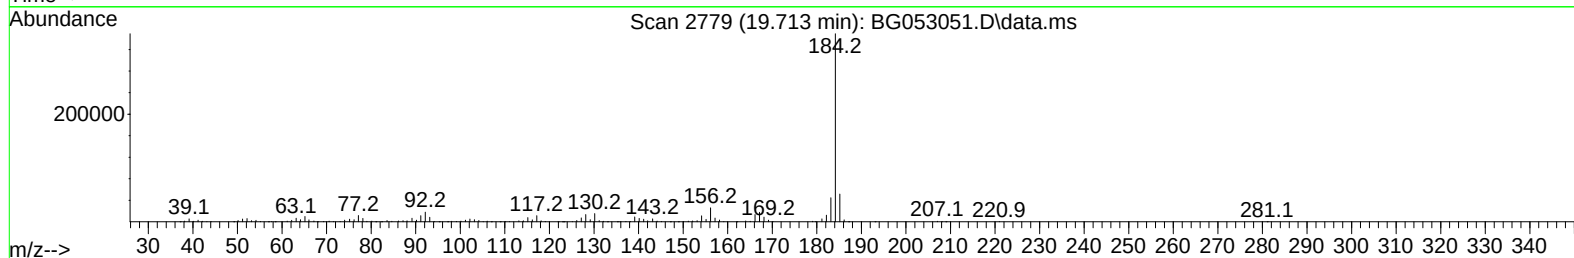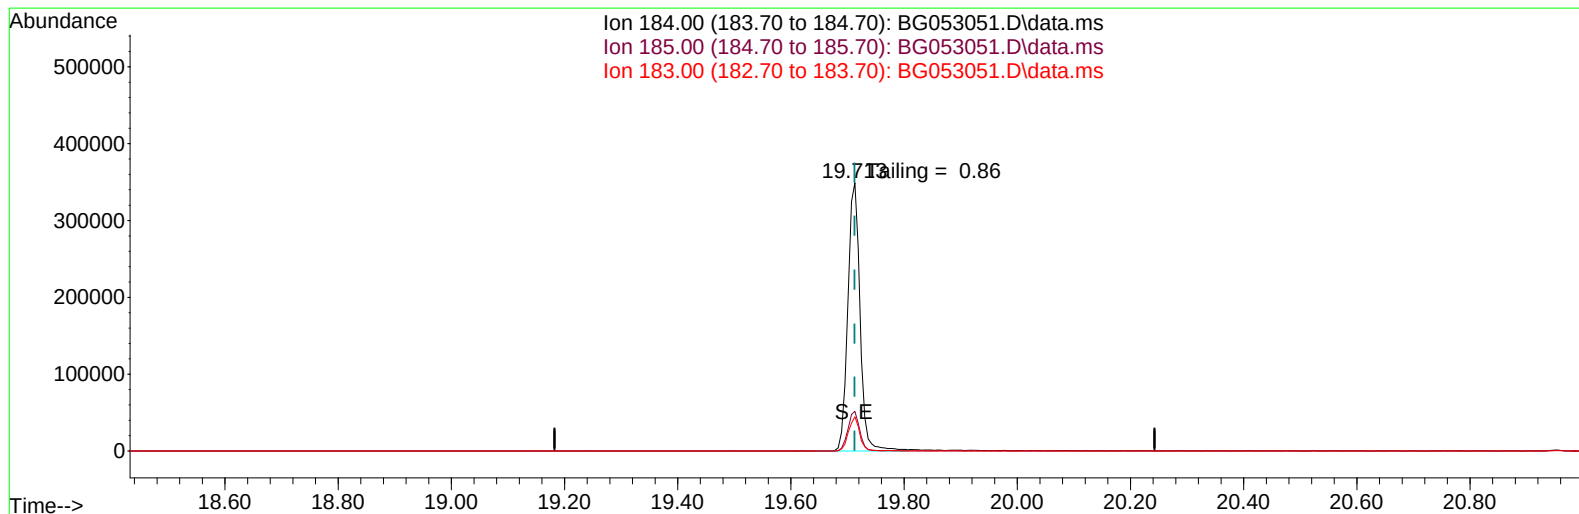

TIC: BG053051.D\data.ms

(77) Benzidine

19.713min (+ 0.001) 69801.02 ng

response 525690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.79
183.00	11.80	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2022	BNA_G	<u>BG053051.D</u>
Compound Name	Response	Retention Time
DDT	267451	20.95
DDD	7335	20.5
DDE	525	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7860	275311	2.85

Instrument :
BNA_G
ClientSampleId :
DFTPP