
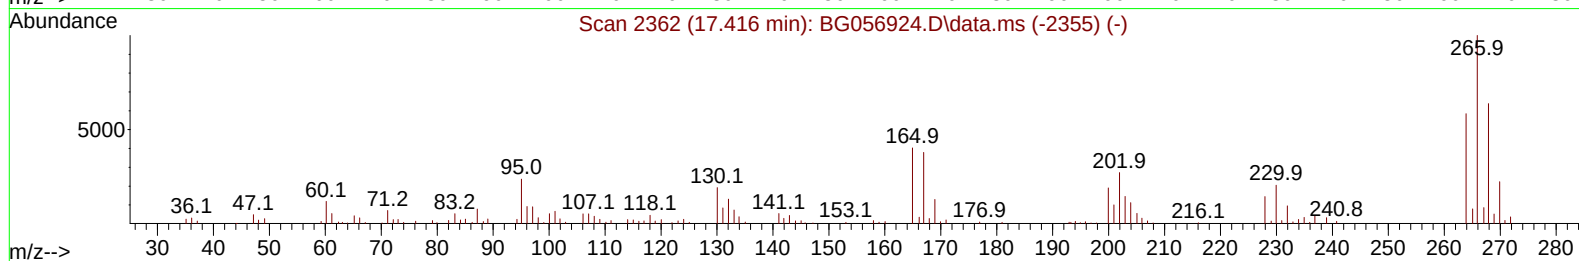
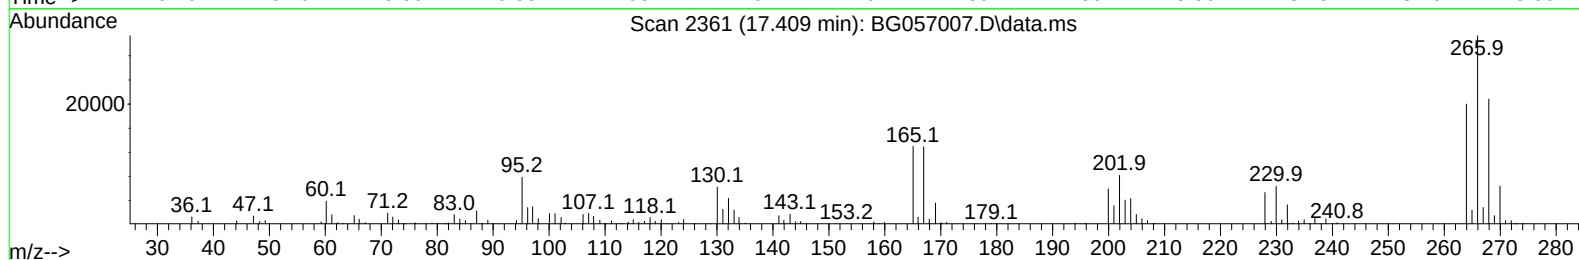


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040623\
Data File : BG057007.D
Acq On : 6 Apr 2023 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:07:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 01:33:41 2023
Response via : Initial Calibration

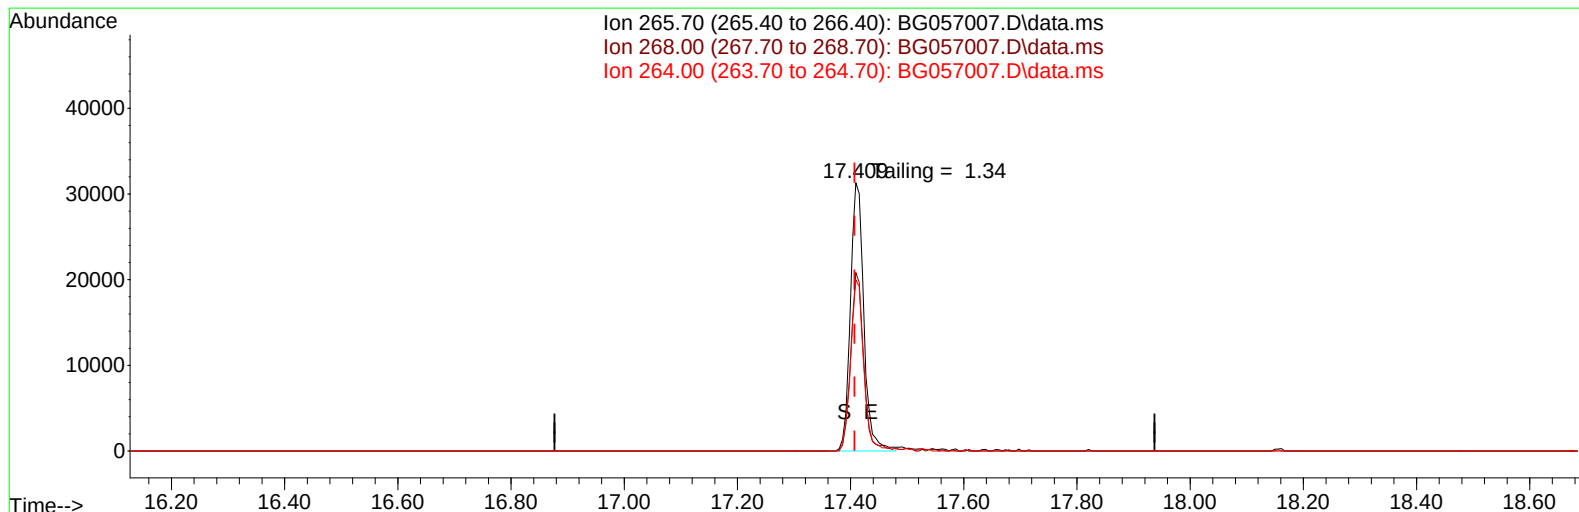

TIC: BG057007.D\data.ms

(70) Pentachlorophenol (C)




17.409min (+ 0.003) 103276.02 ng

response 51662

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	66.47
264.00	58.50	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040623\
Data File : BG057007.D
Acq On : 6 Apr 2023 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:07:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 01:33:41 2023
Response via : Initial Calibration

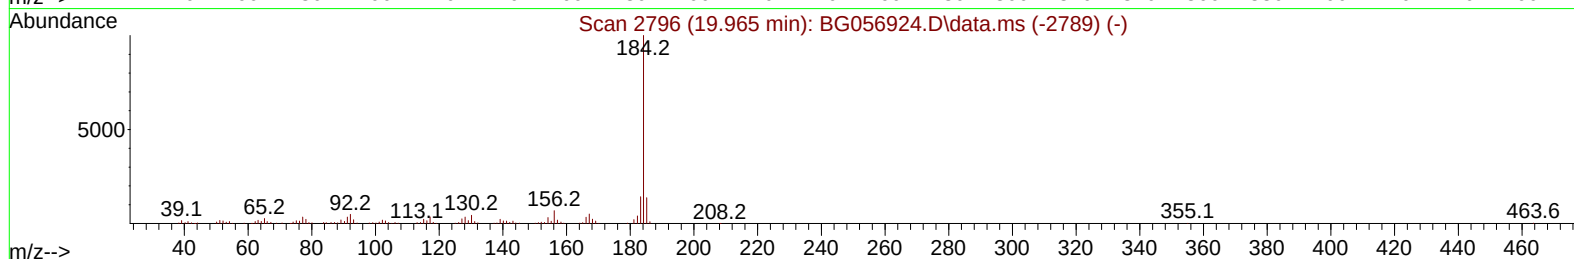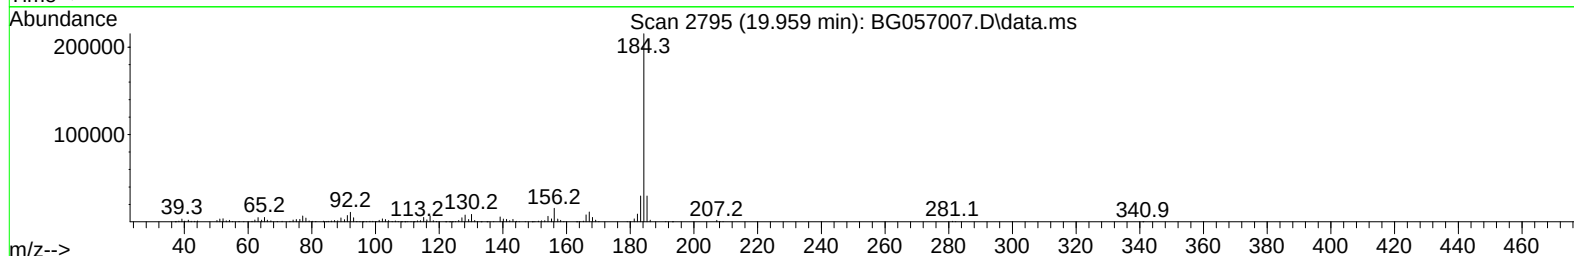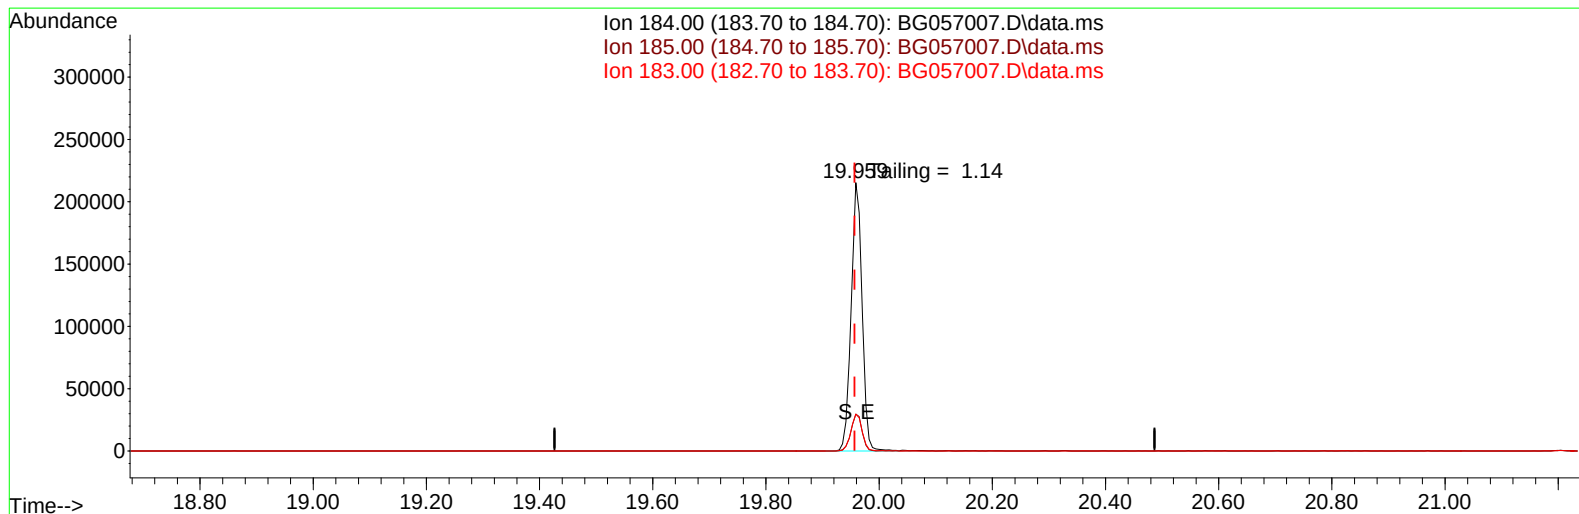

TIC: BG057007.D\data.ms

(77) Benzidine**19.959min (+ 0.003) 31160.81 ng****response 289587**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.80
183.00	14.20	13.76
0.00	0.00	0.00