


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040623\
Data File : BG057007.D
Acq On : 6 Apr 2023 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 07 01:33:41 2023

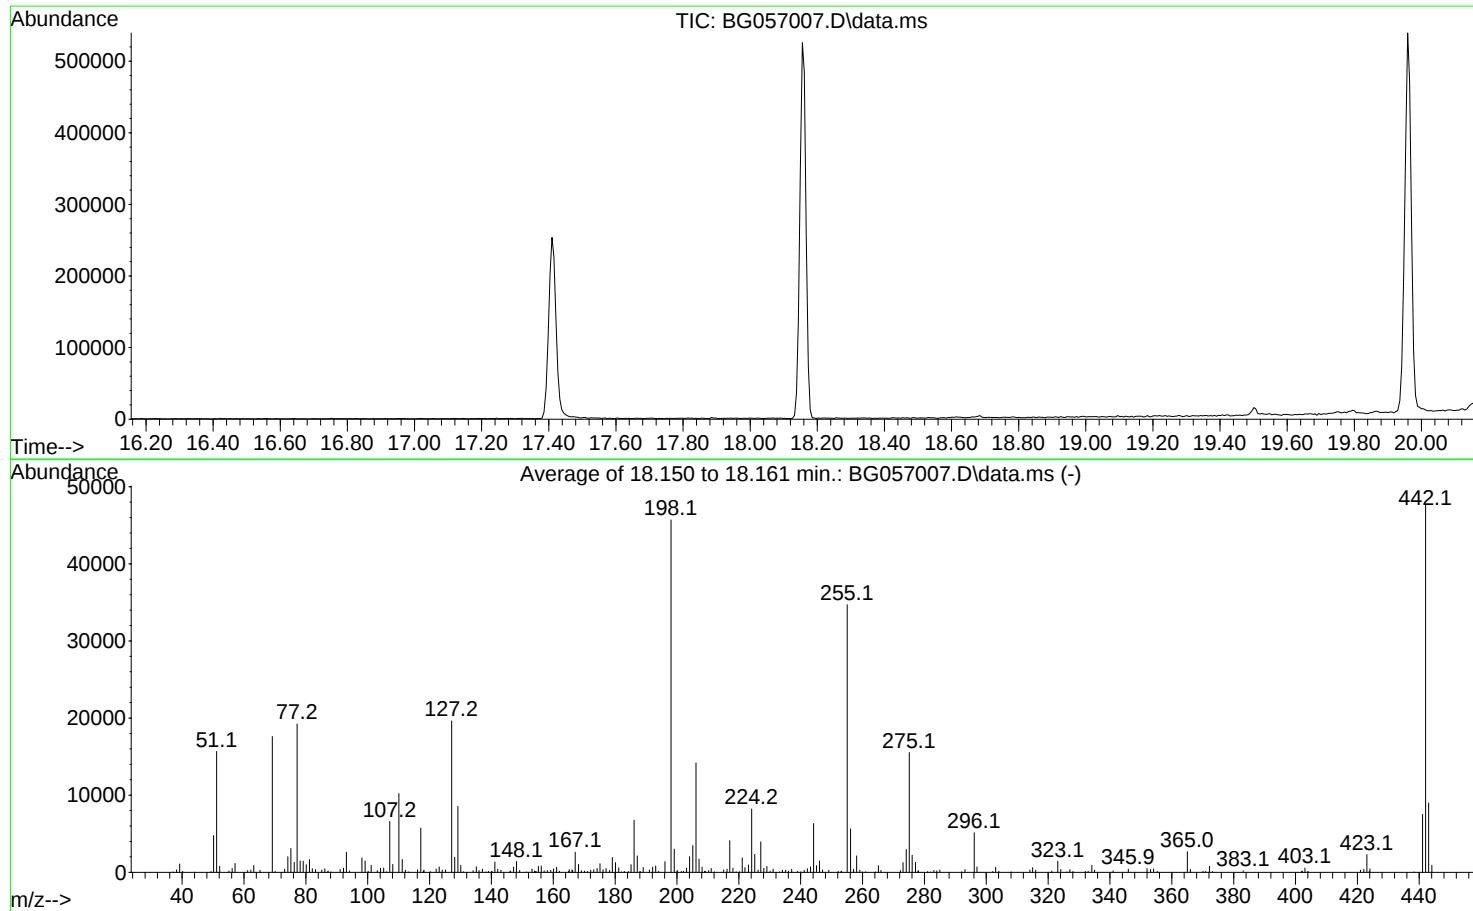




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	15674	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.5	17611	PASS
70	69	0.00	2	0.6	106	PASS
127	198	10	80	42.9	19611	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45696	PASS
199	198	5	9	6.6	3006	PASS
275	198	10	60	34.0	15535	PASS
365	198	1	100	5.8	2658	PASS
441	198	0.01	100	16.4	7500	PASS
442	442	50	100	100.0	47704	PASS
443	442	15	24	18.9	8995	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040623\
 Data File : BG057007.D
 Acq On : 6 Apr 2023 10:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 04:07:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 07 01:33:41 2023
 Response via : Initial Calibration

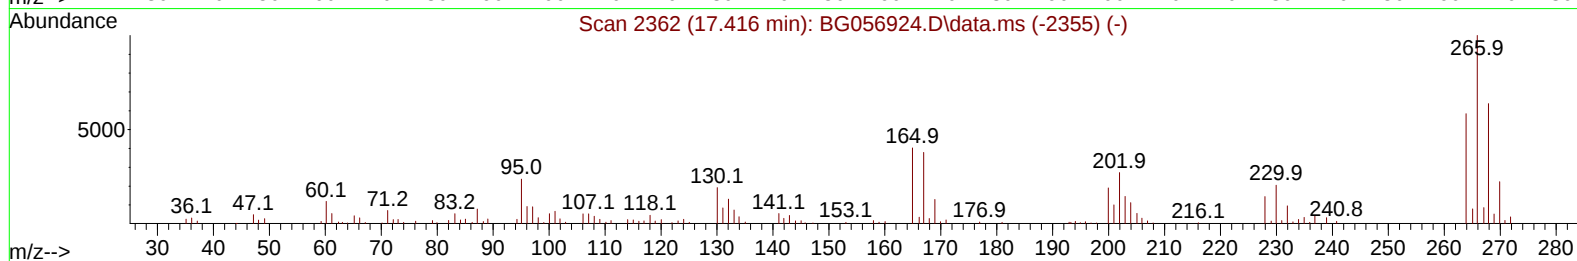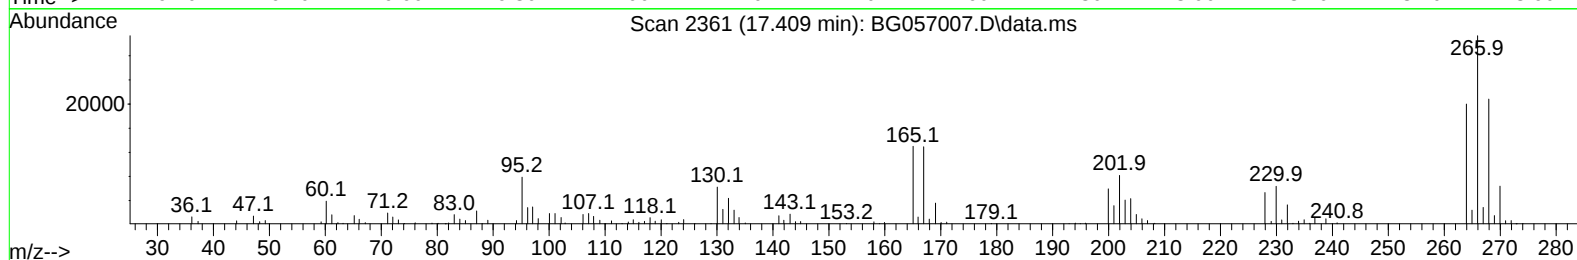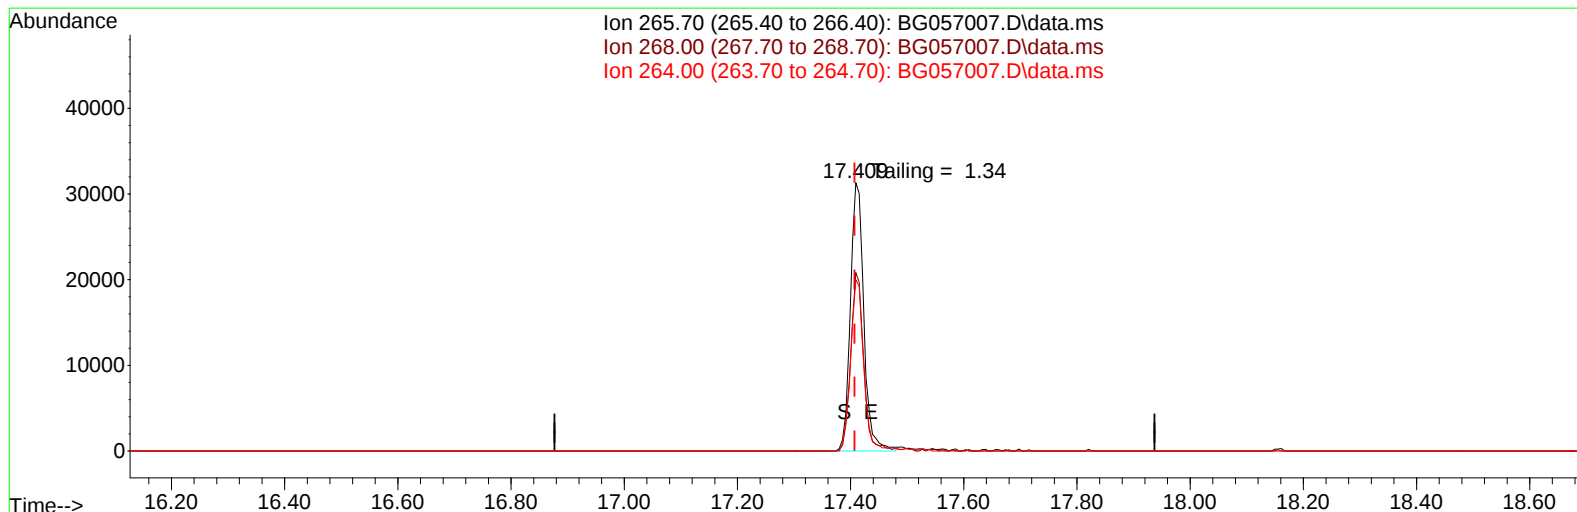

TIC: BG057007.D\data.ms

(70) Pentachlorophenol (C)

17.409min (+ 0.003) 103276.02 ng




response 51662

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	66.47
264.00	58.50	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040623\
Data File : BG057007.D
Acq On : 6 Apr 2023 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 07 04:07:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 07 01:33:41 2023
Response via : Initial Calibration

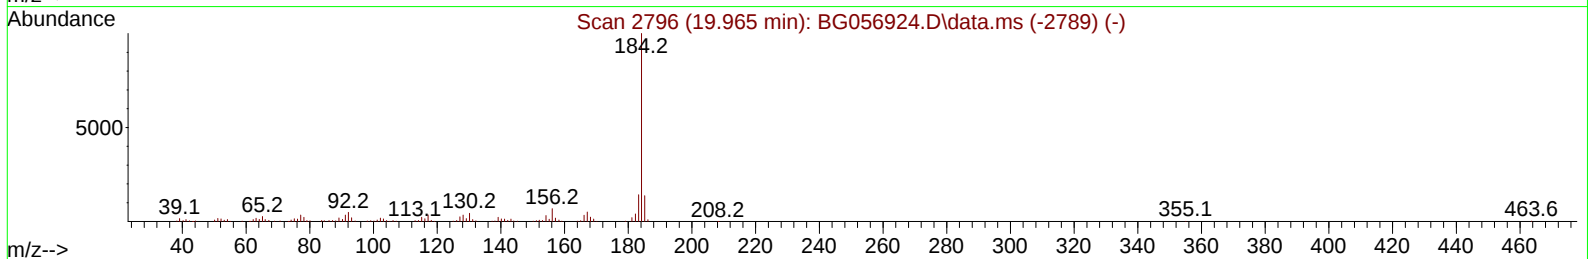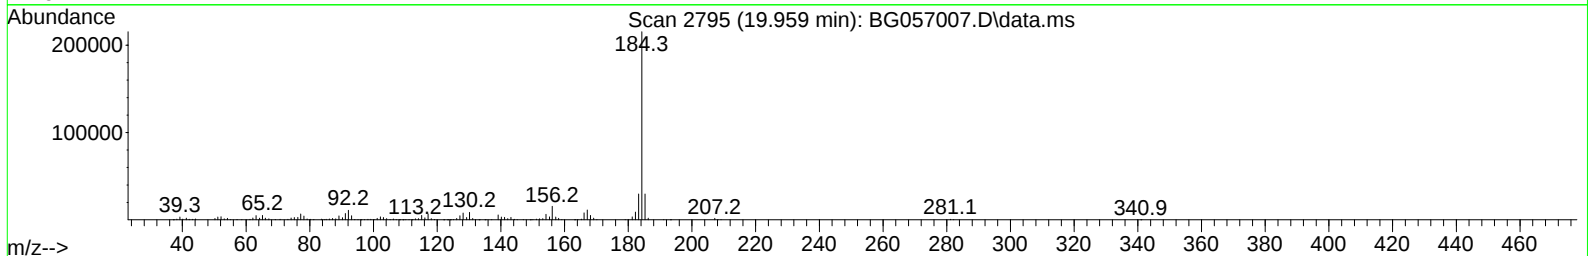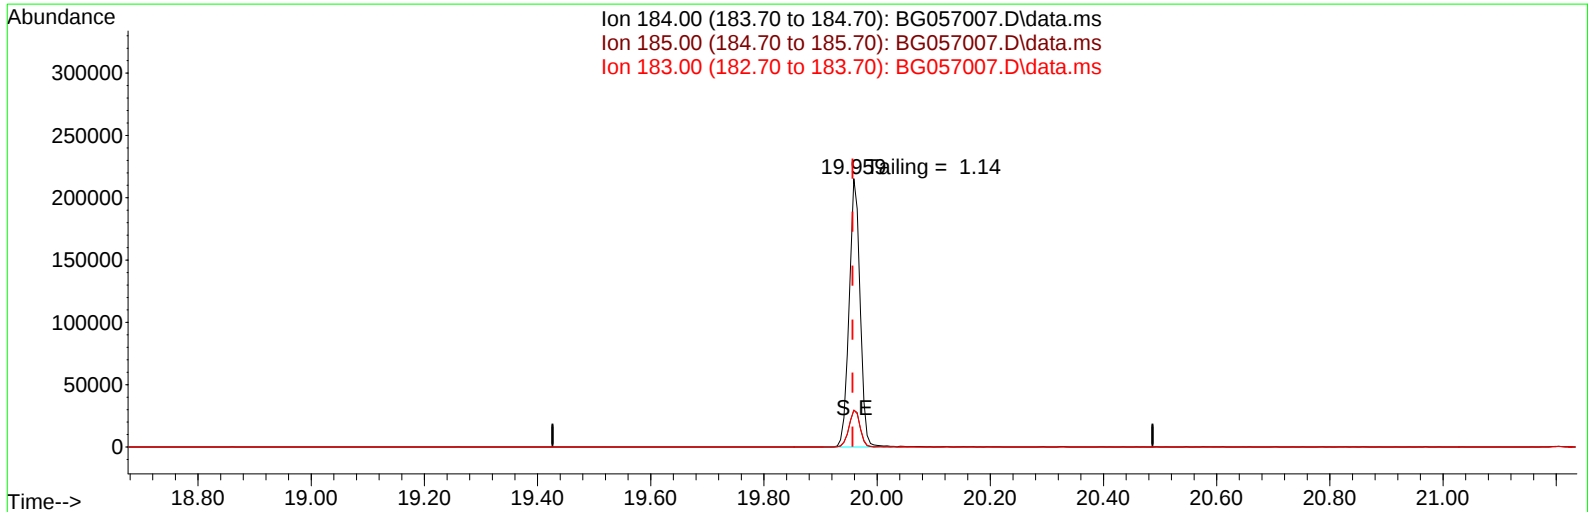

TIC: BG057007.D\data.ms

(77) Benzidine

19.959min (+ 0.003) 31160.81 ng

response 289587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.80
183.00	14.20	13.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2023	BNA_G	BG057007.D
Compound Name	Response	Retention Time
DDT	125487	21.204
DDD	3472	20.74
DDE	0	20.245
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3472	128959	2.69

Instrument :
BNA_G
ClientSampleId :
DFTPP