

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040715\
 Data File : BG016260.D
 Acq On : 7 Apr 2015 17:15
 Operator : TP/IZ
 Sample : G1776-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-38

Quant Time: Apr 08 02:39:30 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 08 03:25:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	63381	20.00	ng	0.00
21) Naphthalene-d8	10.48	136	299667	20.00	ng	0.00
38) Acenaphthene-d10	14.34	164	183478	20.00	ng	0.00
63) Phenanthrene-d10	17.08	188	402157	20.00	ng	0.00
75) Chrysene-d12	21.25	240	354724	20.00	ng	0.00
86) Perylene-d12	23.50	264	327041	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	227446	56.63	ng	0.00
7) Phenol-d6	6.87	99	208376	34.56	ng	0.00
23) Nitrobenzene-d5	8.86	82	443194	85.68	ng	0.00
41) 2,4,6-Tribromophenol	15.82	330	200703	161.75	ng	0.00
44) 2-Fluorobiphenyl	12.96	172	990936	91.95	ng	0.00
78) Terphenyl-d14	19.71	244	1254879	82.80	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040715\
Data File : BG016260.D
Acq On : 7 Apr 2015 17:15
Operator : TP/IZ
Sample : G1776-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-38

Quant Time: Apr 08 02:39:30 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 08 03:25:31 2015
Response via : Initial Calibration

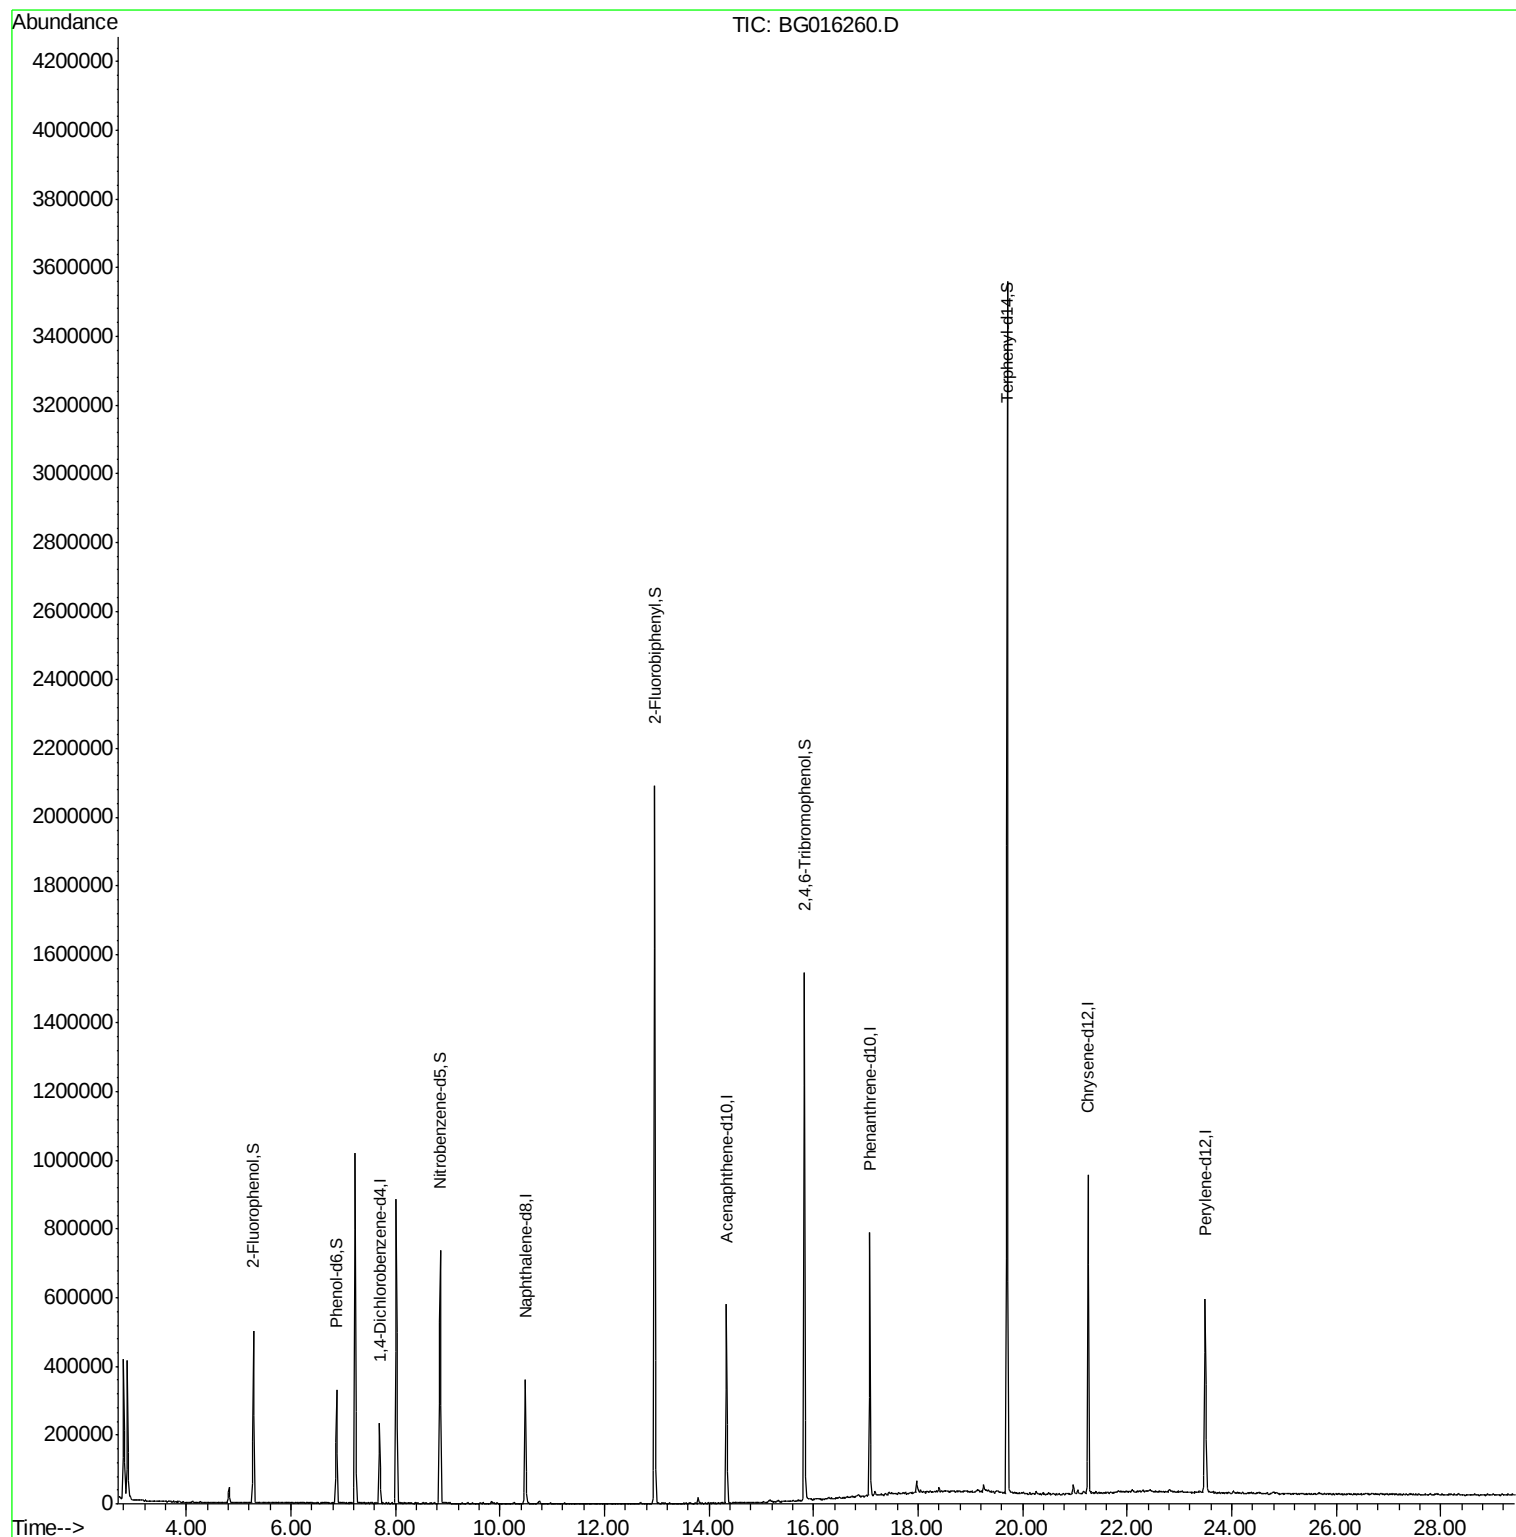

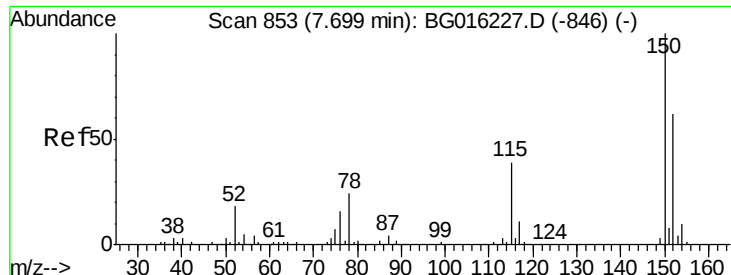


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.70 min Scan# 853
Delta R.T. -0.00 min
Lab File: BG016260.D
Acq: 7 Apr 2015 17:15

Instrument :
BNA_G
ClientSampleId :
MW-38

Tgt Ion:152 Resp: 63381
Ion Ratio Lower Upper
152 100
150 155.1 130.1 195.1
115 59.5 50.5 75.7

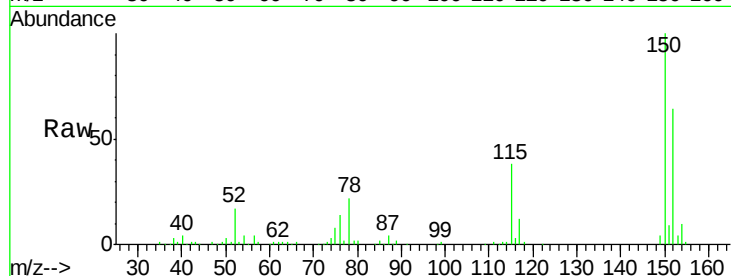


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

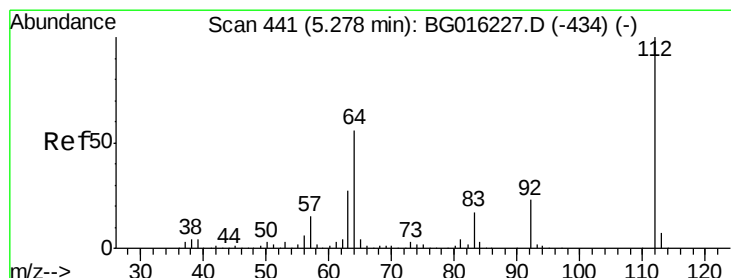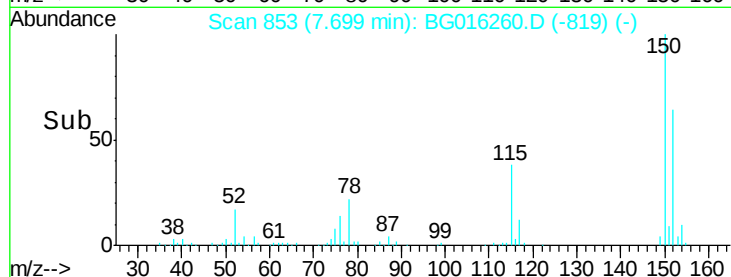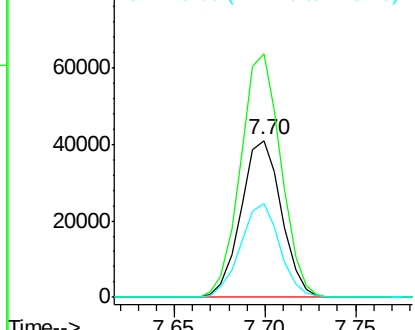



#5


2-Fluorophenol
Concen: 56.63 ng
RT: 5.28 min Scan# 441
Delta R.T. -0.00 min
Lab File: BG016260.D
Acq: 7 Apr 2015 17:15

Tgt Ion:112 Resp: 227446
Ion Ratio Lower Upper
112 100
64 54.3 44.5 66.7
63 25.7 21.4 32.0

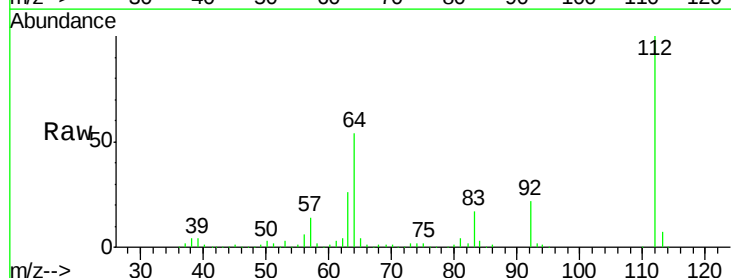

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

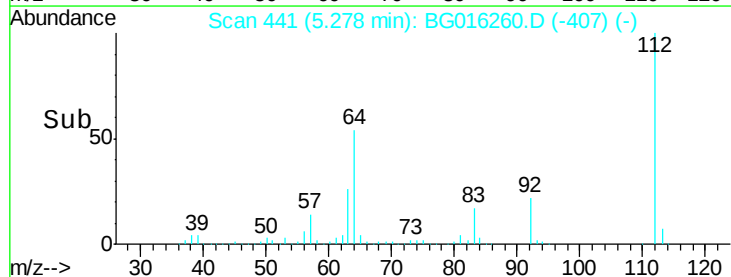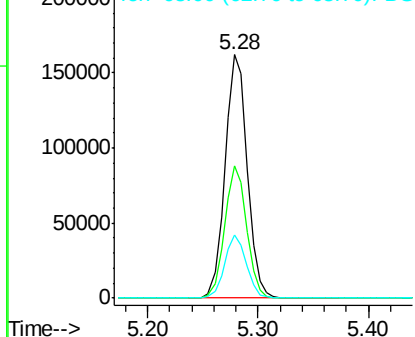

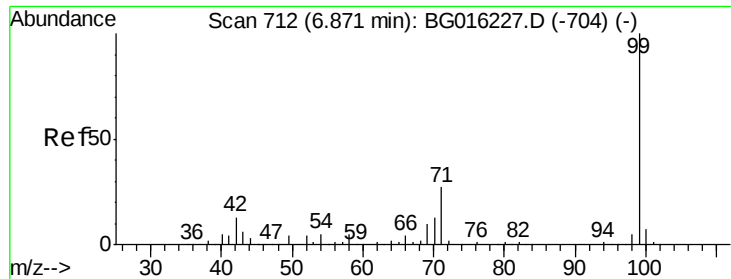

#7

Phenol-d6

Concen: 34.56 ng

RT: 6.87 min Scan# 712

Delta R.T. -0.00 min

Lab File: BG016260.D

Acq: 7 Apr 2015 17:15

Instrument :

BNA_G

ClientSampled :

MW-38


Tgt Ion: 99 Resp: 208376

Ion Ratio Lower Upper


99 100

42 11.7 10.0 15.0



71 24.7 21.5 32.3

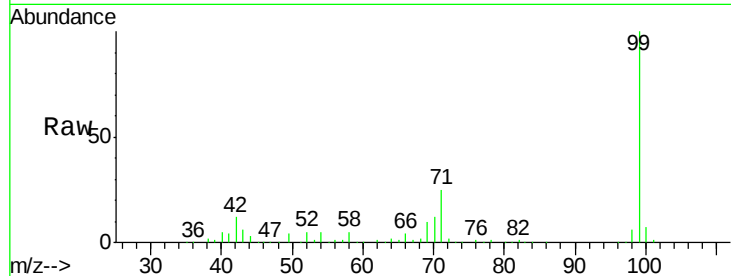

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

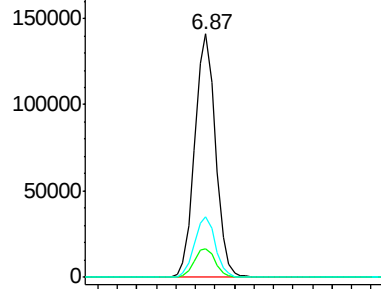

Time-->

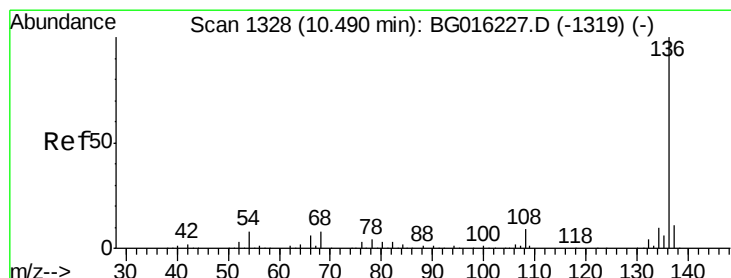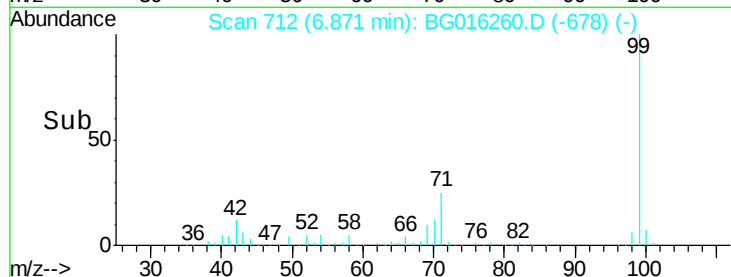

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.48 min Scan# 1327

Delta R.T. -0.00 min

Lab File: BG016260.D

Acq: 7 Apr 2015 17:15

Tgt Ion: 136 Resp: 299667


Ion Ratio Lower Upper

136 100


137 11.0 8.7 13.1

54 7.4 6.3 9.5


68 7.2 6.5 9.7

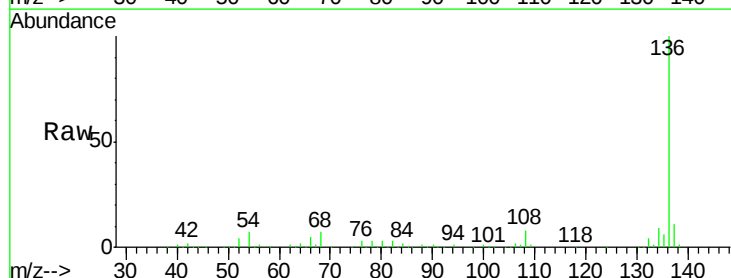


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

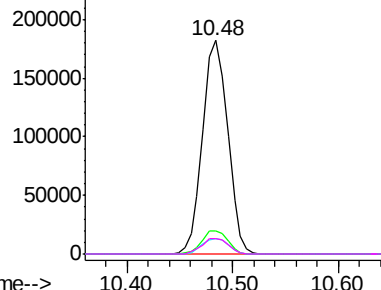

Time-->

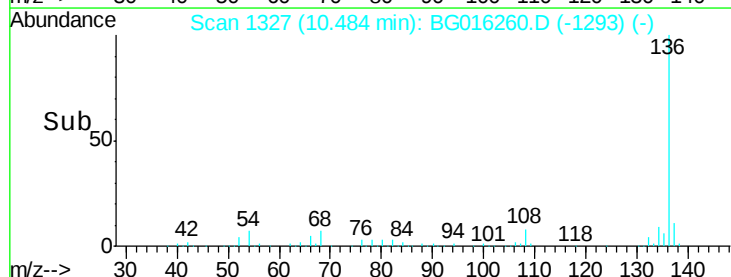


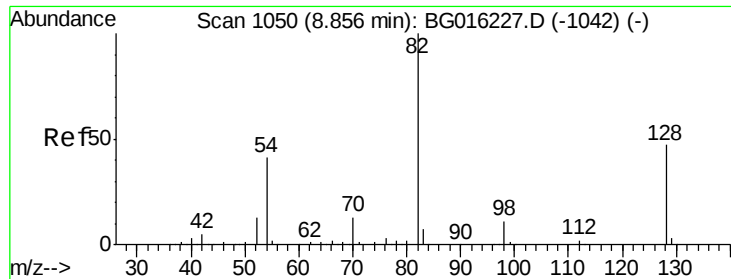




#23
 Nitrobenzene-d5
 Concen: 85.68 ng
 RT: 8.86 min Scan# 1050
 Delta R.T. -0.00 min
 Lab File: BG016260.D
 Acq: 7 Apr 2015 17:15

Instrument :
 BNA_G
 ClientSampleId :
 MW-38

Tgt Ion: 82 Resp: 443194
 Ion Ratio Lower Upper
 82 100
 128 52.3 37.8 56.8
 54 41.0 32.6 49.0

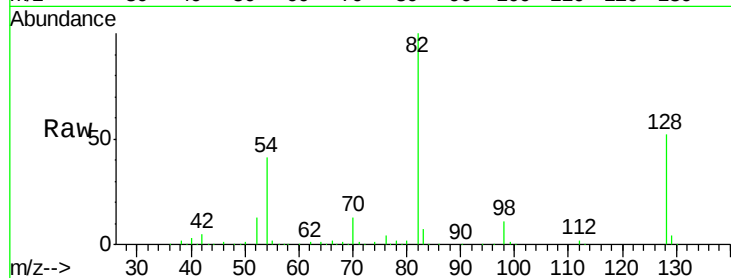


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

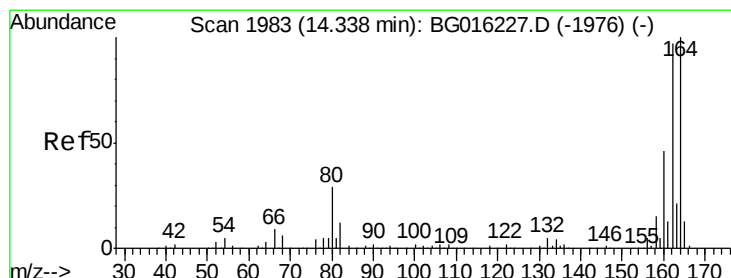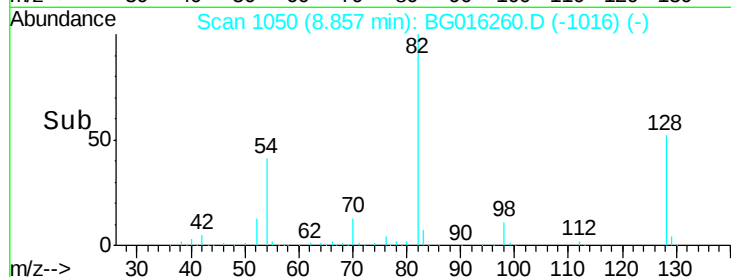
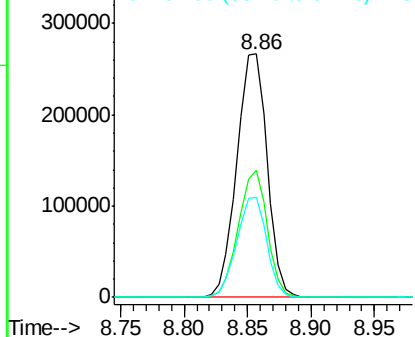



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.34 min Scan# 1983
 Delta R.T. -0.00 min
 Lab File: BG016260.D
 Acq: 7 Apr 2015 17:15

Tgt Ion: 164 Resp: 183478
 Ion Ratio Lower Upper
 164 100
 162 99.9 77.3 115.9
 160 45.7 36.7 55.1

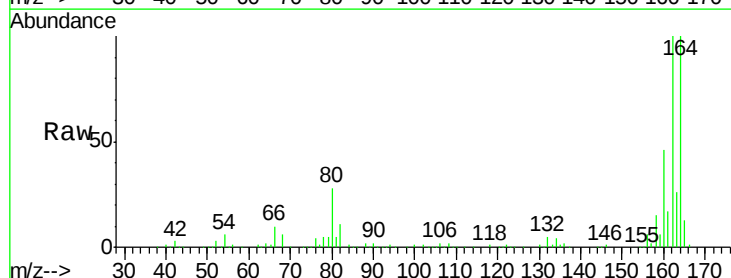

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

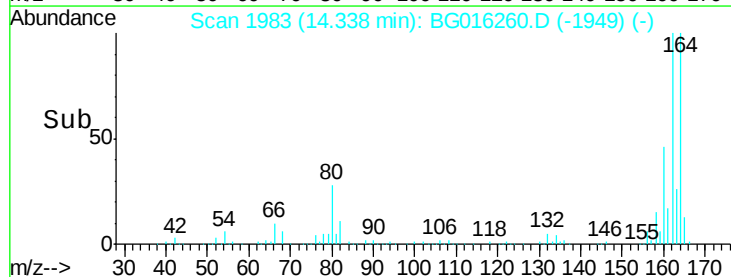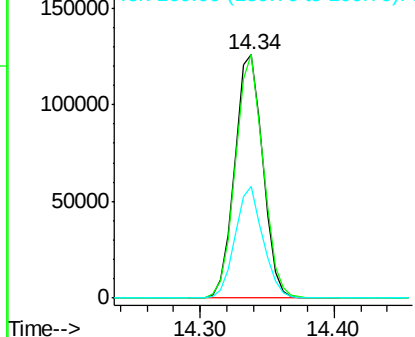


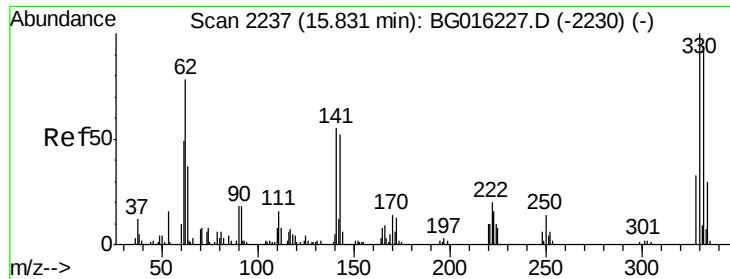




#41
 2,4,6-Tribromophenol
 Concen: 161.75 ng
 RT: 15.82 min Scan# 2236
 Delta R.T. -0.01 min
 Lab File: BG016260.D
 Acq: 7 Apr 2015 17:15

Instrument :
 BNA_G
 ClientSampleId :
 MW-38

Tgt Ion:330 Resp: 200703
 Ion Ratio Lower Upper
 330 100
 332 96.2 75.8 113.6
 141 56.4 46.6 69.8

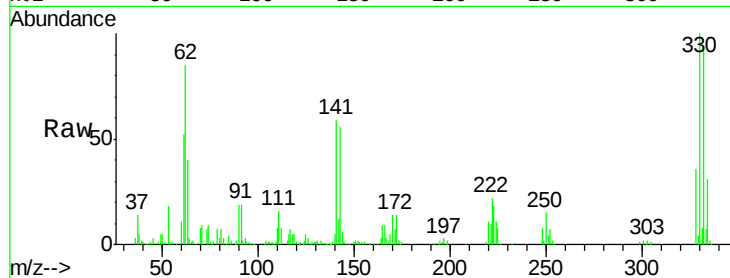


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

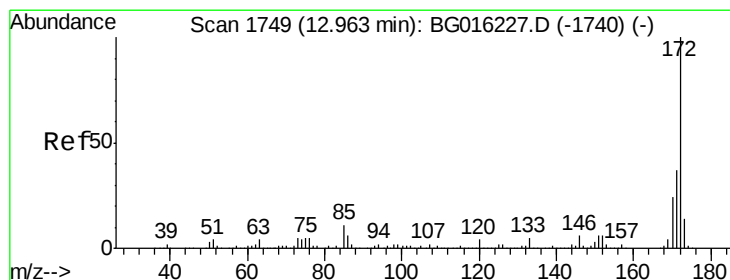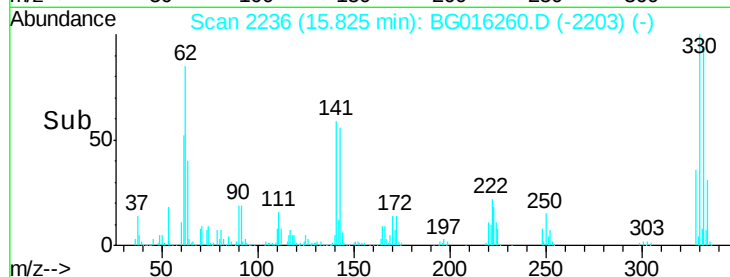
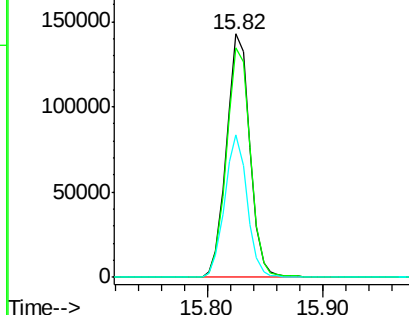



#44
 2-Fluorobiphenyl
 Concen: 91.95 ng
 RT: 12.96 min Scan# 1748
 Delta R.T. -0.01 min
 Lab File: BG016260.D
 Acq: 7 Apr 2015 17:15

Tgt Ion:172 Resp: 990936
 Ion Ratio Lower Upper
 172 100
 171 37.5 29.6 44.4
 170 24.4 19.4 29.2

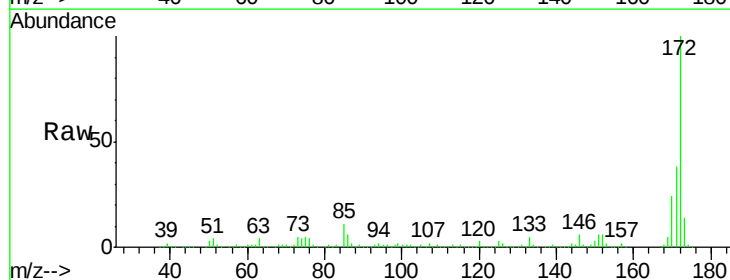

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

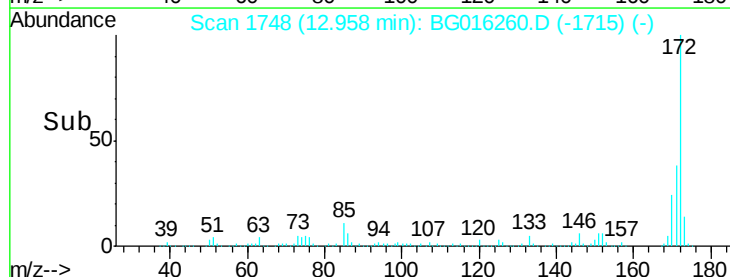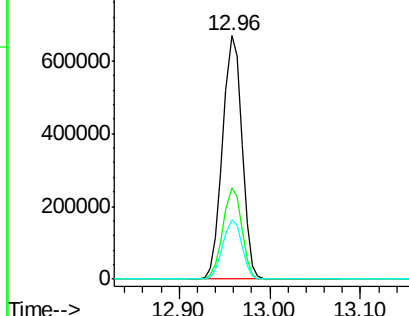


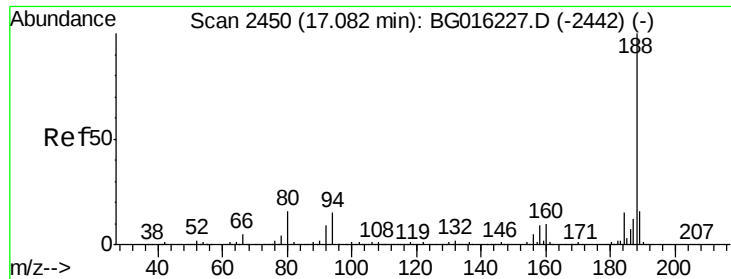




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.08 min Scan# 2449
Delta R.T. -0.00 min
Lab File: BG016260.D
Acq: 7 Apr 2015 17:15

Instrument :
BNA_G
ClientSampleId :
MW-38

Tgt Ion	Ratio	Lower	Upper
188	100		
94	14.7	12.2	18.4
80	15.2	12.8	19.2

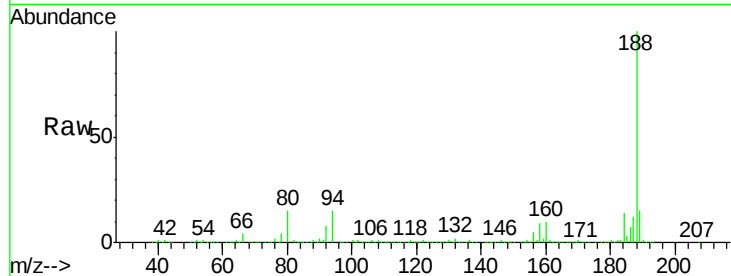


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

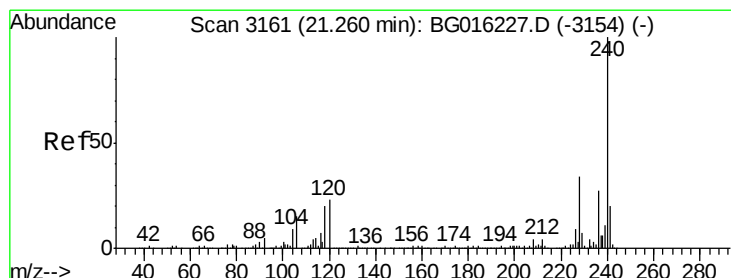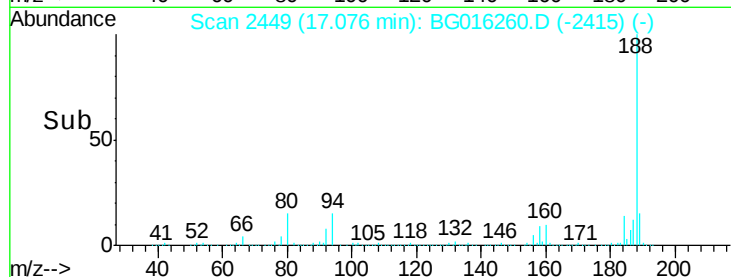
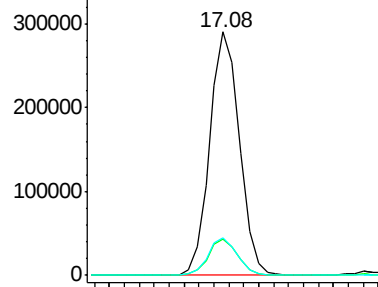



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.25 min Scan# 3160
Delta R.T. -0.01 min
Lab File: BG016260.D
Acq: 7 Apr 2015 17:15

Tgt Ion	Ratio	Lower	Upper
240	100		
120	21.0	18.6	28.0
236	25.6	21.7	32.5

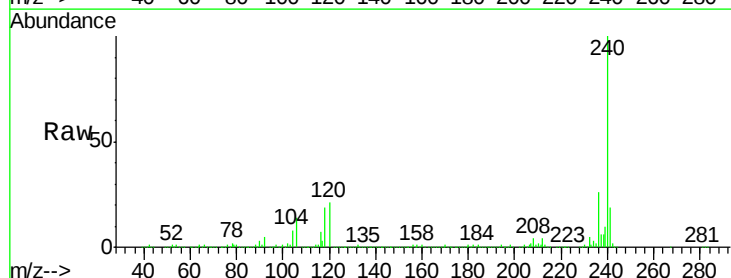

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

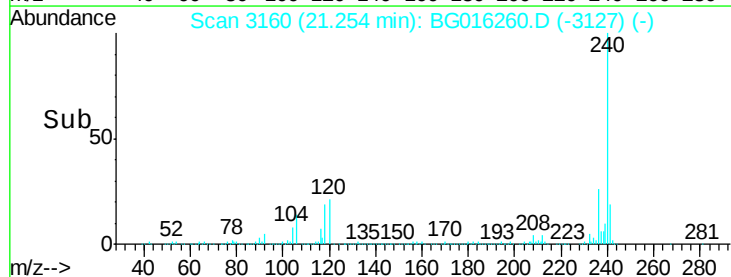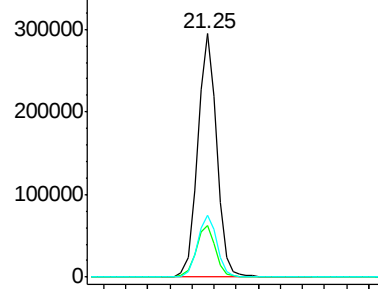

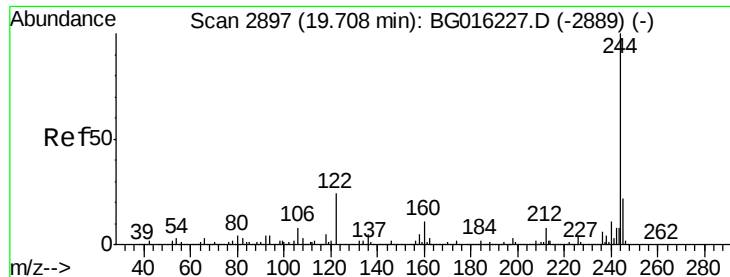

#78

Terphenyl-d14

Concen: 82.80 ng

RT: 19.71 min Scan# 2897

Delta R.T. -0.00 min

Lab File: BG016260.D

Acq: 7 Apr 2015 17:15

Instrument :

BNA_G

ClientSampleId :

MW-38


Tgt Ion:244 Resp: 1254879

Ion Ratio Lower Upper

244 100

212 8.8 6.6 9.8




122 24.1 19.1 28.7

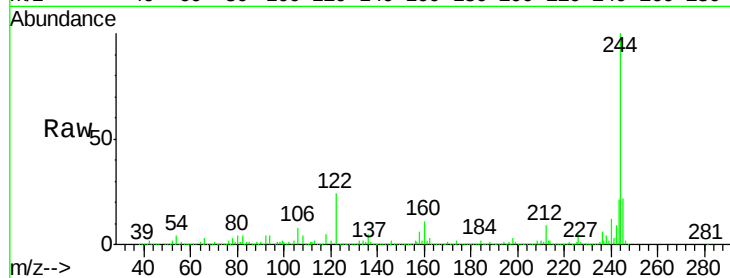

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

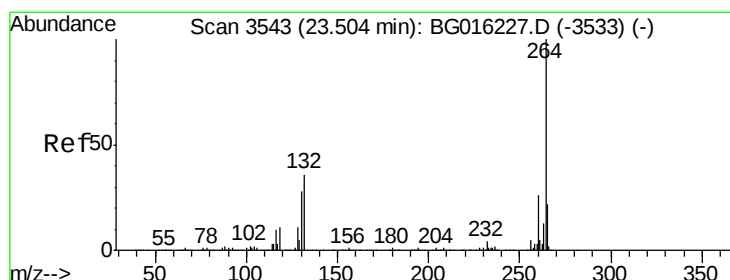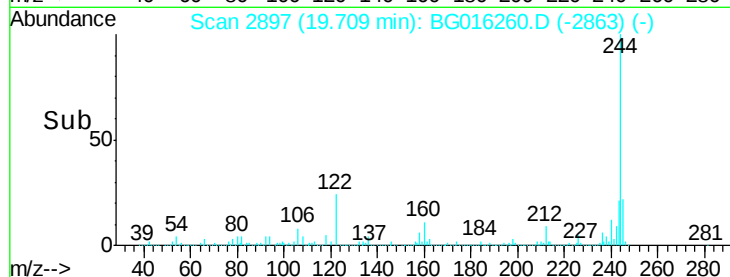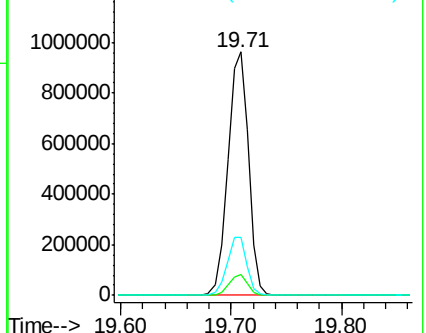

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.50 min Scan# 3542

Delta R.T. -0.00 min

Lab File: BG016260.D

Acq: 7 Apr 2015 17:15


Tgt Ion:264 Resp: 327041

Ion Ratio Lower Upper

264 100

260 23.7 20.4 30.6

265 21.2 17.2 25.8

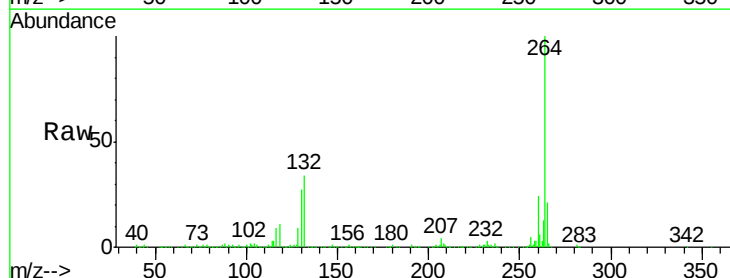

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

