


Data Path : Z:\HPCHEM1\BNA_G\Data\BG040715\
 Data File : BG016255.D
 Acq On : 7 Apr 2015 14:15
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 04:17:17 2015

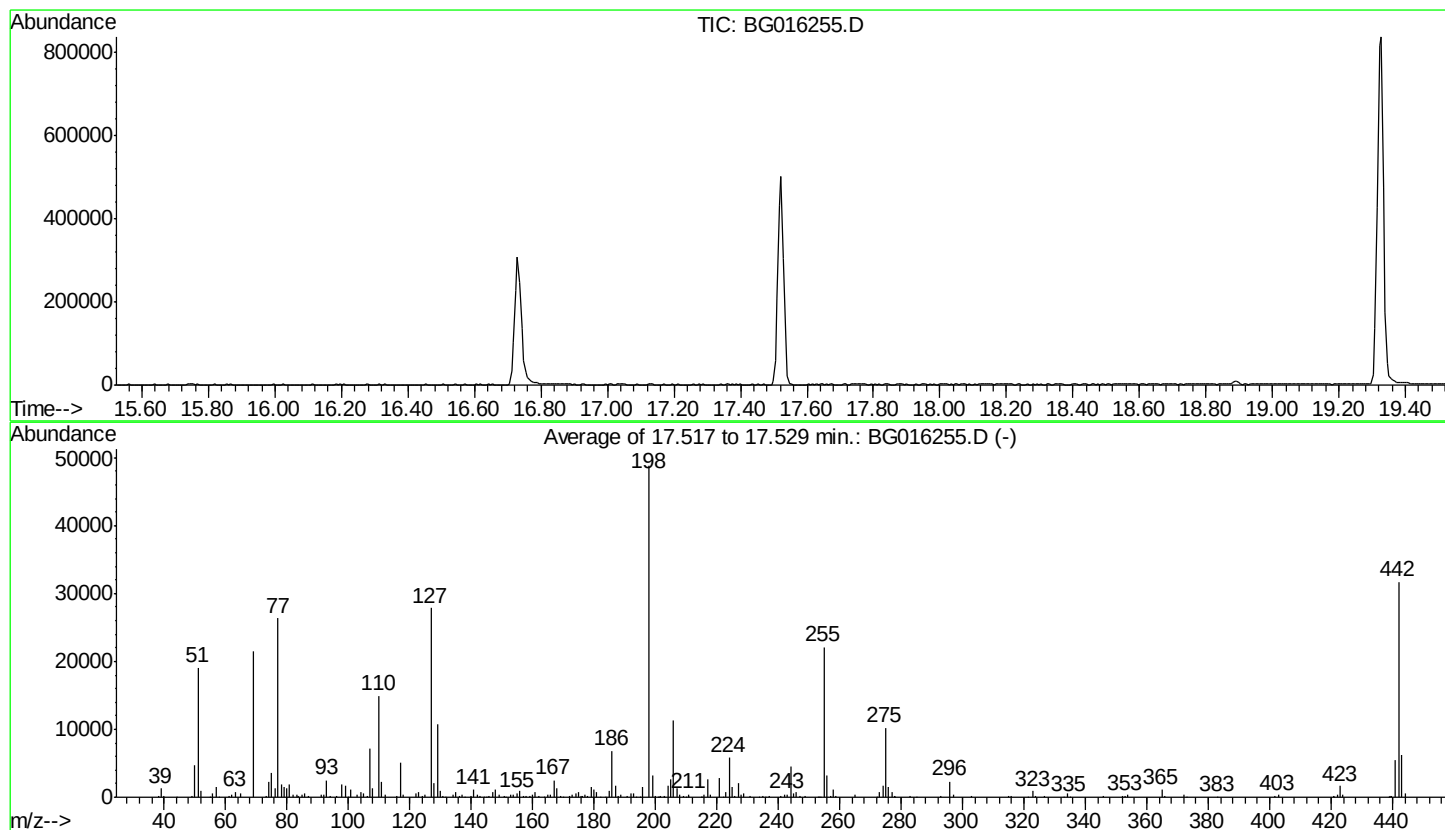

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	19082	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.9	21449	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.0	27829	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48829	PASS
199	198	5	9	6.7	3264	PASS
275	198	10	60	21.0	10235	PASS
365	198	1	100	2.2	1068	PASS
441	442	0.01	24	17.5	5561	PASS
442	198	50	100	65.0	31757	PASS
443	442	15	24	19.5	6202	PASS