
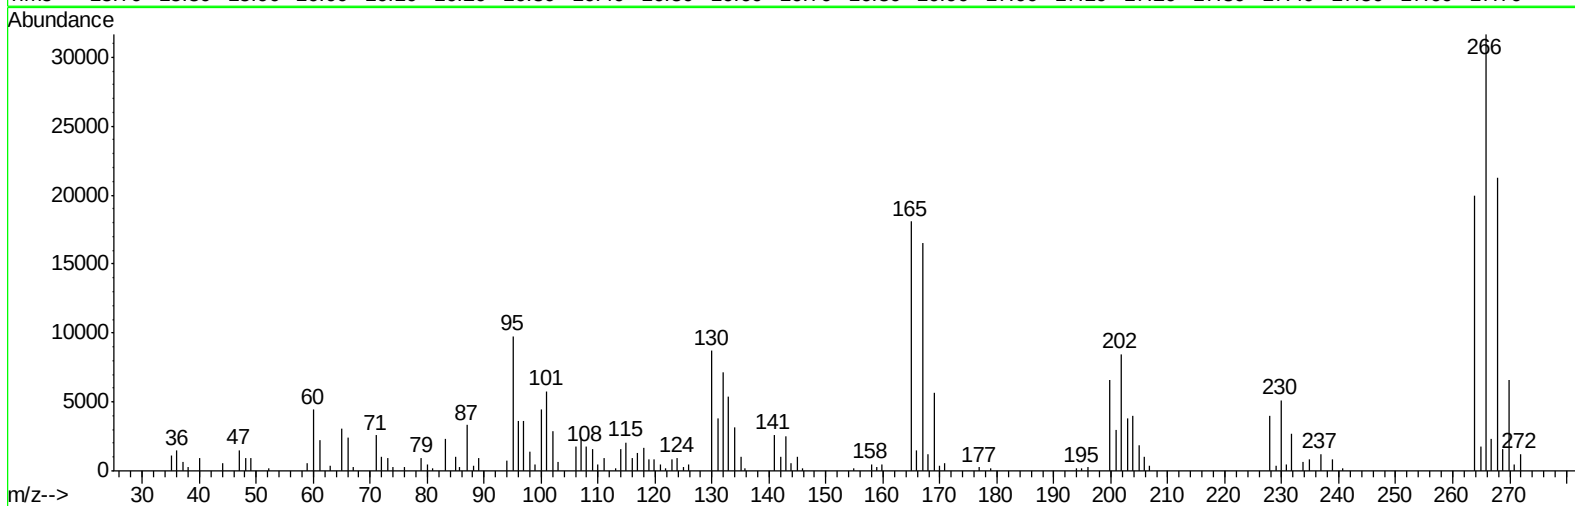


Data Path : Z:\HPCHEM1\BNA G\Data\BG040715\
Data File : BG016255.D
Acq On : 7 Apr 2015 14:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:40:12 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

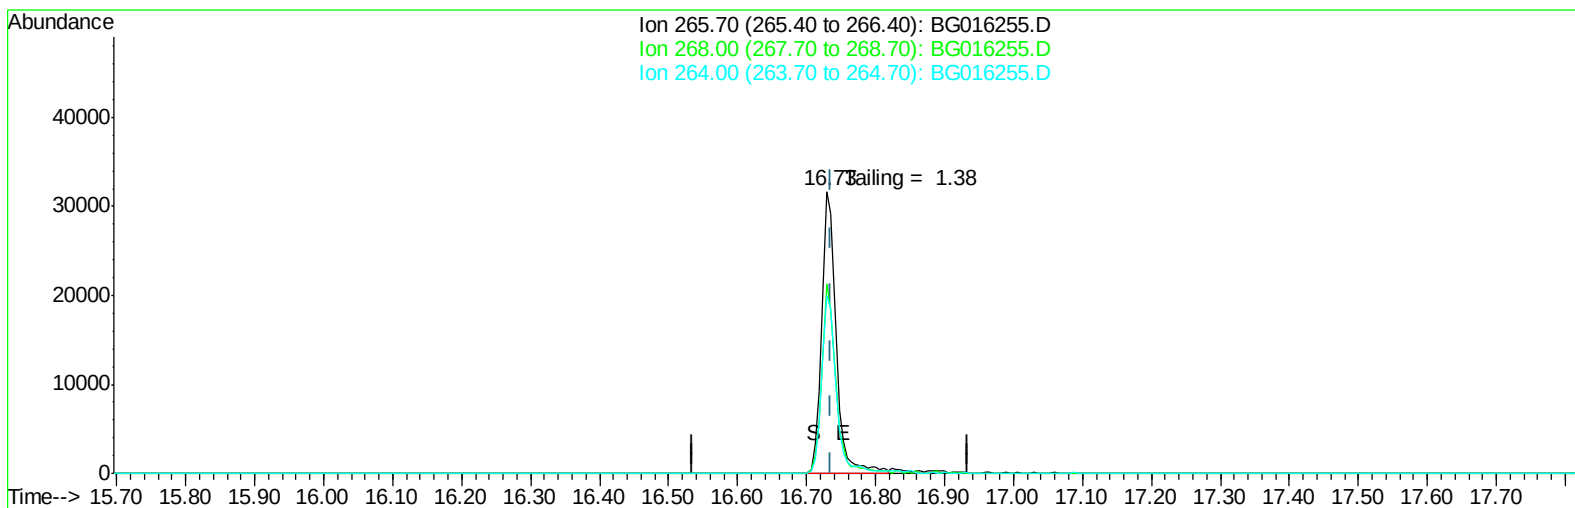

TIC: BG016255.D

(69) Pentachlorophenol (C)



16.730min (-0.005) 0.00ng

response 46102

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	67.14
264.00	66.00	63.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG040715\
Data File : BG016255.D
Acq On : 7 Apr 2015 14:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:40:12 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

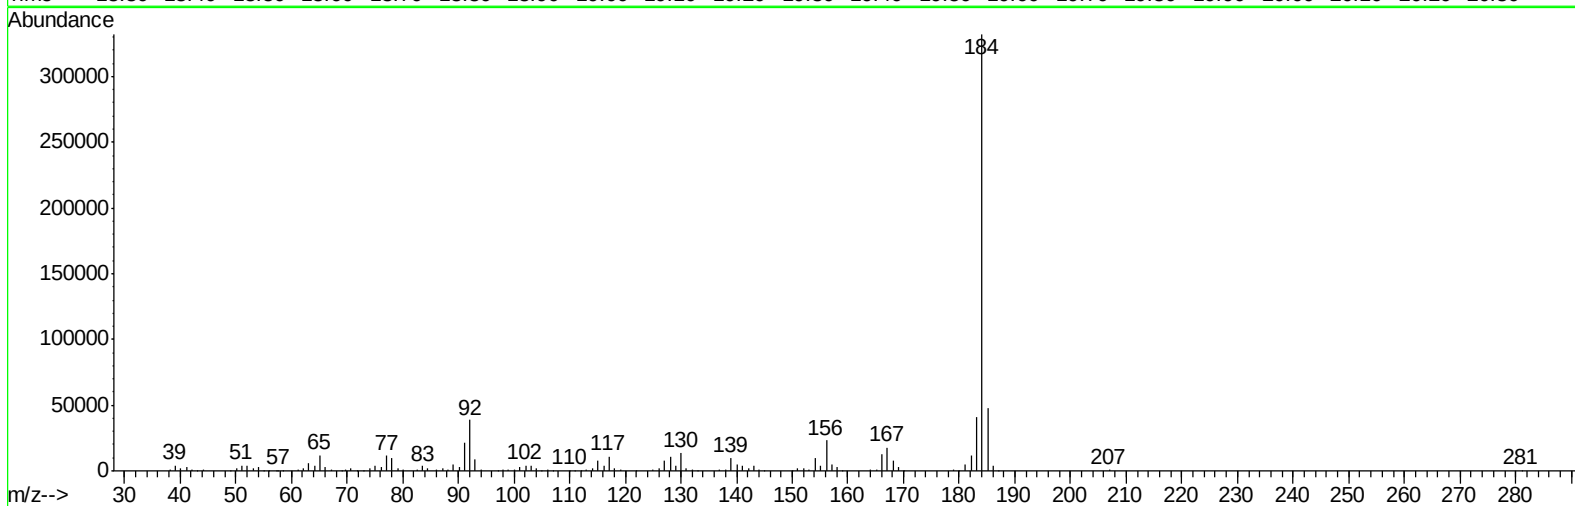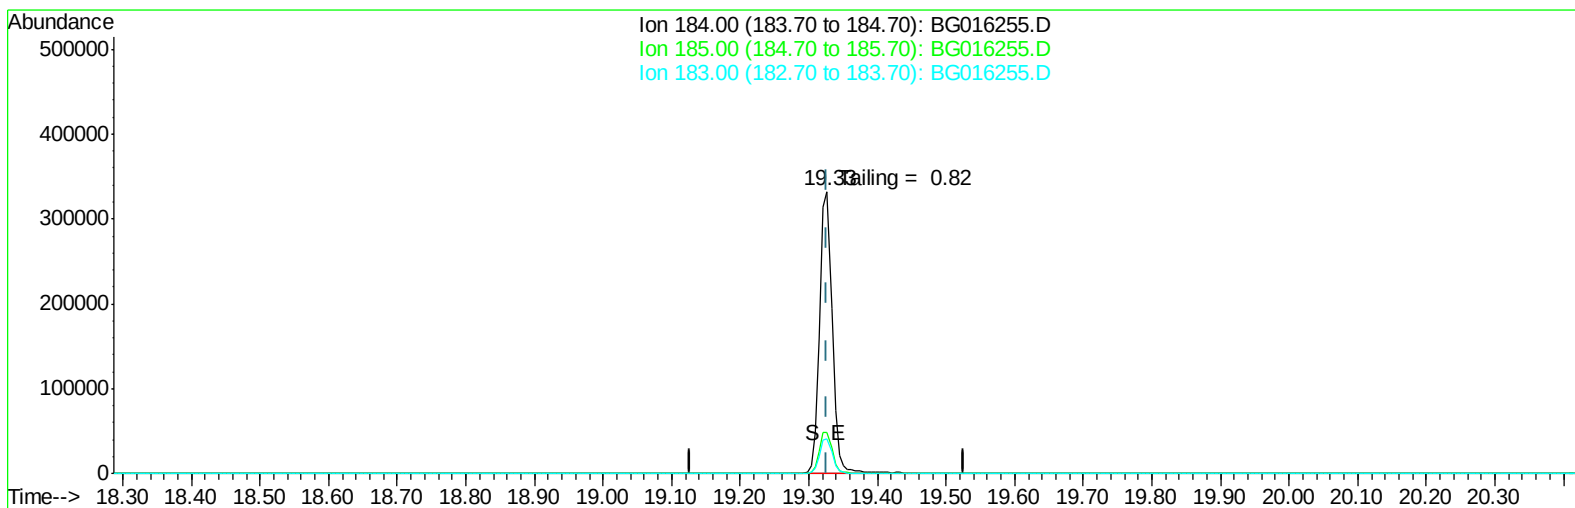

TIC: BG016255.D

(76) Benzidine

19.327min (+0.000) 0.00ng

response 418640

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.50
183.00	13.00	12.39
0.00	0.00	0.00