
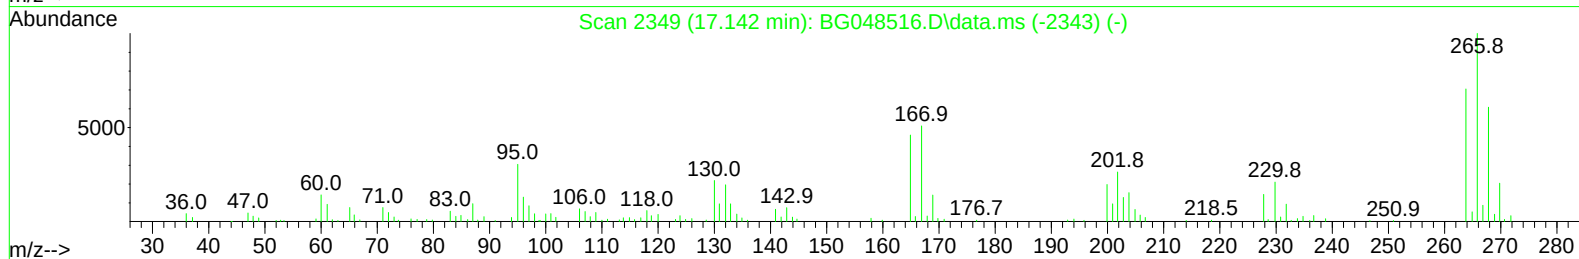
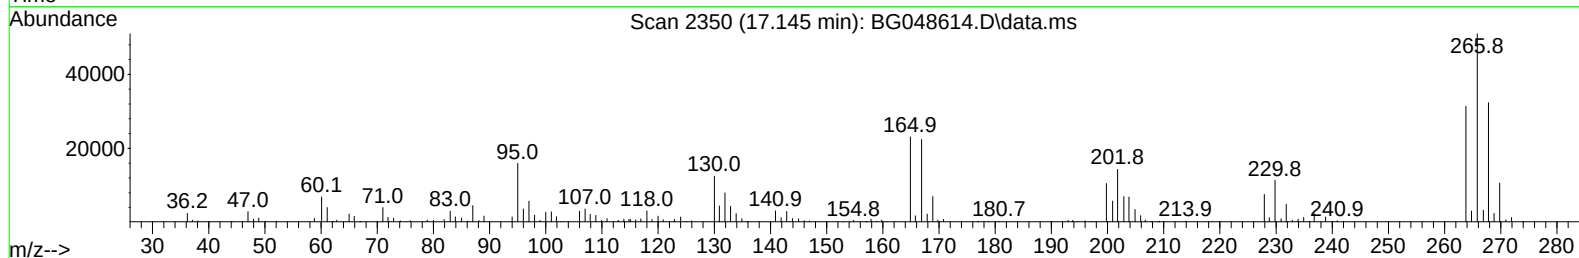


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040721\
Data File : BG048614.D
Acq On : 7 Apr 2021 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 13:25:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

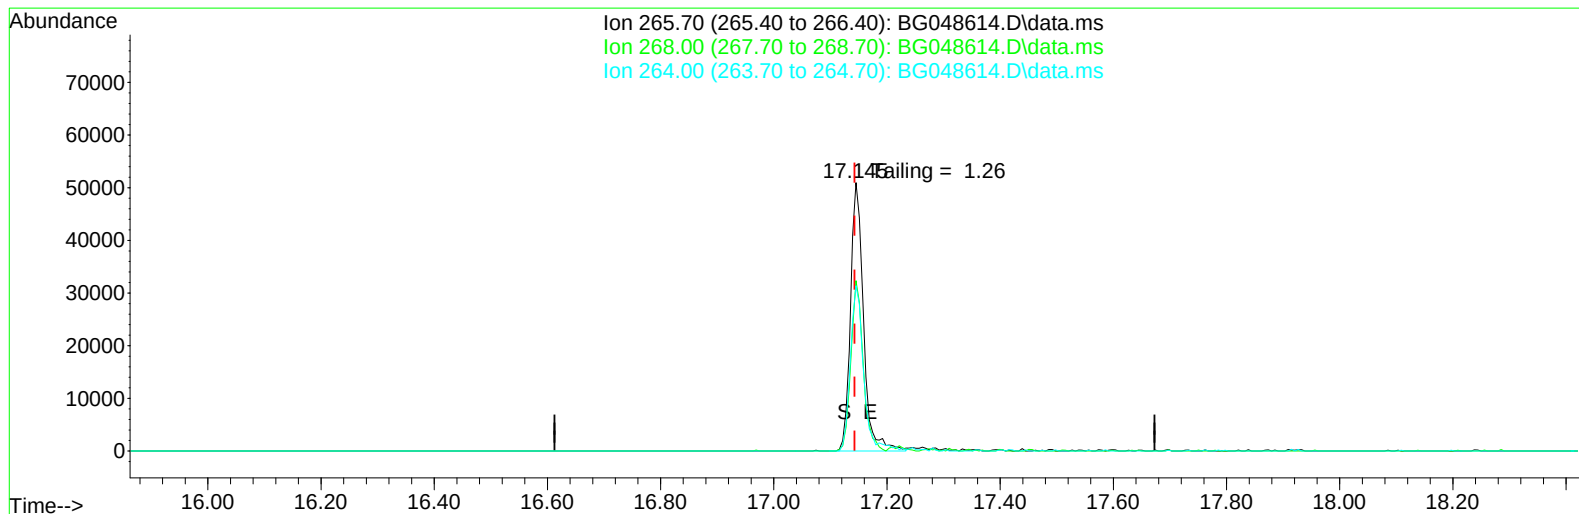

TIC: BG048614.D\data.ms

(70) Pentachlorophenol (C)




17.145min (+ 0.003) 0.00 ng

response 81248

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	63.46
264.00	70.50	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040721\
Data File : BG048614.D
Acq On : 7 Apr 2021 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 13:25:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

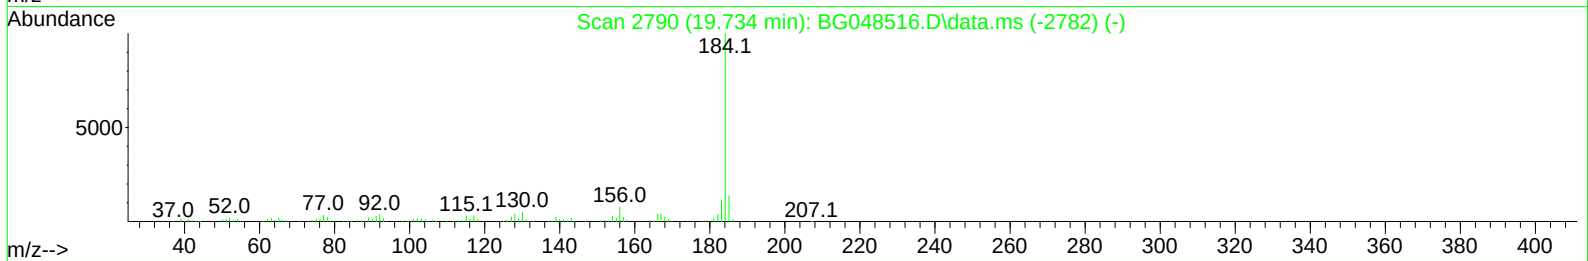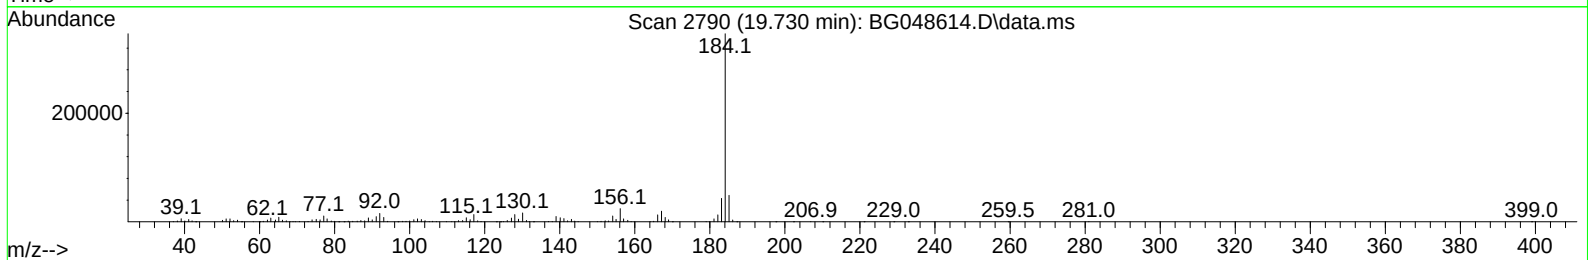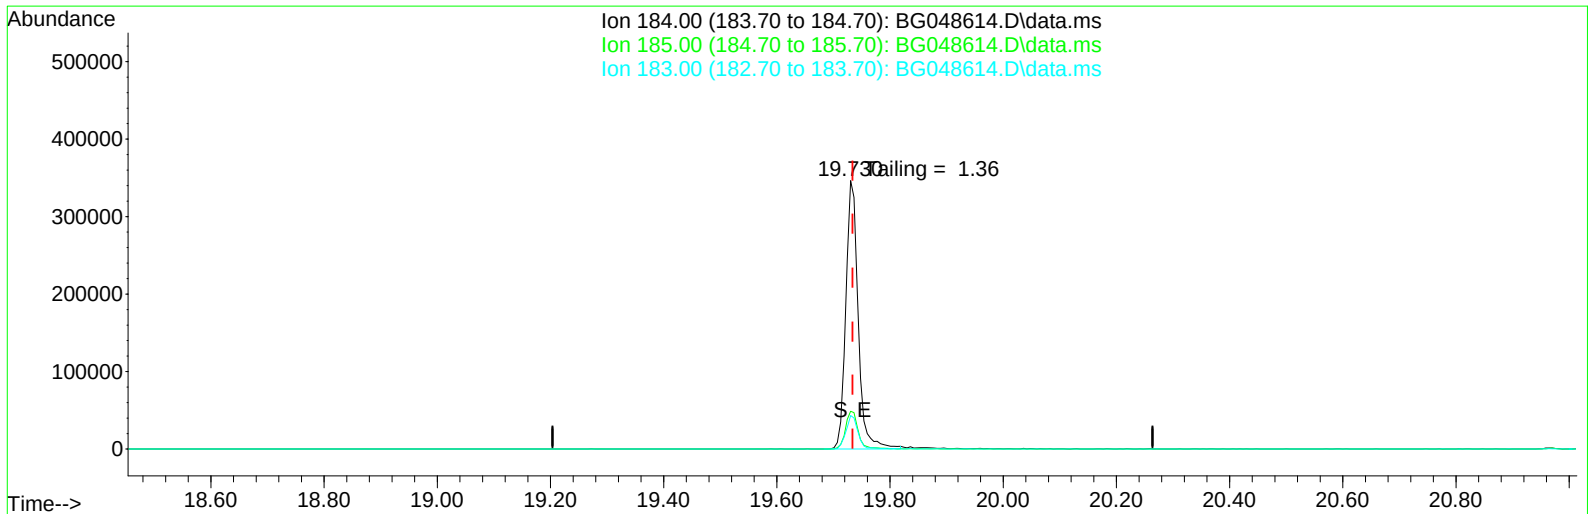

TIC: BG048614.D\data.ms

(77) Benzidine**19.730min (-0.003) 157493.12 ng****response 527986**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.07
183.00	11.50	12.45
0.00	0.00	0.00