
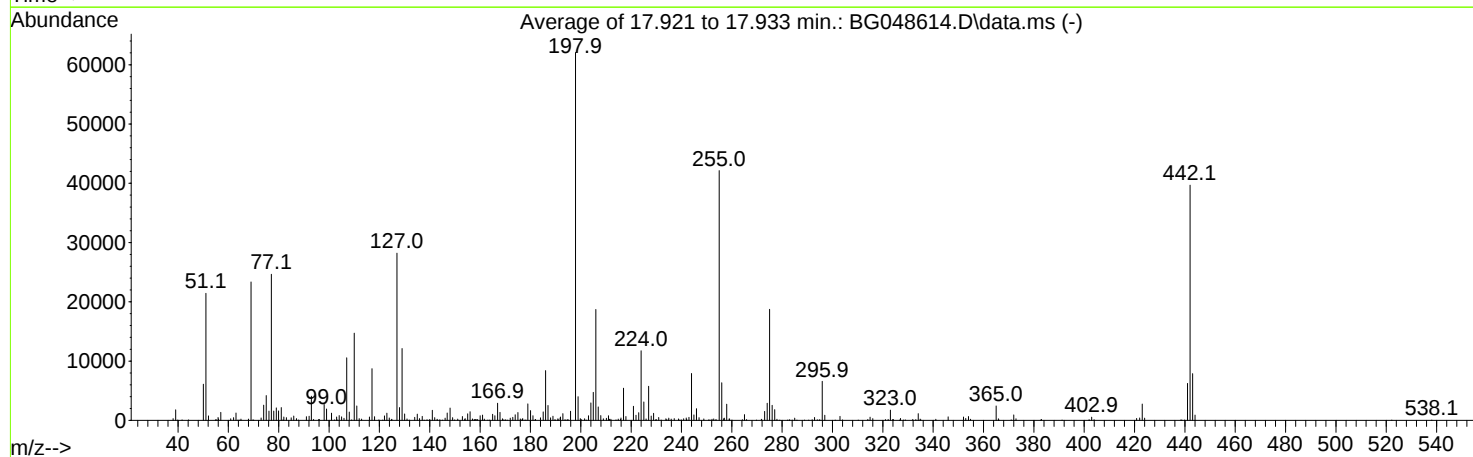


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040721\
 Data File : BG048614.D
 Acq On : 7 Apr 2021 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:06:00 2021

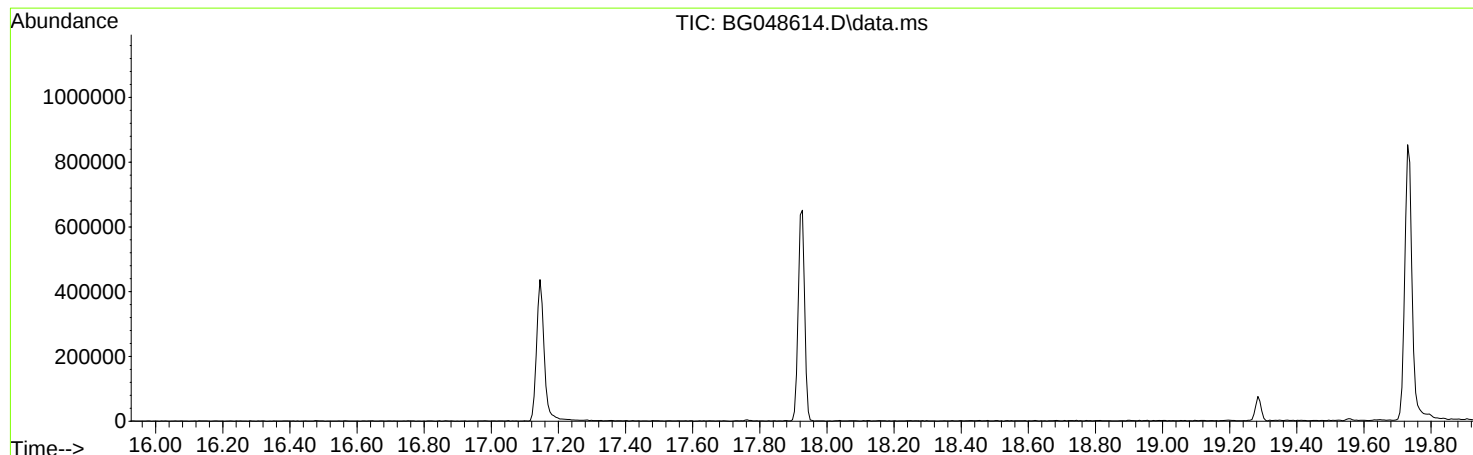

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	21436	PASS
68	69	0.00	2	1.0	230	PASS
69	198	0.00	100	37.6	23355	PASS
70	69	0.00	2	0.4	93	PASS
127	198	10	80	45.4	28203	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62067	PASS
199	198	5	9	6.4	3996	PASS
275	198	10	60	30.2	18747	PASS
365	198	1	100	3.9	2425	PASS
441	198	0.01	100	10.1	6246	PASS
442	198	50	100	63.9	39680	PASS
443	442	15	24	19.9	7884	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2021	BNA_G	<u>BG048614.D</u>
Compound Name	Response	Retention Time
DDT	294594	20.96
DDD	5068	20.51
DDE	882	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5950	300544	1.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040721\
Data File : BG048614.D
Acq On : 7 Apr 2021 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 07 13:25:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

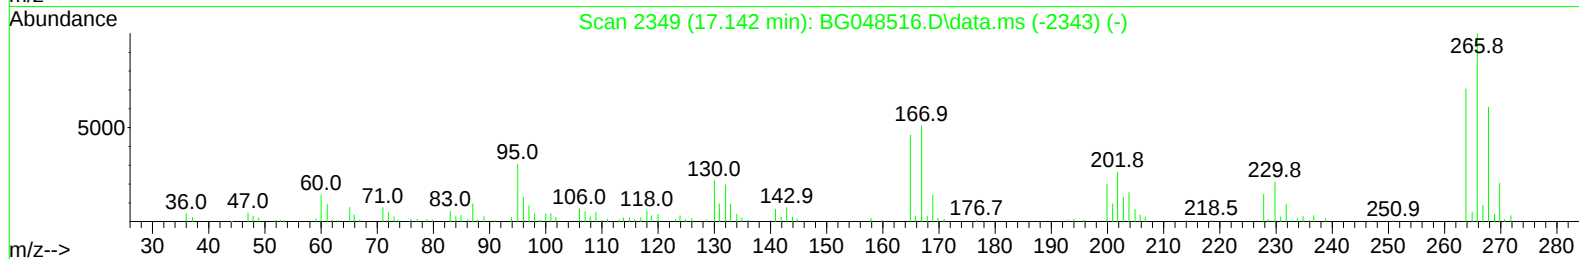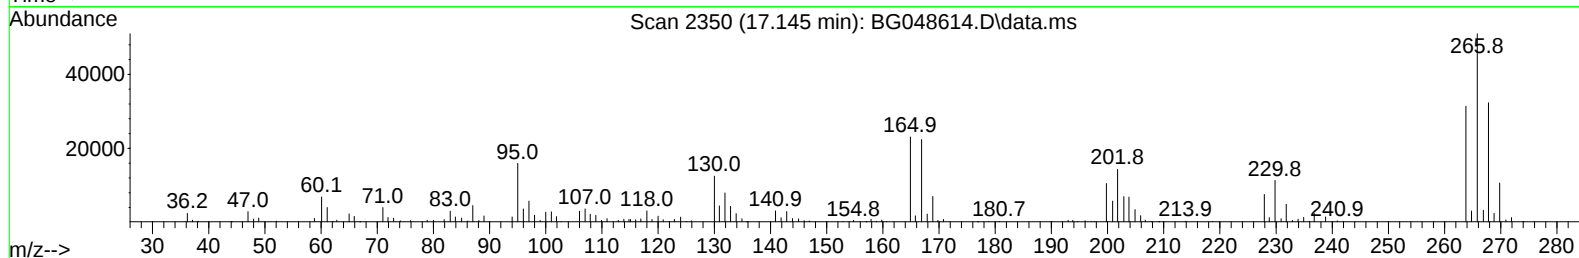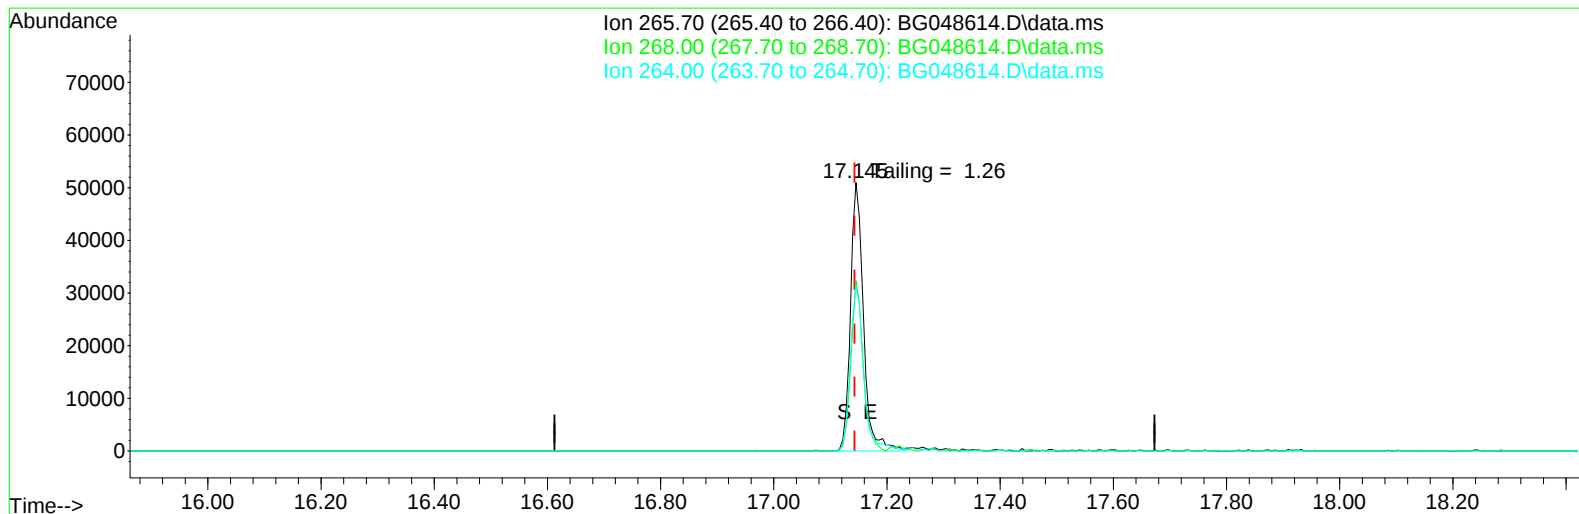

TIC: BG048614.D\data.ms

(70) Pentachlorophenol (C)

17.145min (+ 0.003) 0.00 ng




response 81248

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	63.46
264.00	70.50	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040721\
 Data File : BG048614.D
 Acq On : 7 Apr 2021 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 13:25:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 07 10:06:00 2021
 Response via : Initial Calibration

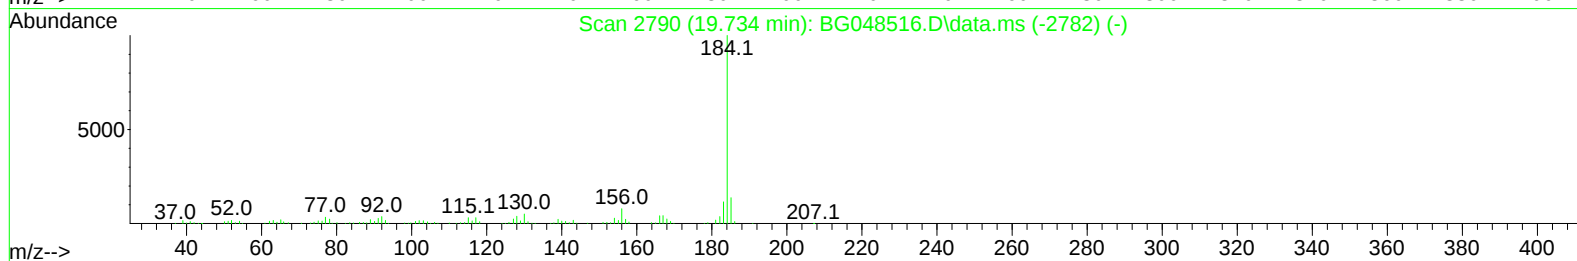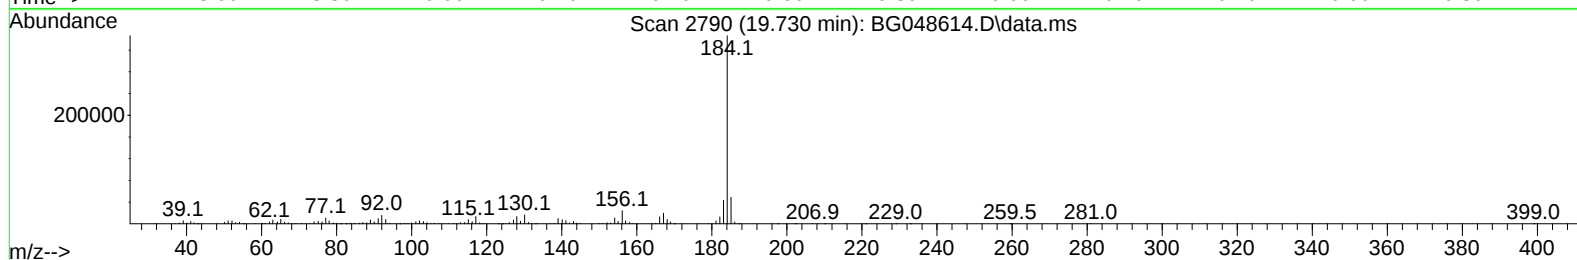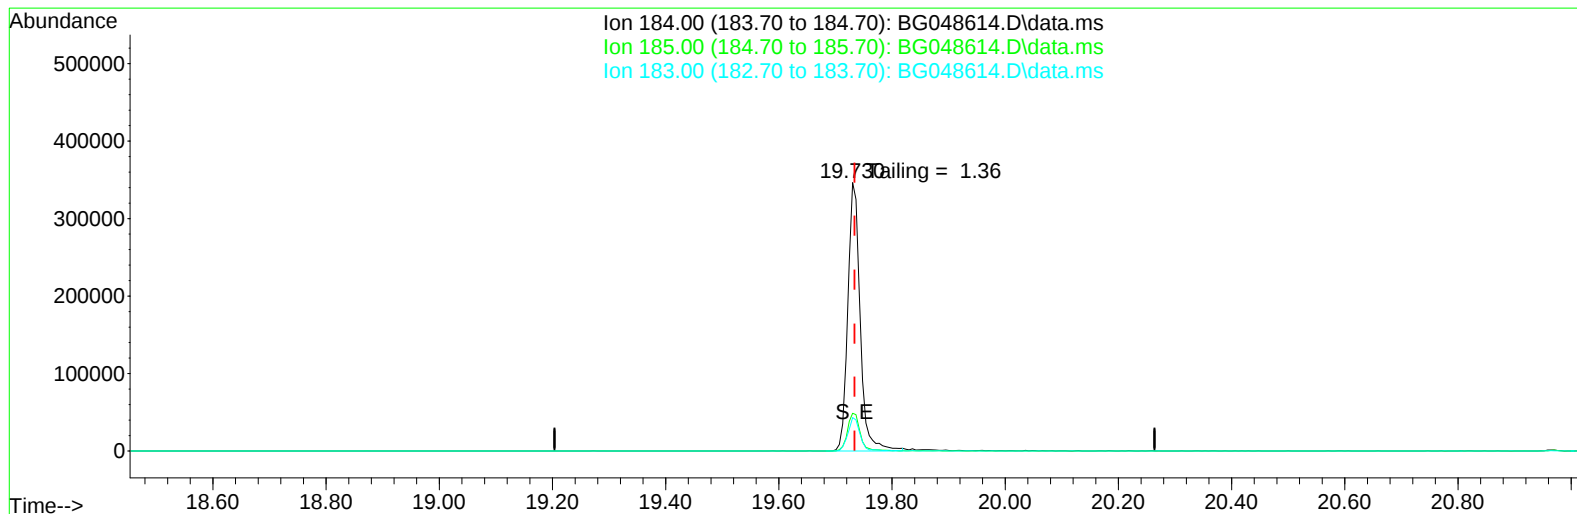

TIC: BG048614.D\data.ms

(77) Benzidine

19.730min (-0.003) 157493.12 ng

response 527986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.07
183.00	11.50	12.45
0.00	0.00	0.00