
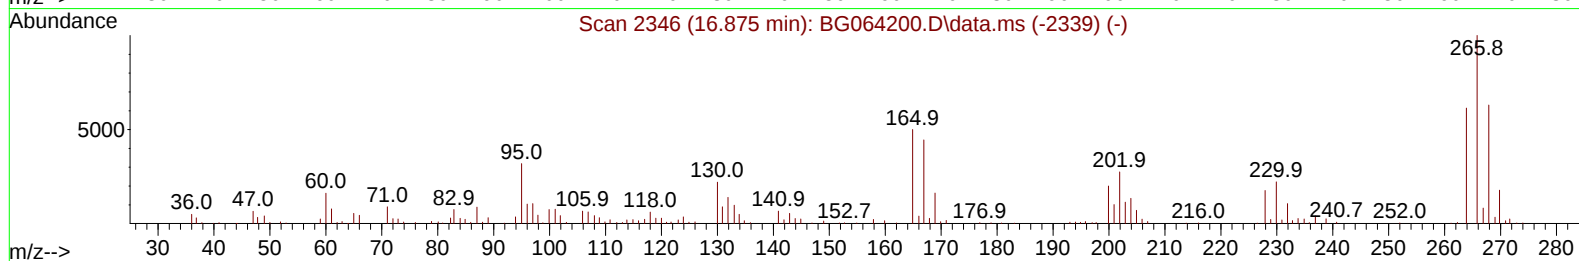
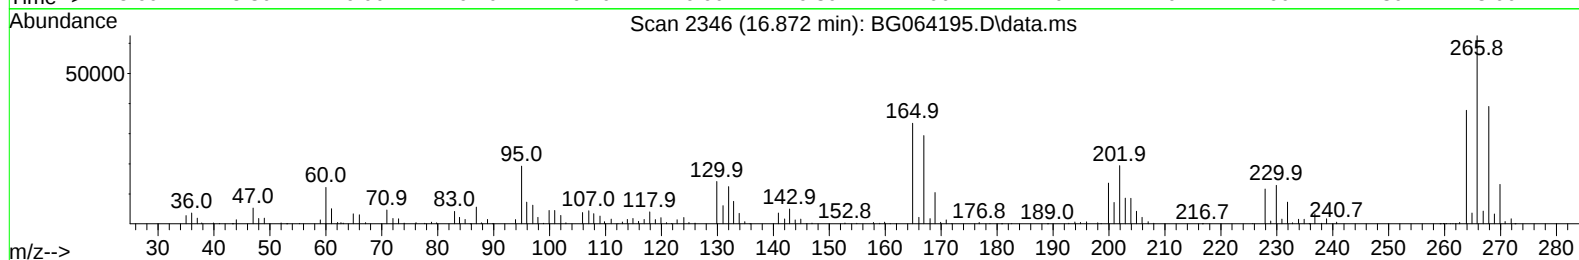


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040725\
Data File : BG064195.D
Acq On : 7 Apr 2025 8:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 07 17:00:17 2025
Response via : Initial Calibration

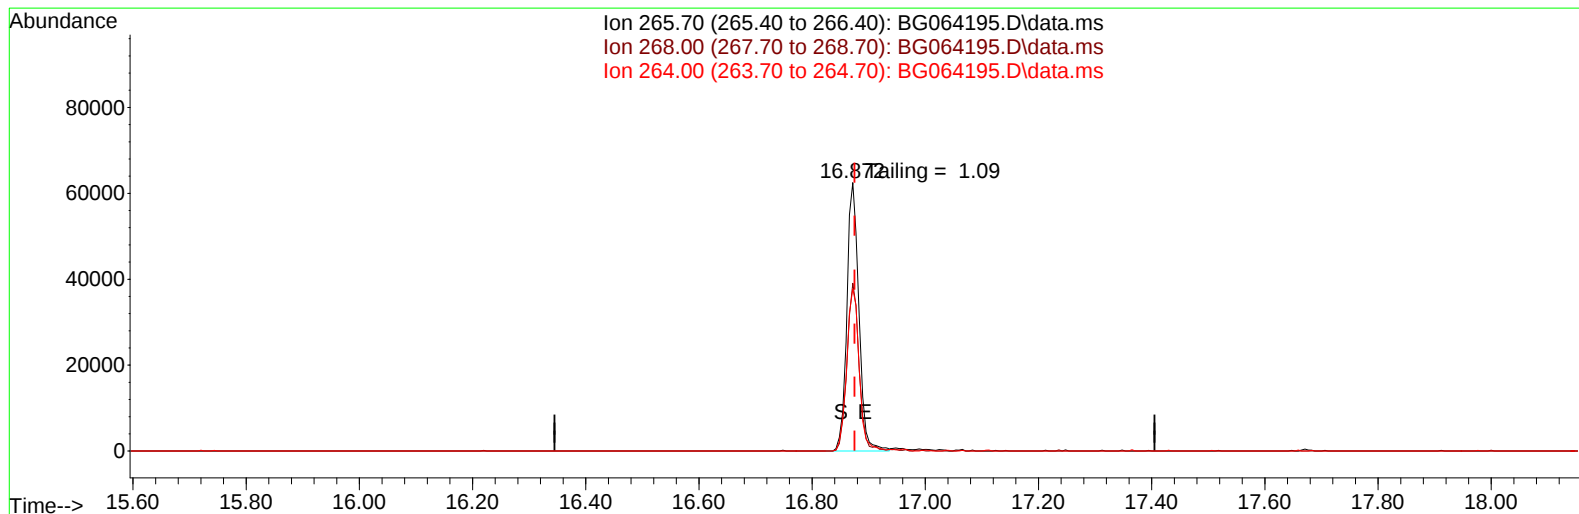

TIC: BG064195.D\data.ms

(70) Pentachlorophenol (C)




16.872min (-0.003) 15255.01 ng

response 92312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.47
264.00	61.40	60.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040725\
Data File : BG064195.D
Acq On : 7 Apr 2025 8:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 07 17:00:17 2025
Response via : Initial Calibration

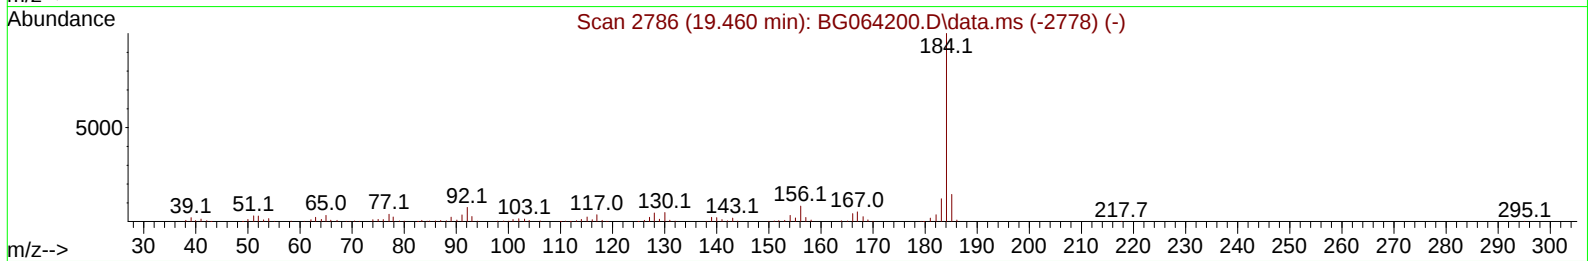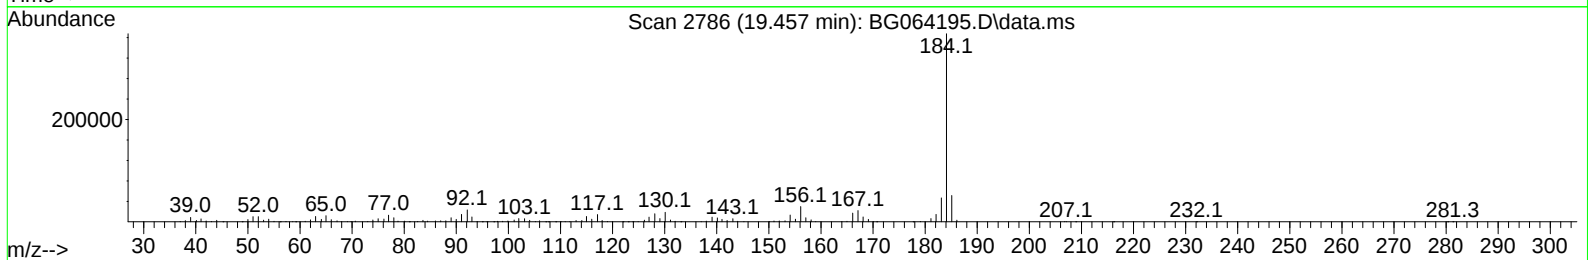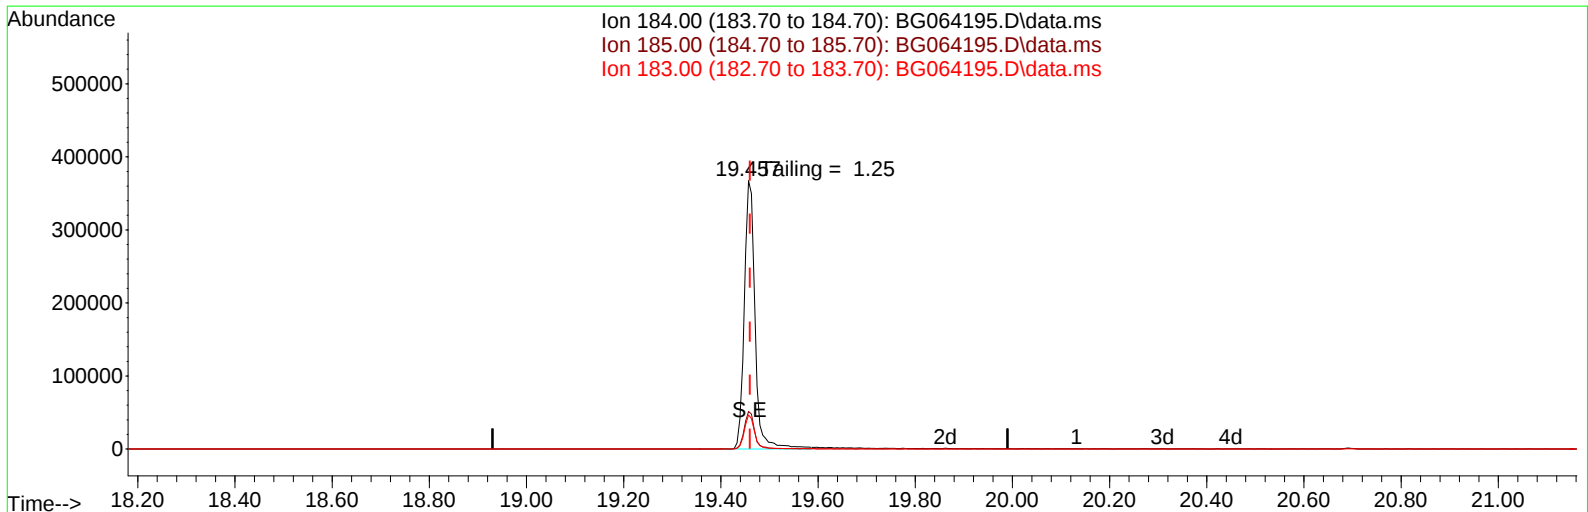

TIC: BG064195.D\data.ms

(77) Benzidine

19.457min (-0.003) 735829.89 ng m

response 591654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.01
183.00	12.20	12.69
0.00	0.00	0.00