
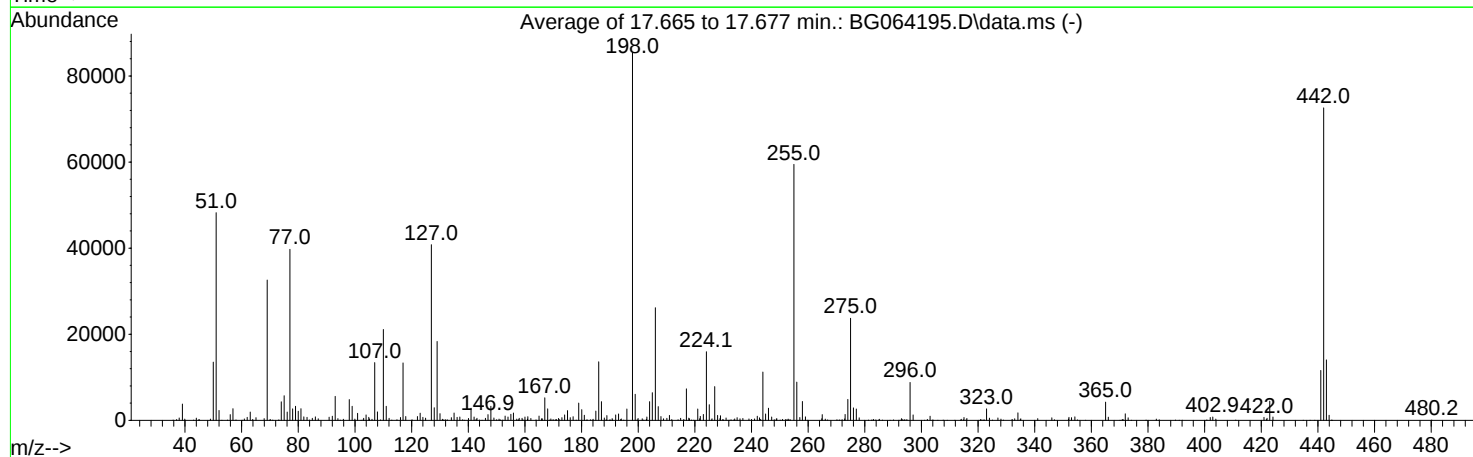


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040725\
Data File : BG064195.D
Acq On : 7 Apr 2025 8:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 07 17:00:17 2025

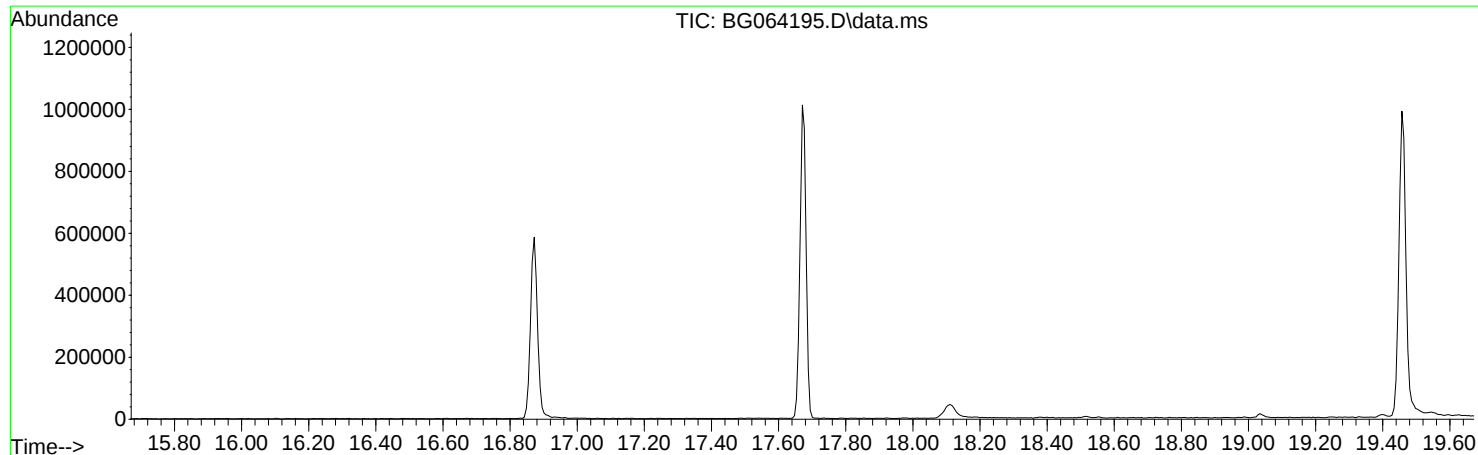




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	48243	PASS
68	69	0.00	2	1.2	401	PASS
69	198	0.00	100	38.2	32619	PASS
70	69	0.00	2	0.7	213	PASS
127	198	10	80	47.7	40797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85451	PASS
199	198	5	9	7.1	6057	PASS
275	198	10	60	27.7	23704	PASS
365	198	1	100	5.0	4236	PASS
441	198	0.01	100	13.6	11604	PASS
442	442	50	100	100.0	72592	PASS
443	442	15	24	19.4	14057	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040725\
Data File : BG064195.D
Acq On : 7 Apr 2025 8:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 07 17:00:17 2025
Response via : Initial Calibration

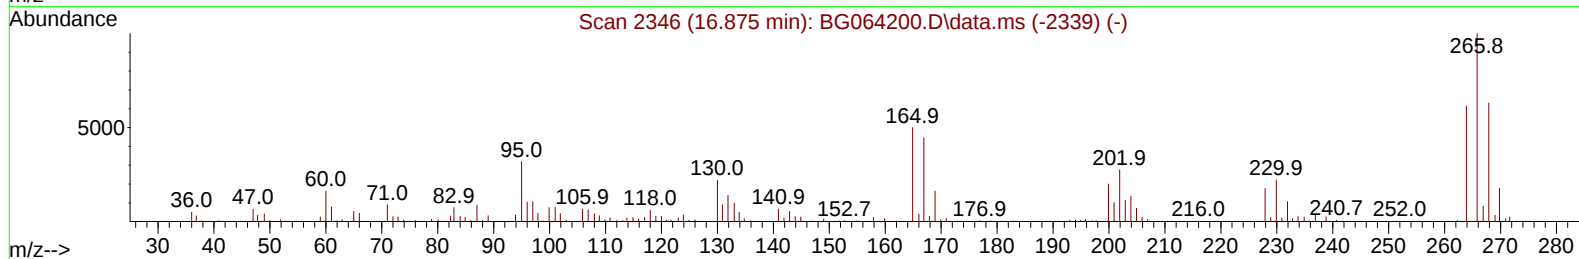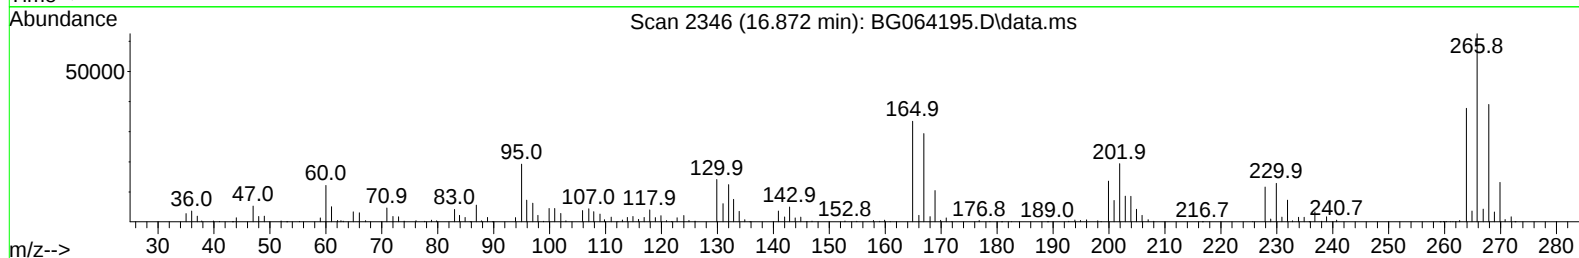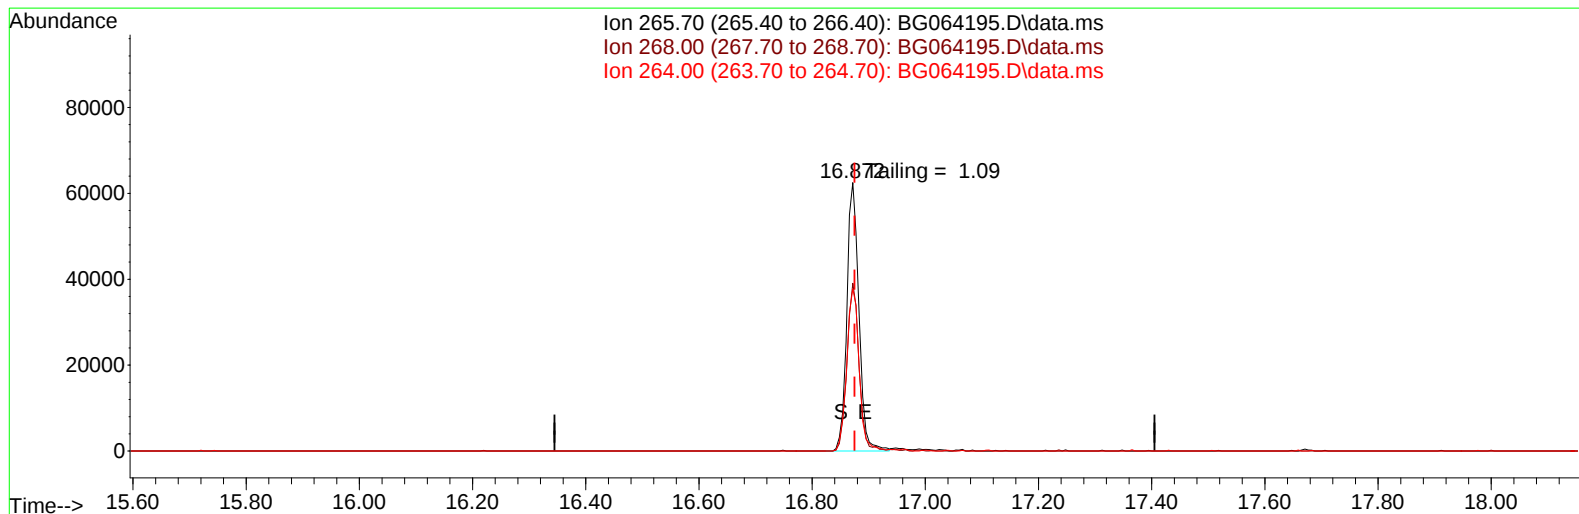

TIC: BG064195.D\data.ms

(70) Pentachlorophenol (C)

16.872min (-0.003) 15255.01 ng




response 92312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.47
264.00	61.40	60.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040725\
Data File : BG064195.D
Acq On : 7 Apr 2025 8:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 07 17:00:17 2025
Response via : Initial Calibration

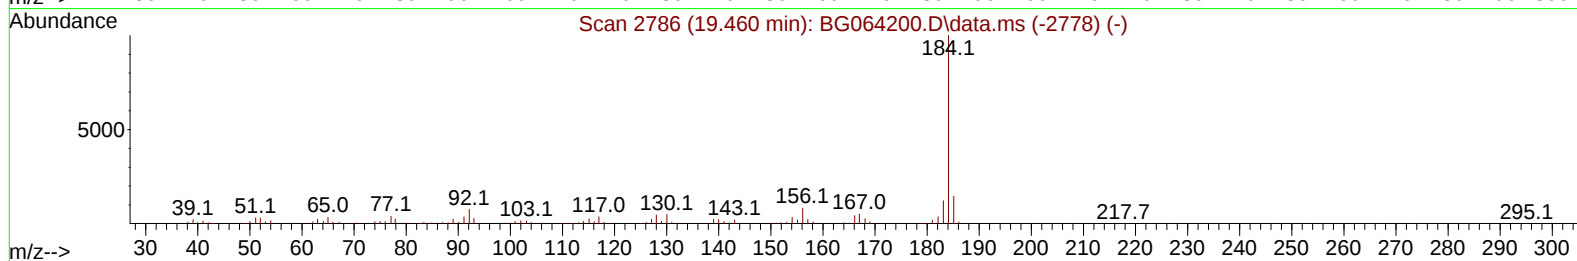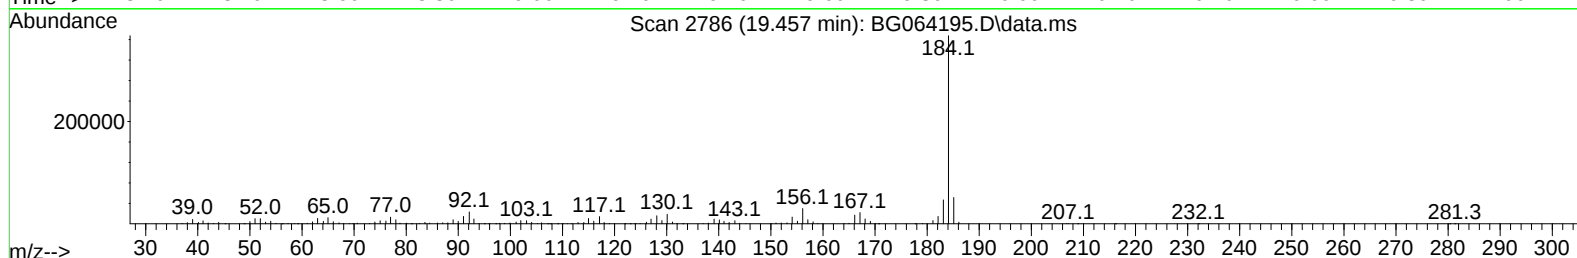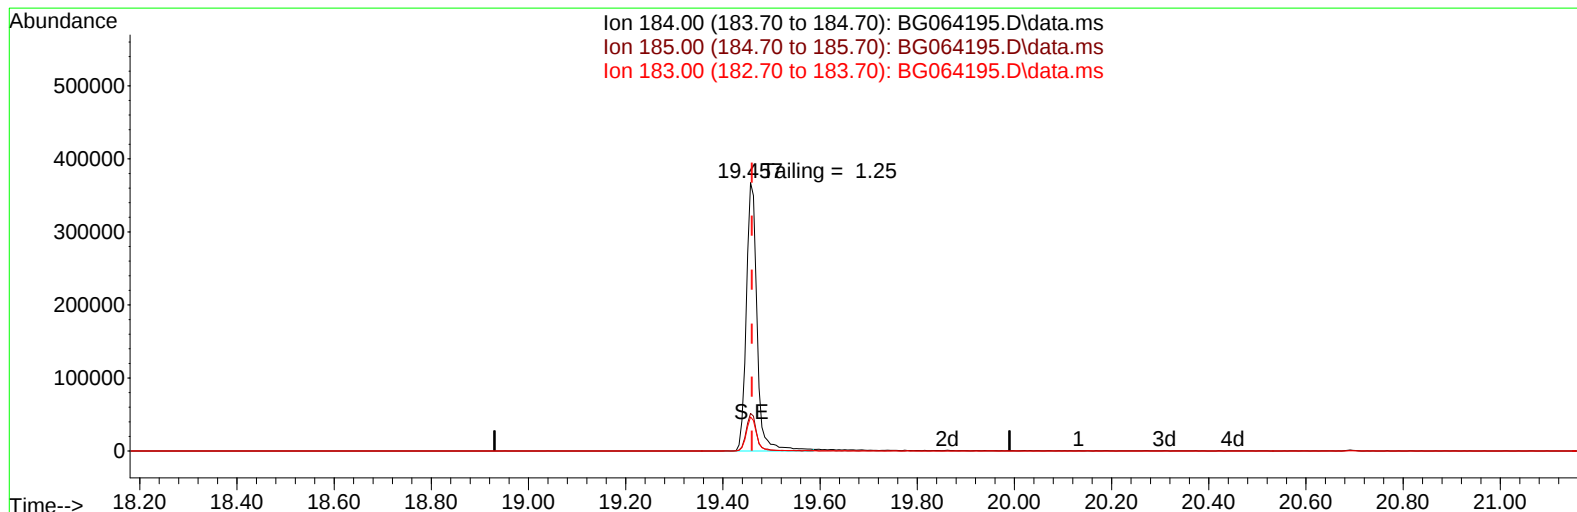

TIC: BG064195.D\data.ms

(77) Benzidine

19.457min (-0.003) 735829.89 ng m

response 591654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.01
183.00	12.20	12.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2025	BNA_G	<u>BG064195.D</u>
Compound Name	Response	Retention Time
DDT	271132	20.691
DDD	3245	20.303
DDE	0	19.753
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3245	274377	1.18

Instrument :
BNA_G
ClientSampleId :
DFTPP