
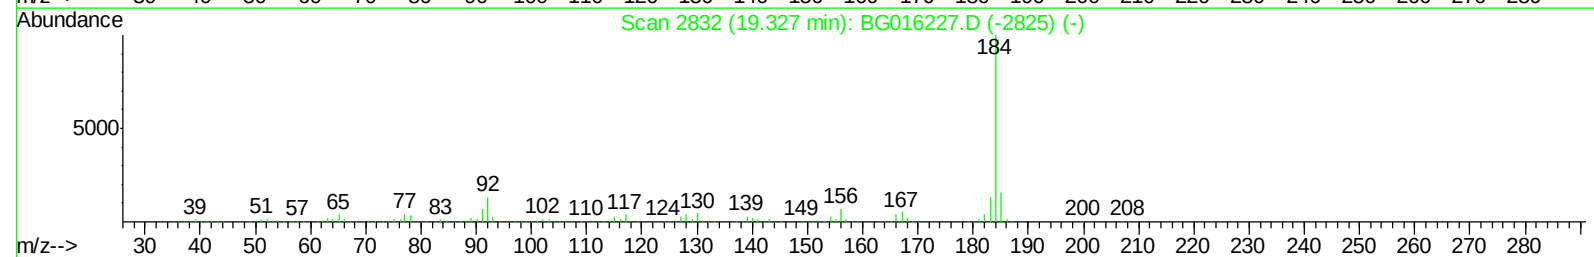
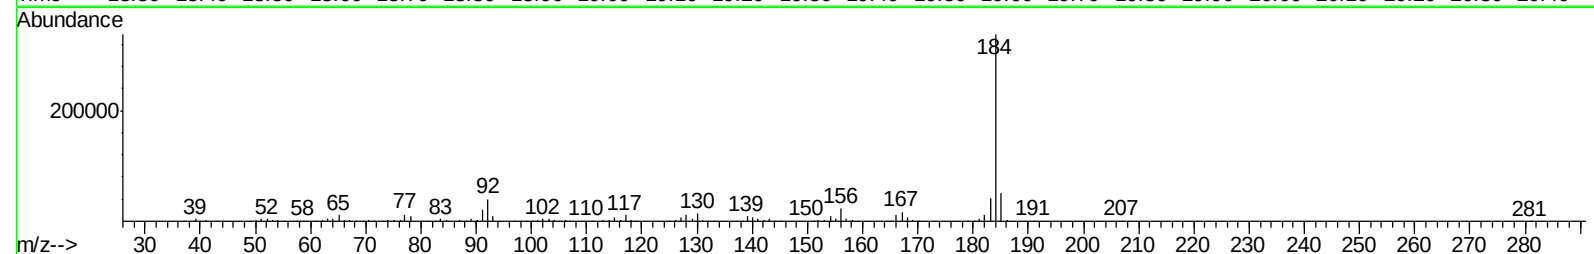



```
Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040815\  
Data File : BG016275.D  
Acq On    : 8 Apr 2015 11:03  
Operator  : TP/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Apr 09 08:06:49 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 02:28:50 2015
Response via : Initial Calibration

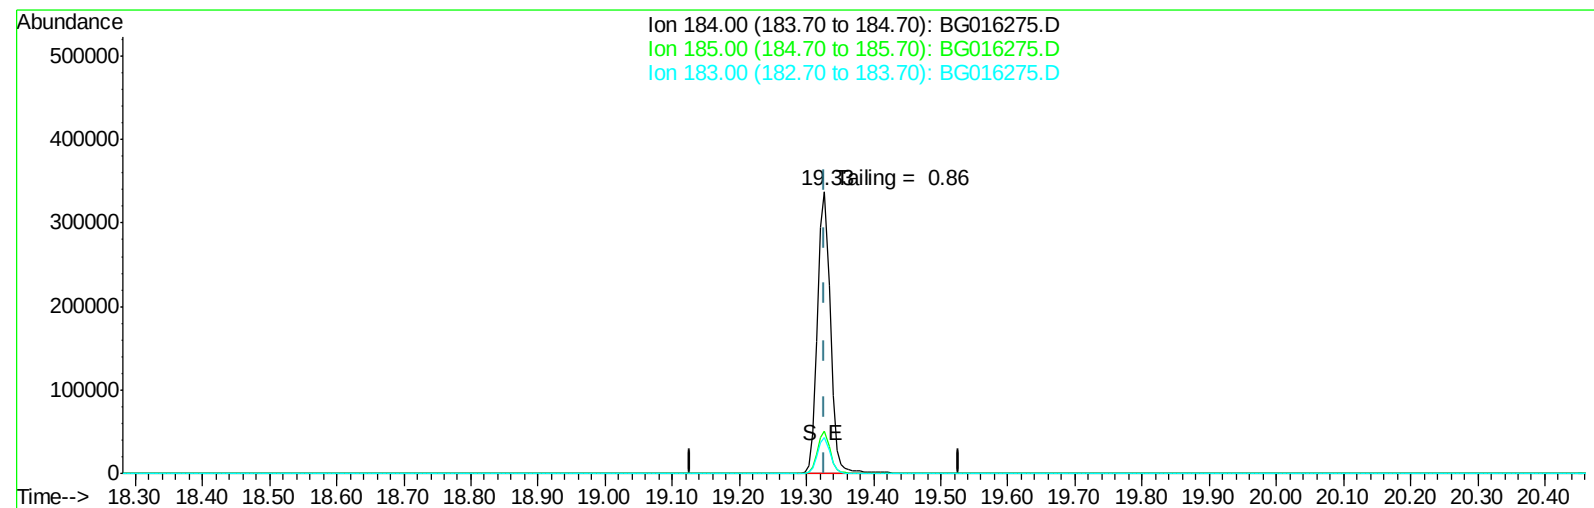

TIC: BG016275.D

(76) Benzidine

19.327min (-0.000) 161154.20ng

response 437384

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.80
183.00	13.00	12.62
0.00	0.00	0.00