
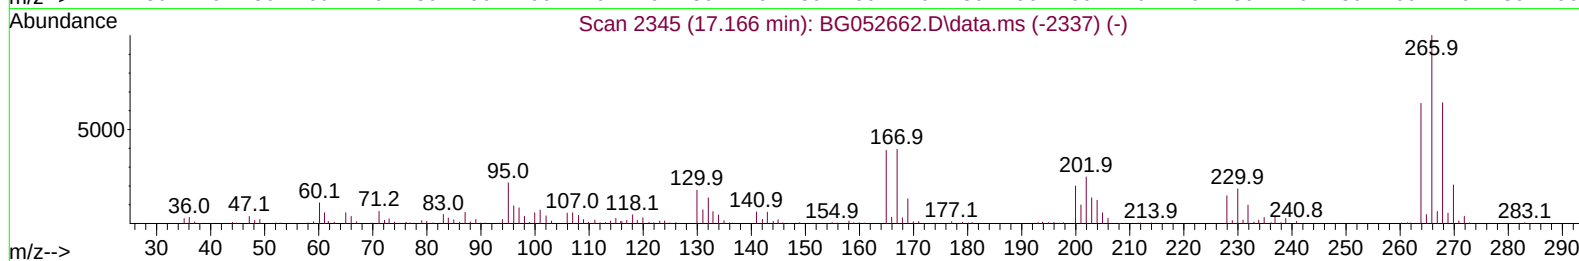
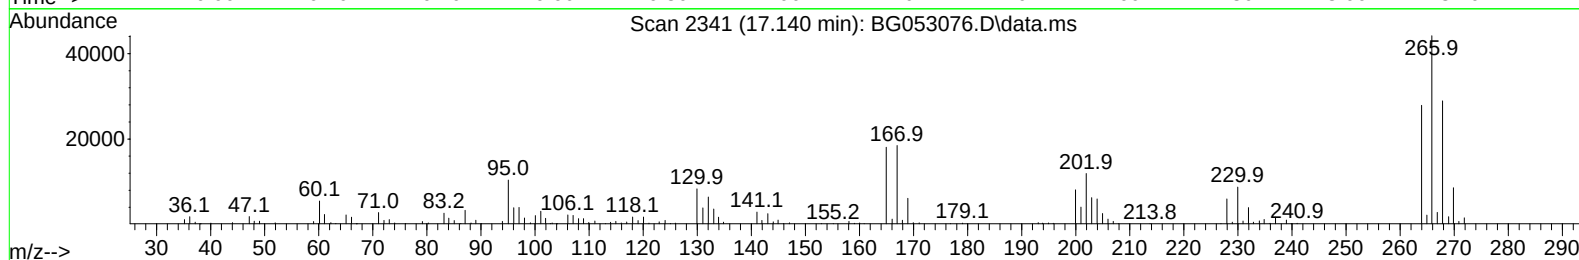


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
Data File : BG053076.D
Acq On : 8 Apr 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 14:52:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 14:49:00 2022
Response via : Initial Calibration

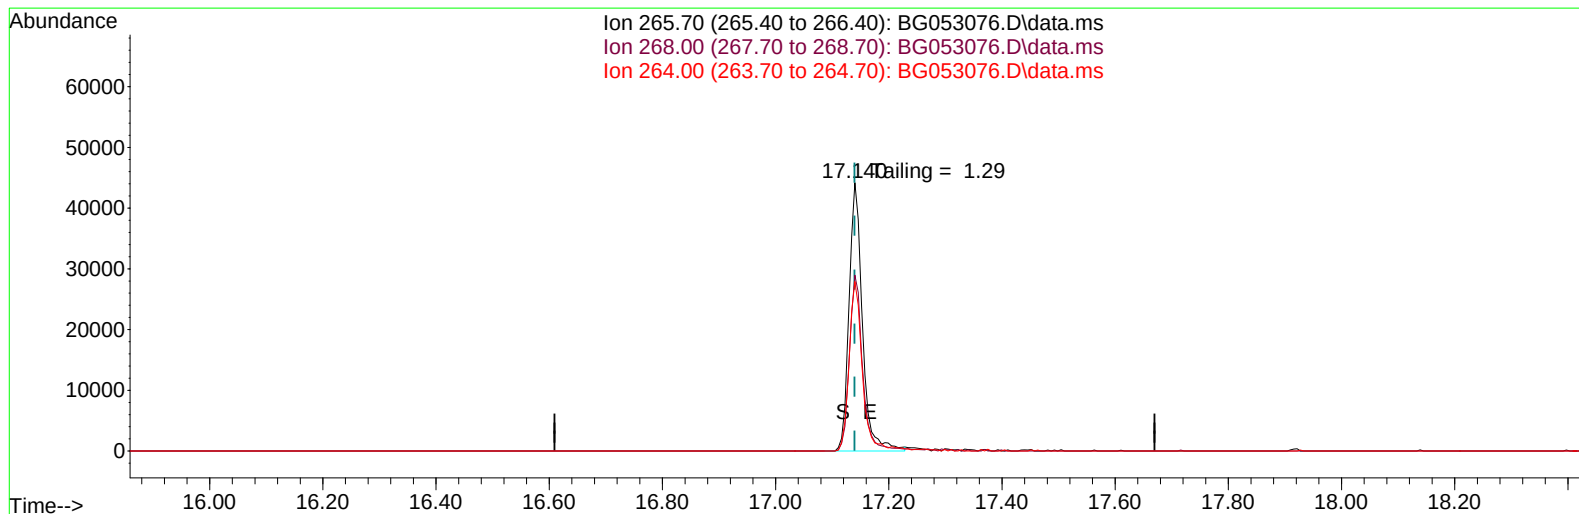

TIC: BG053076.D\data.ms

(70) Pentachlorophenol (C)




17.140min (+ 0.001) 20971.30 ng

response 72498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.52
264.00	56.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
 Data File : BG053076.D
 Acq On : 8 Apr 2022 9:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 14:52:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 14:49:00 2022
 Response via : Initial Calibration

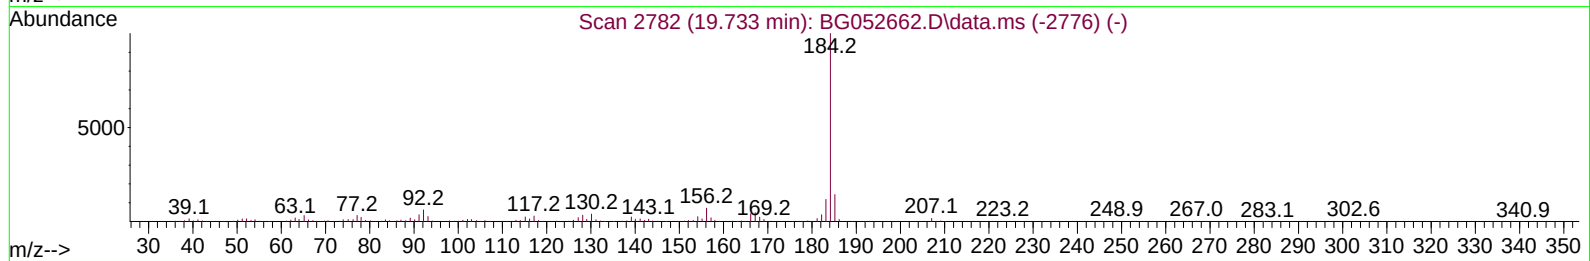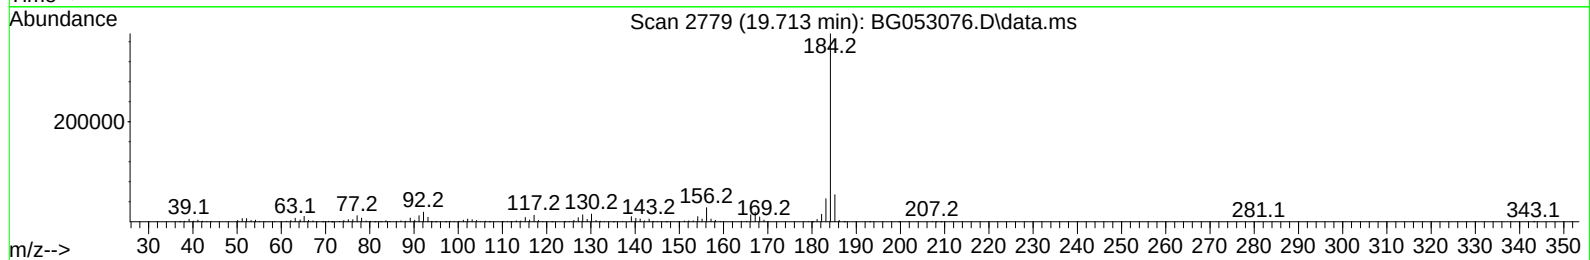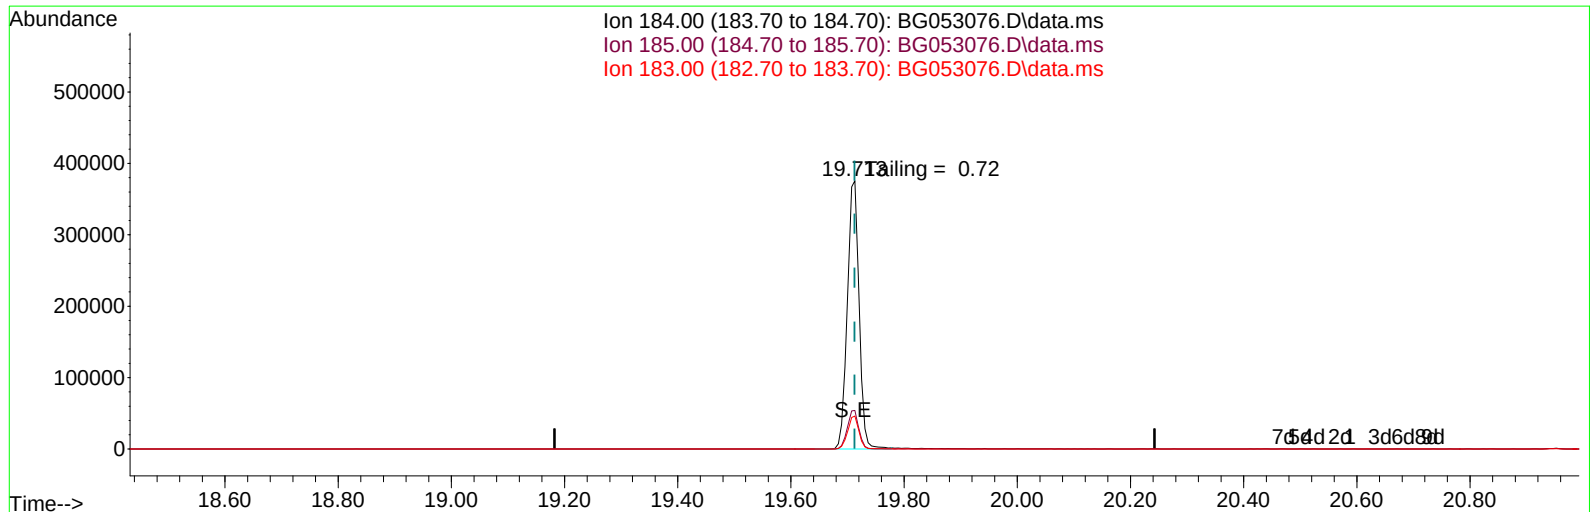

TIC: BG053076.D\data.ms

(77) Benzidine

19.713min (+ 0.001) 394926.44 ng m

response 550041

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	11.80	12.28
0.00	0.00	0.00