

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
 Data File : BG053089.D
 Acq On : 8 Apr 2022 18:20
 Operator : CG/JU
 Sample : PB143990BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143990BL

Quant Time: Apr 09 07:03:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.123	152	25934	20.000	ng	0.00
21) Naphthalene-d8	10.937	136	106183	20.000	ng	# 0.00
39) Acenaphthene-d10	14.743	164	79373	20.000	ng	0.00
64) Phenanthrene-d10	17.486	188	204079	20.000	ng	0.00
76) Chrysene-d12	21.769	240	240376	20.000	ng	0.00
86) Perylene-d12	25.070	264	237348	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.685	112	208046	137.514	ng	0.00
7) Phenol-d6	7.277	99	297178	127.377	ng	0.00
23) Nitrobenzene-d5	9.280	82	215721	82.490	ng	0.00
42) 2,4,6-Tribromophenol	16.229	330	159426	126.249	ng	0.00
45) 2-Fluorobiphenyl	13.368	172	477579	82.967	ng	0.00
79) Terphenyl-d14	20.089	244	1142012	80.239	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
Data File : BG053089.D
Acq On : 8 Apr 2022 18:20
Operator : CG/JU
Sample : PB143990BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143990BL


Quant Time: Apr 09 07:03:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

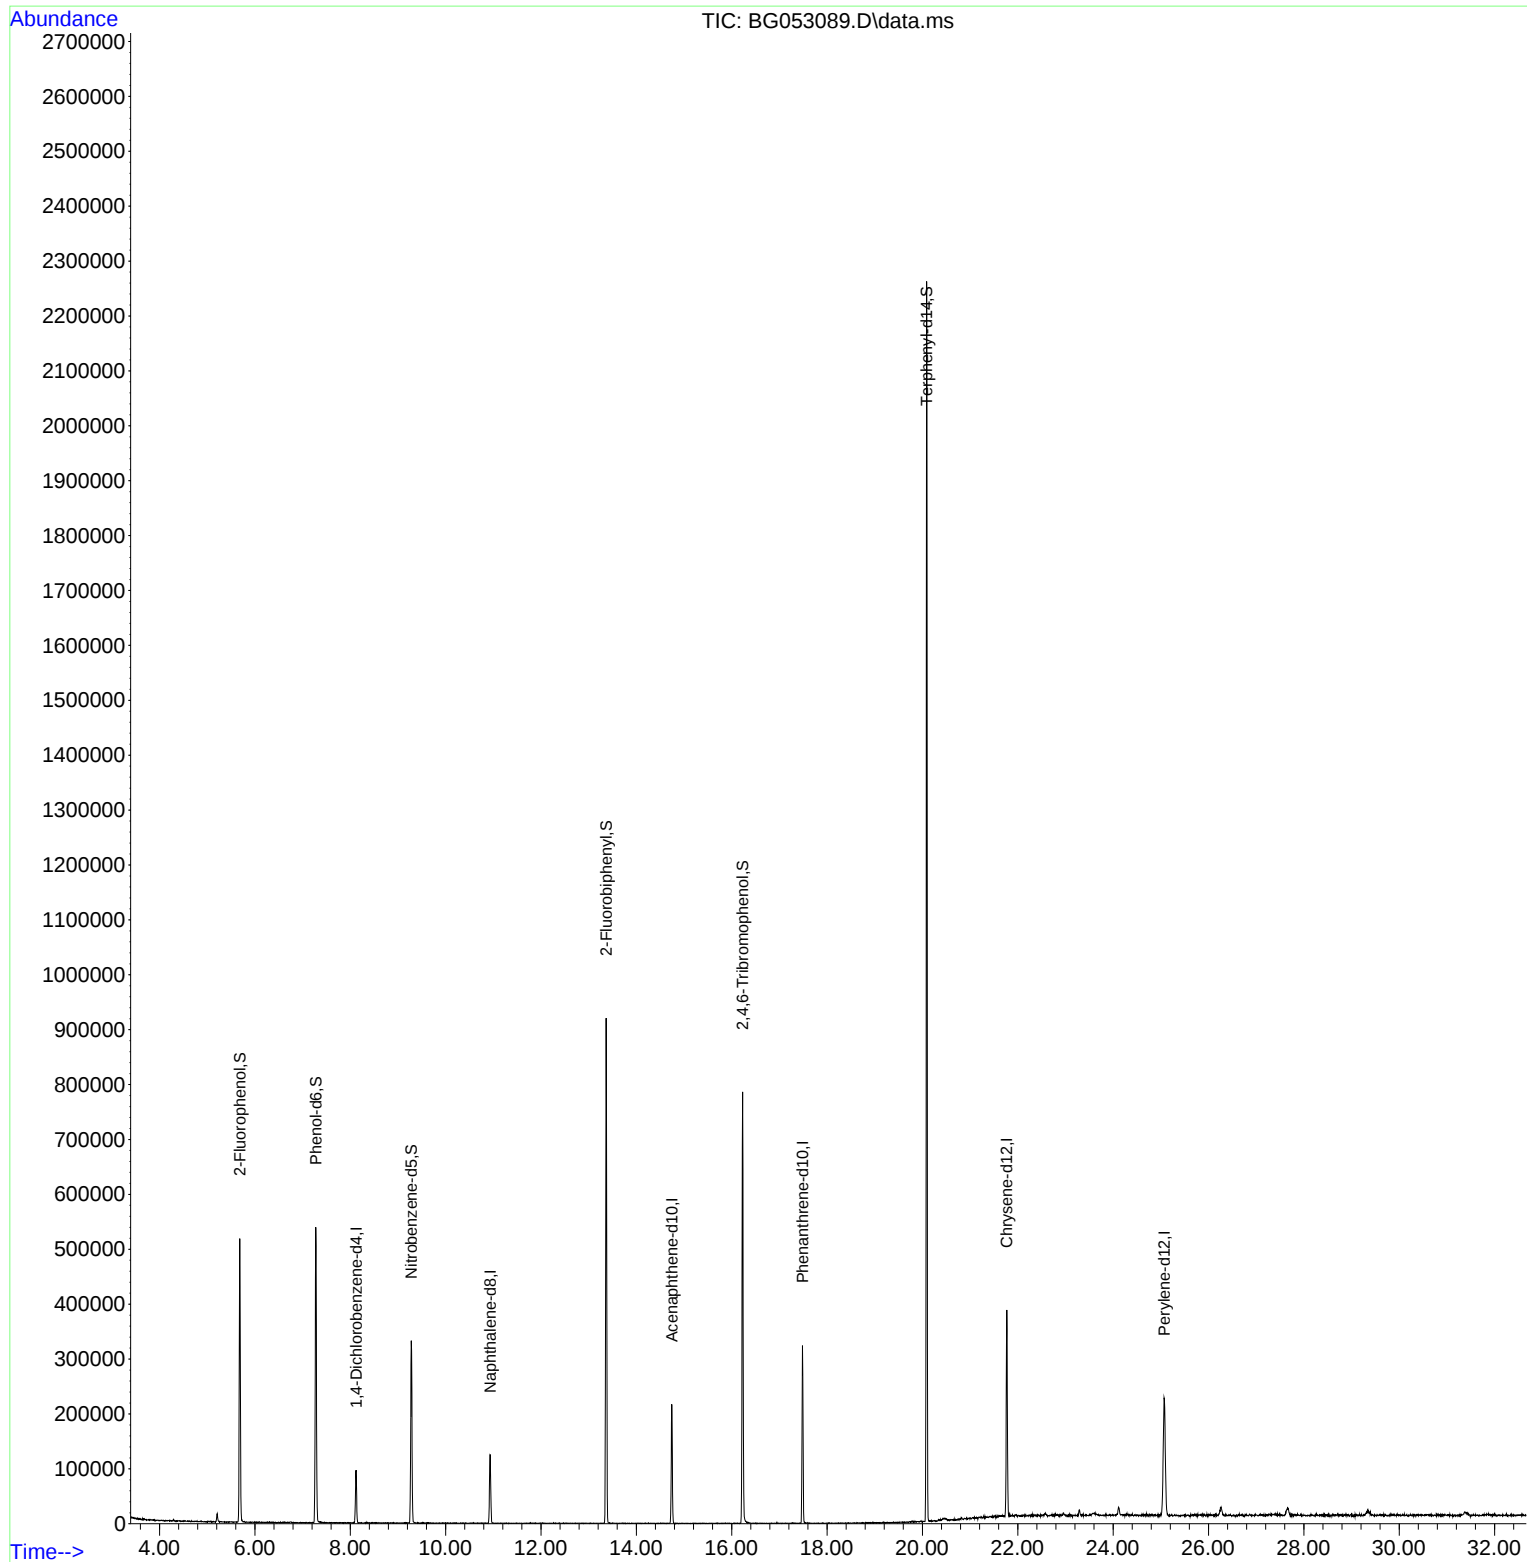






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.123 min Scan# 806
Delta R.T. 0.001 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20

Instrument :
BNA_G
ClientSampleId :
PB143990BL



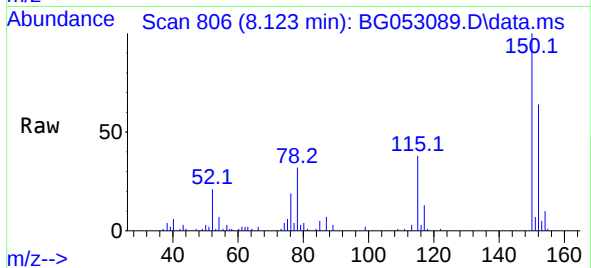



Tgt Ion:152 Resp: 25934
Ion Ratio Lower Upper
152 100
150 155.4 114.6 172.0
115 59.6 45.9 68.9

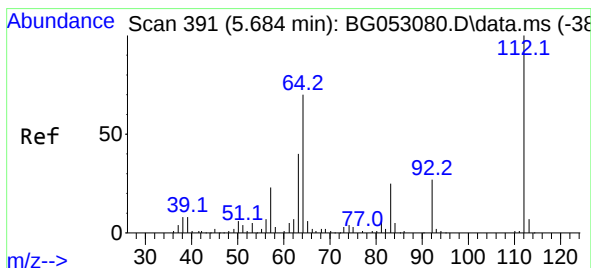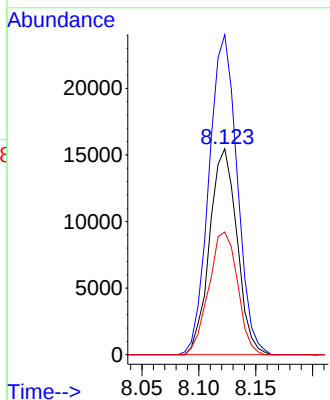

#5
2-Fluorophenol
Concen: 137.514 ng
RT: 5.685 min Scan# 391
Delta R.T. 0.001 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20

Tgt Ion:112 Resp: 208046
Ion Ratio Lower Upper
112 100
64 71.3 48.0 72.0
63 40.0 26.5 39.7#


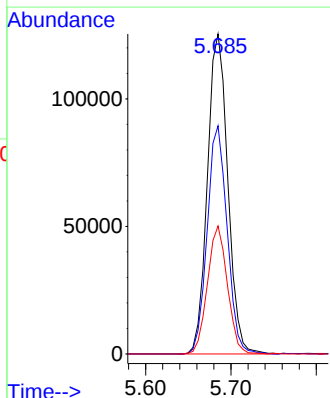
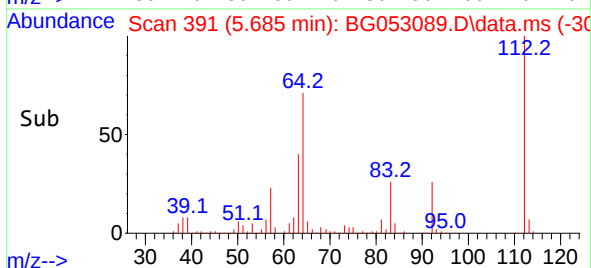
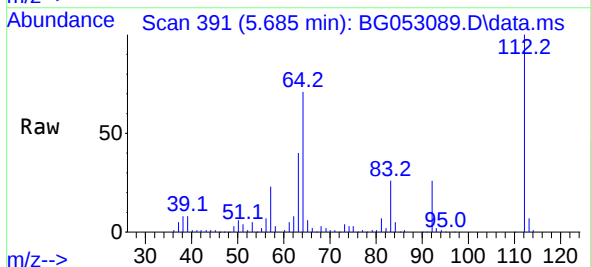




#7
Phenol-d6
Concen: 127.377 ng
RT: 7.277 min Scan# 60
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20




Instrument :
BNA_G
ClientSampleId :
PB143990BL


Tgt Ion: 99 Resp: 297178
Ion Ratio Lower Upper
99 100
42 20.3 14.7 22.1
71 43.5 29.2 43.8

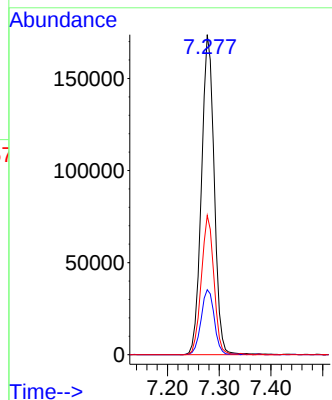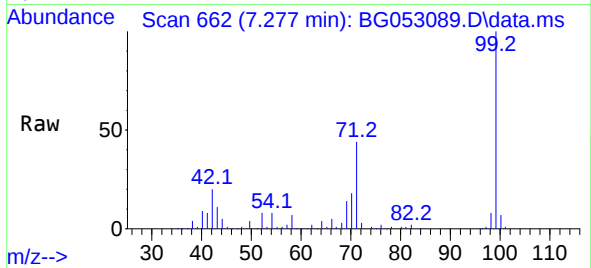

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.937 min Scan# 1285
Delta R.T. 0.001 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20

Tgt Ion: 136 Resp: 106183
Ion Ratio Lower Upper
136 100
137 12.4 9.4 14.2
54 9.3 6.4 9.6
68 4.2 5.0 7.6#


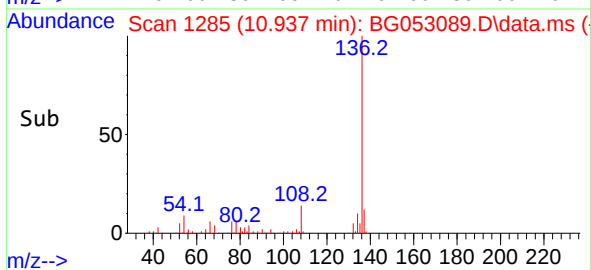
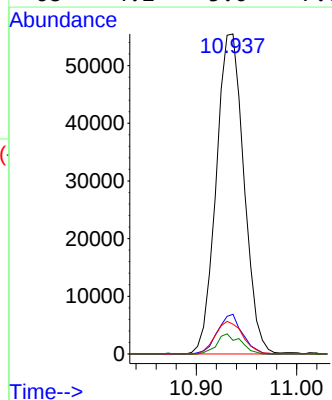
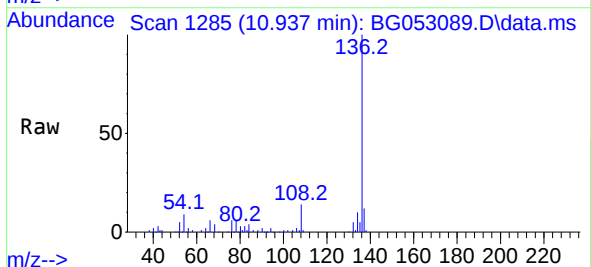




#23
Nitrobenzene-d5
Concen: 82.490 ng
RT: 9.280 min Scan# 10
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20




Instrument :
BNA_G
ClientSampleId :
PB143990BL


Tgt Ion: 82 Resp: 215721
Ion Ratio Lower Upper
82 100
128 34.8 31.3 46.9
54 49.4 37.8 56.8

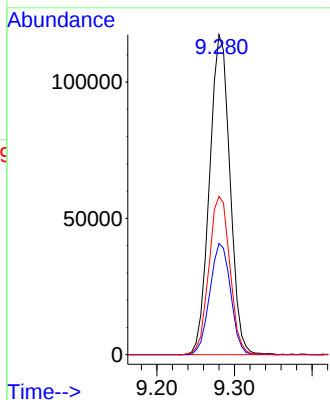

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.743 min Scan# 1933
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20


Tgt Ion:164 Resp: 79373
Ion Ratio Lower Upper
164 100
162 107.7 80.0 120.0
160 44.2 38.8 58.2

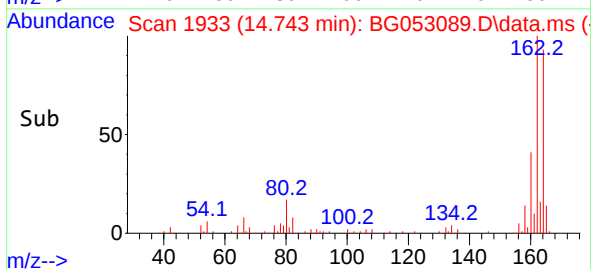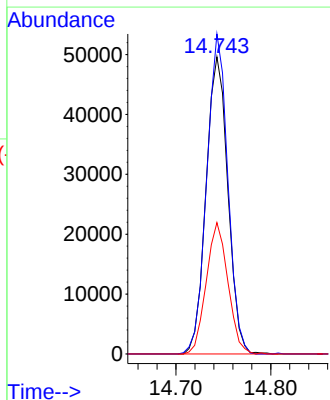






#42
2,4,6-Tribromophenol
Concen: 126.249 ng
RT: 16.229 min Scan# 2186
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20


Instrument :
BNA_G
ClientSampleId :
PB143990BL

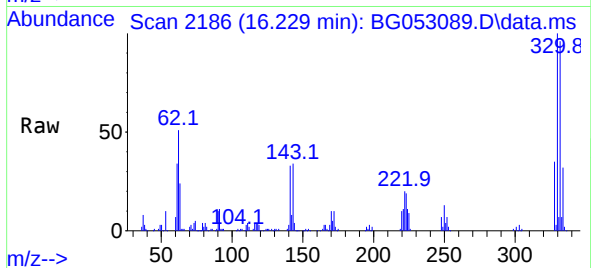



Tgt Ion:330 Resp: 159426
Ion Ratio Lower Upper
330 100
332 95.9 75.8 113.6
141 32.9 24.6 36.8

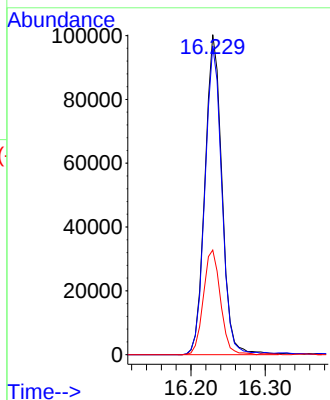


#45
2-Fluorobiphenyl
Concen: 82.967 ng
RT: 13.368 min Scan# 1699
Delta R.T. 0.001 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20




Tgt Ion:172 Resp: 477579
Ion Ratio Lower Upper
172 100
171 36.4 28.3 42.5
170 22.7 18.0 27.0

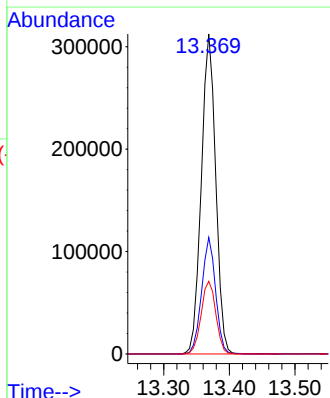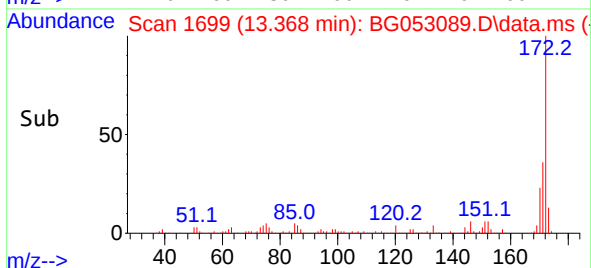






#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.486 min Scan# 2401
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20

Instrument :
BNA_G
ClientSampleId :
PB143990BL







Tgt Ion:188 Resp: 204079
Ion Ratio Lower Upper
188 100
94 6.9 5.7 8.5
80 8.0 7.2 10.8

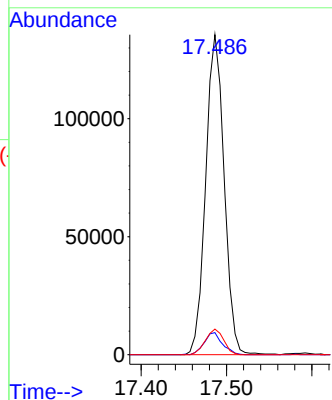

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.769 min Scan# 3129
Delta R.T. -0.005 min
Lab File: BG053089.D
Acq: 8 Apr 2022 18:20


Tgt Ion:240 Resp: 240376
Ion Ratio Lower Upper
240 100
120 6.6 5.4 8.0
236 25.1 19.8 29.6

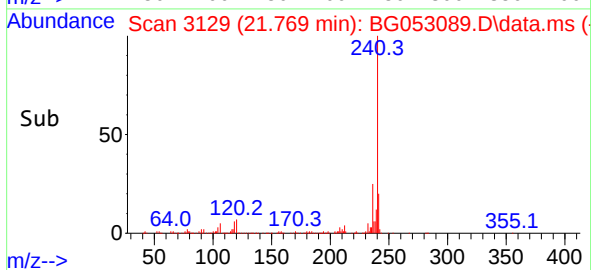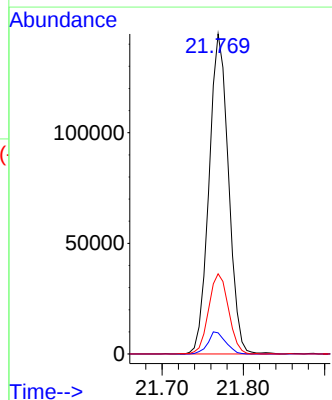






#79
 Terphenyl-d14
 Concen: 80.239 ng
 RT: 20.089 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BG053089.D
 Acq: 8 Apr 2022 18:20

Instrument :
 BNA_G
 ClientSampleId :
 PB143990BL

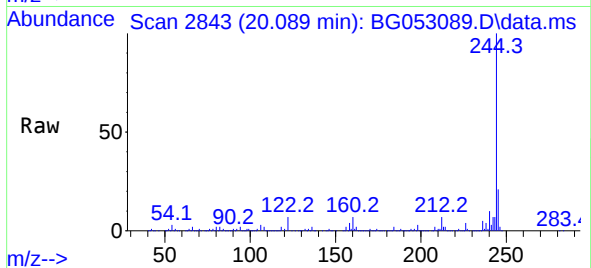

Tgt Ion:244 Resp: 1142012

Ion	Ratio	Lower	Upper
244	100		
212	7.5	5.4	8.2
122	6.9	5.8	8.6

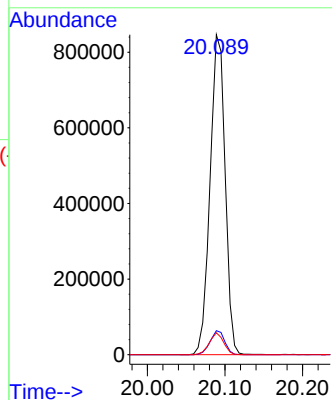

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.070 min Scan# 3691
 Delta R.T. -0.005 min
 Lab File: BG053089.D
 Acq: 8 Apr 2022 18:20

Tgt Ion:264 Resp: 237348

Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.2	27.2
265	22.3	15.1	22.7

