


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
 Data File : BG053076.D
 Acq On : 8 Apr 2022 9:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

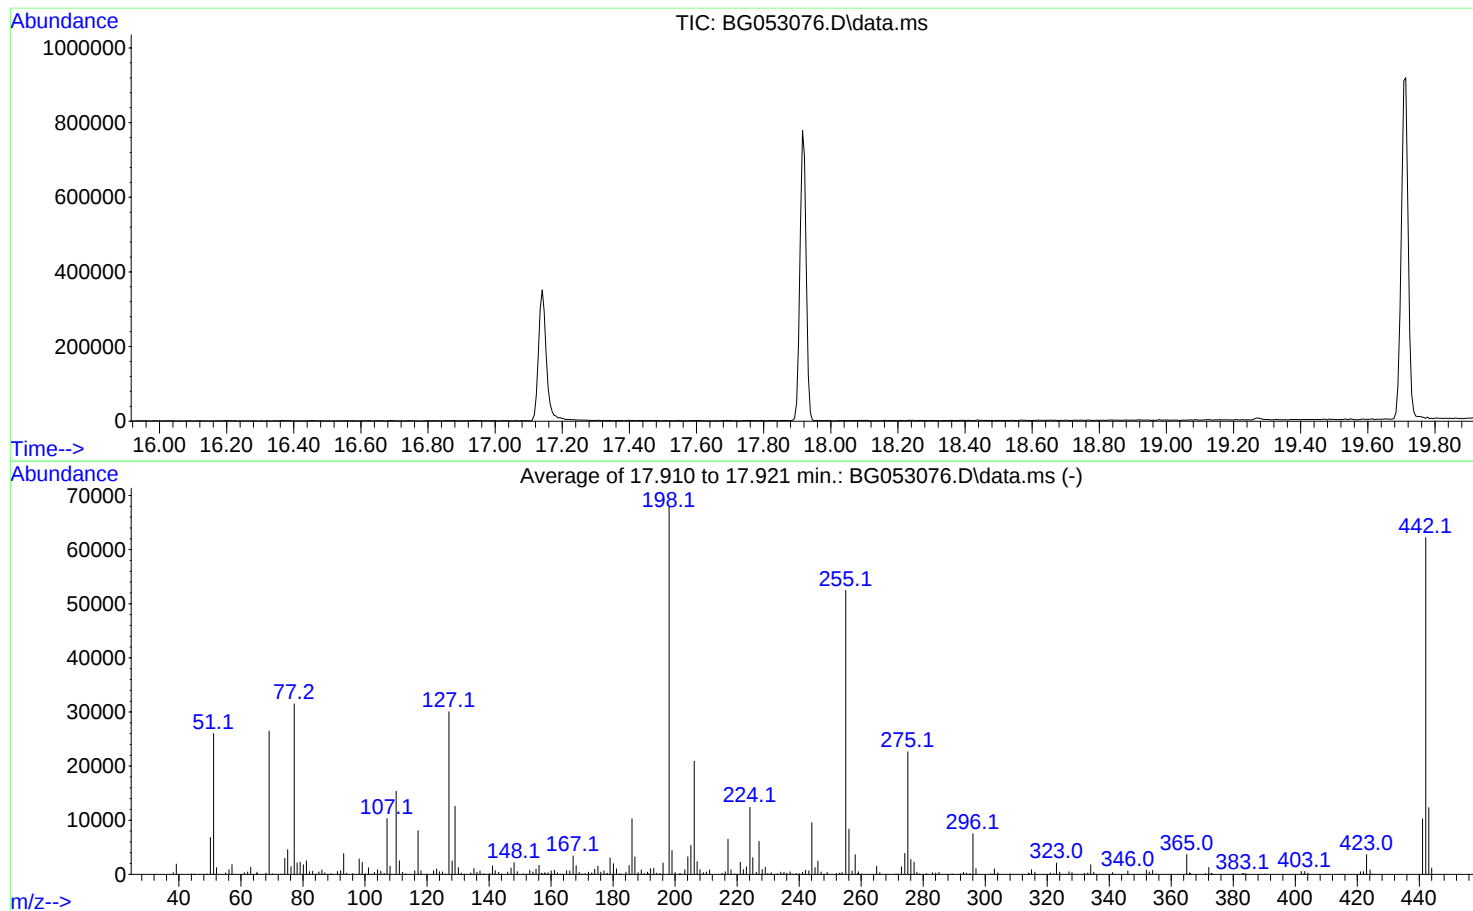




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	26011	PASS
68	69	0.00	2	0.9	233	PASS
69	198	0.00	100	38.9	26461	PASS
70	69	0.00	2	0.4	113	PASS
127	198	10	80	44.2	30032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67963	PASS
199	198	5	9	6.5	4421	PASS
275	198	10	60	33.3	22634	PASS
365	198	1	100	5.4	3662	PASS
441	198	0.01	100	15.1	10262	PASS
442	442	50	100	100.0	62224	PASS
443	442	15	24	19.8	12337	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
Data File : BG053076.D
Acq On : 8 Apr 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 08 14:52:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 14:49:00 2022
Response via : Initial Calibration

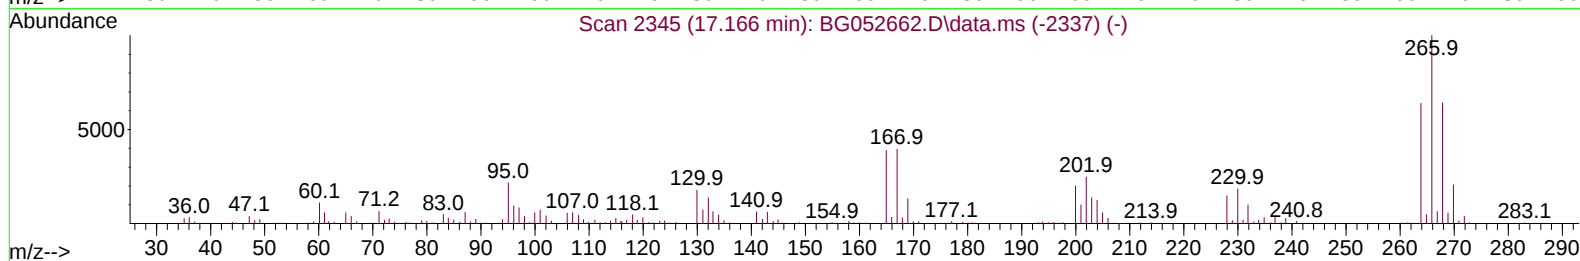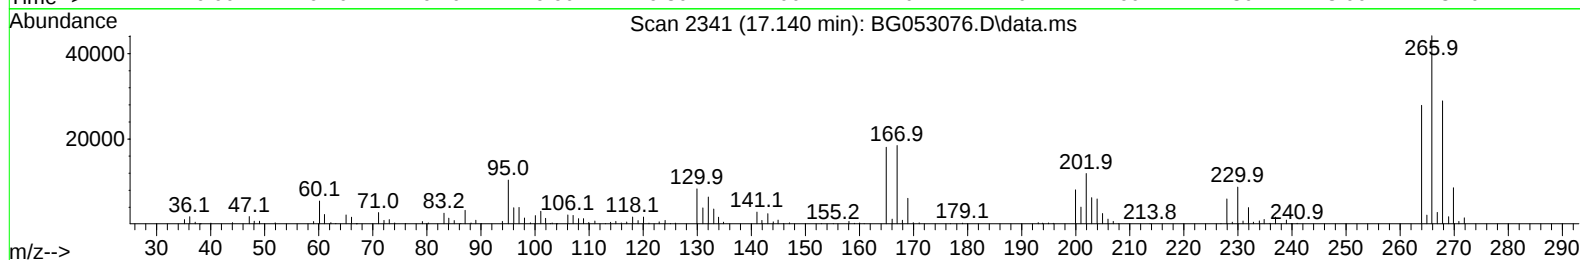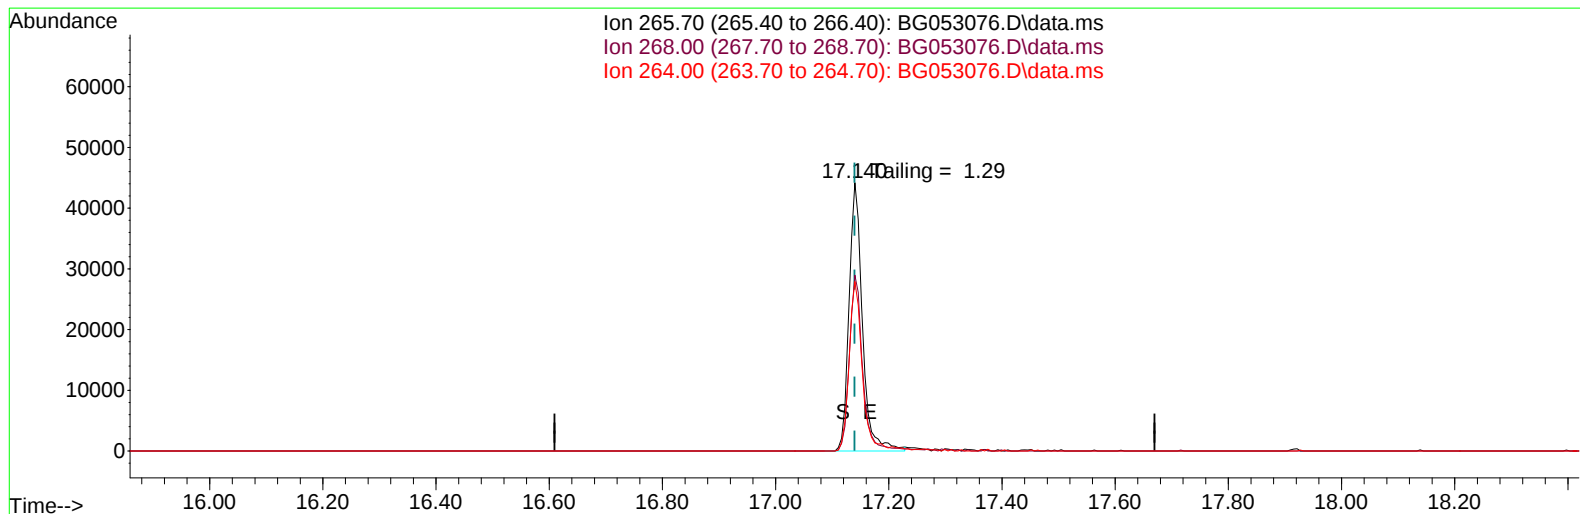

TIC: BG053076.D\data.ms

(70) Pentachlorophenol (C)

17.140min (+ 0.001) 20971.30 ng




response 72498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.52
264.00	56.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040822\
 Data File : BG053076.D
 Acq On : 8 Apr 2022 9:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 14:52:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 14:49:00 2022
 Response via : Initial Calibration

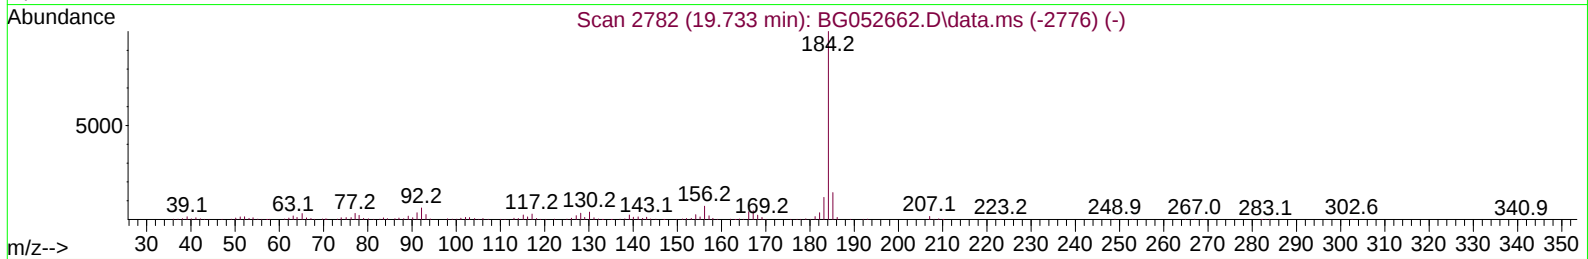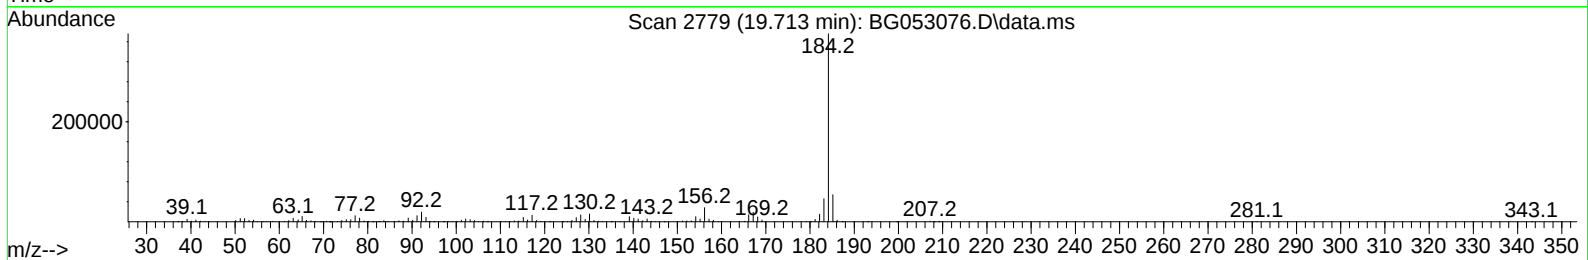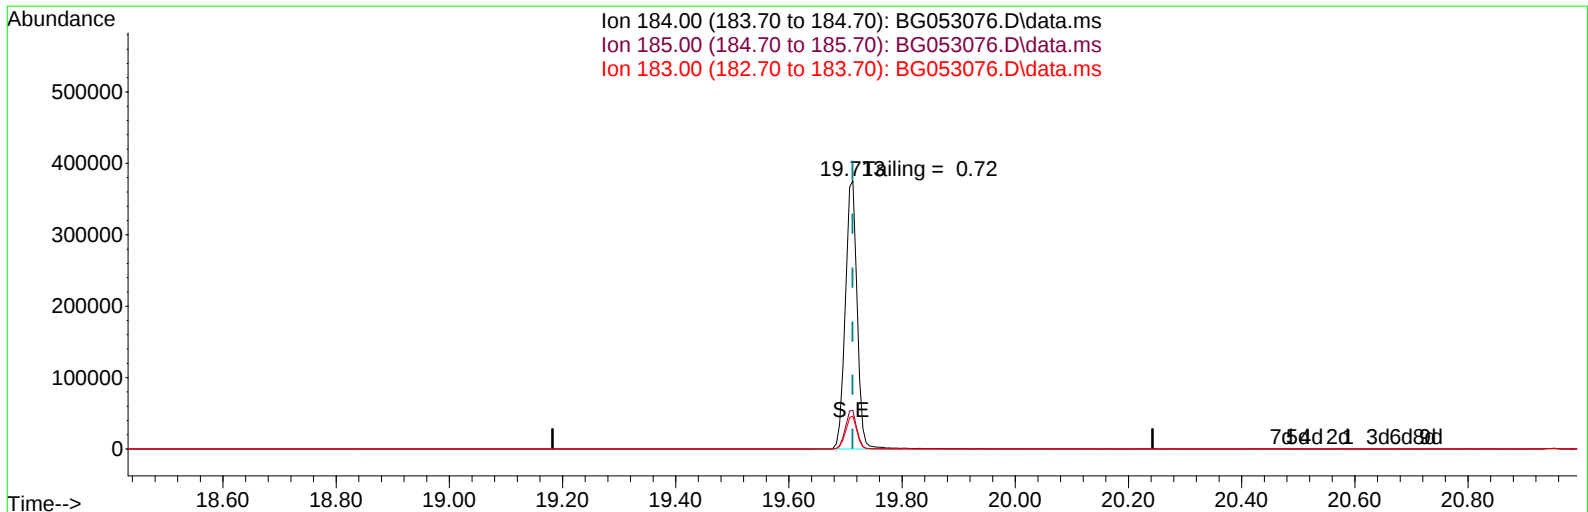

TIC: BG053076.D\data.ms

(77) Benzidine

19.713min (+ 0.001) 394926.44 ng m

response 550041

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	11.80	12.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2022	BNA_G	<u>BG053076.D</u>
Compound Name	Response	Retention Time
DDT	269000	20.94
DDD	564	20.5
DDE	56	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
620	269620	0.23