
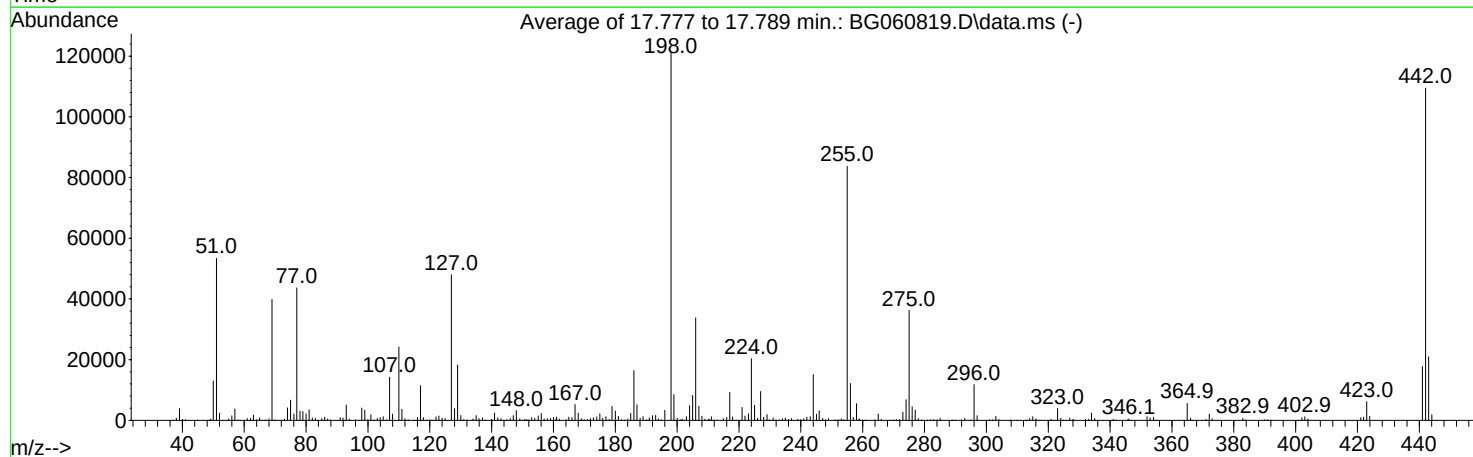


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040824\  
Data File : BG060819.D  
Acq On : 8 Apr 2024 10:23  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG032924.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Mar 30 03:12:26 2024

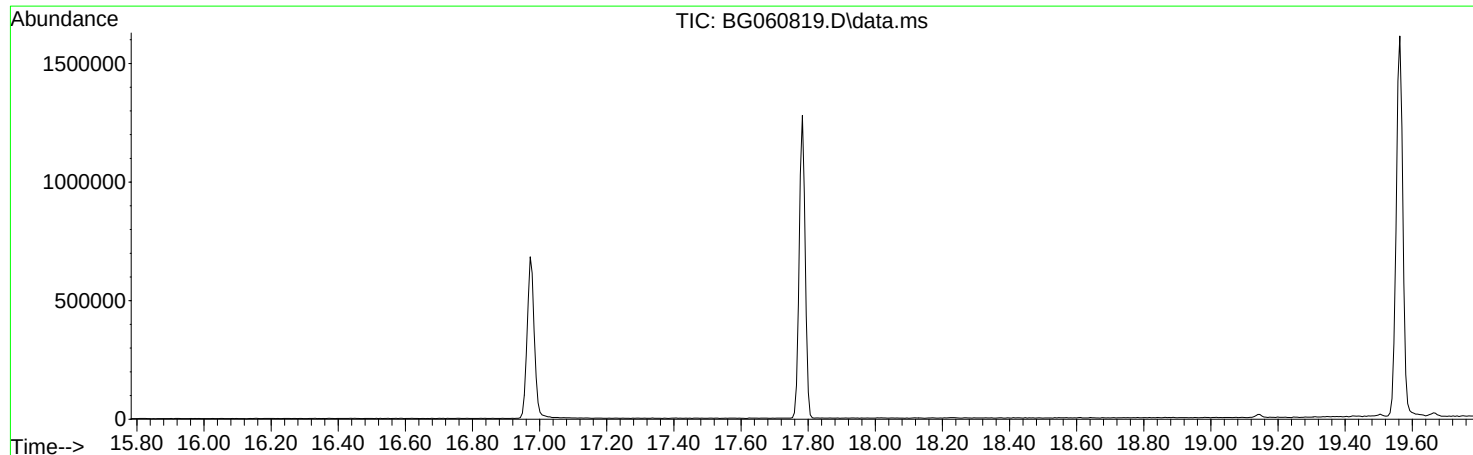

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 51     | 198     | 10     | 80     | 44.0  | 53360  | PASS      |
| 68     | 69      | 0.00   | 2      | 1.3   | 518    | PASS      |
| 69     | 198     | 0.00   | 100    | 32.9  | 39877  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 214    | PASS      |
| 127    | 198     | 10     | 80     | 39.6  | 47973  | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 121197 | PASS      |
| 199    | 198     | 5      | 9      | 7.0   | 8470   | PASS      |
| 275    | 198     | 10     | 60     | 29.9  | 36195  | PASS      |
| 365    | 198     | 1      | 100    | 4.6   | 5588   | PASS      |
| 441    | 198     | 0.01   | 100    | 14.6  | 17697  | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 109445 | PASS      |
| 443    | 442     | 15     | 24     | 19.1  | 20926  | PASS      |