

Data Path : Z:\HPCHEM1\BNA_G\Data\BG040915\
 Data File : BG016299.D
 Acq On : 9 Apr 2015 20:51
 Operator : TP/IZ
 Sample : PB82381BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB82381BS

Quant Time: Apr 10 03:13:24 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\625-TERPINEOL-BG040915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 09 19:35:19 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	87752	20.00	ng	0.00
4) Naphthalene-d8	10.48	136	427043	20.00	ng	0.00
7) Acenaphthene-d10	14.34	164	255348	20.00	ng	0.00
10) Phenanthrene-d10	17.08	188	530694	20.00	ng	0.00
11) Chrysene-d12	21.26	240	449160	20.00	ng	0.00
13) Perylene-d12	23.50	264	425686	20.00	ng	0.00
System Monitoring Compounds						
2) 2-Fluorophenol	5.29	112	474729	84.39	ng	0.00
3) Phenol-d6	6.89	99	696469	80.29	ng	0.00
5) Nitrobenzene-d5	8.86	82	461294	75.75	ng	0.00
8) 2,4,6-Tribromophenol	15.83	330	148033	96.76	ng	0.00
9) 2-Fluorobiphenyl	12.96	172	986368	75.08	ng	0.00
12) Terphenyl-d14	19.70	244	1205518	73.90	ng	0.00
Target Compounds						
6) Terpineol	10.37	59	1275	2.58	ng	Qvalue # 39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG040915\
Data File : BG016299.D
Acq On : 9 Apr 2015 20:51
Operator : TP/IZ
Sample : PB82381BS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82381BS

Quant Time: Apr 10 03:13:24 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\625-TERPINEOL-BG040915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 19:35:19 2015
Response via : Initial Calibration

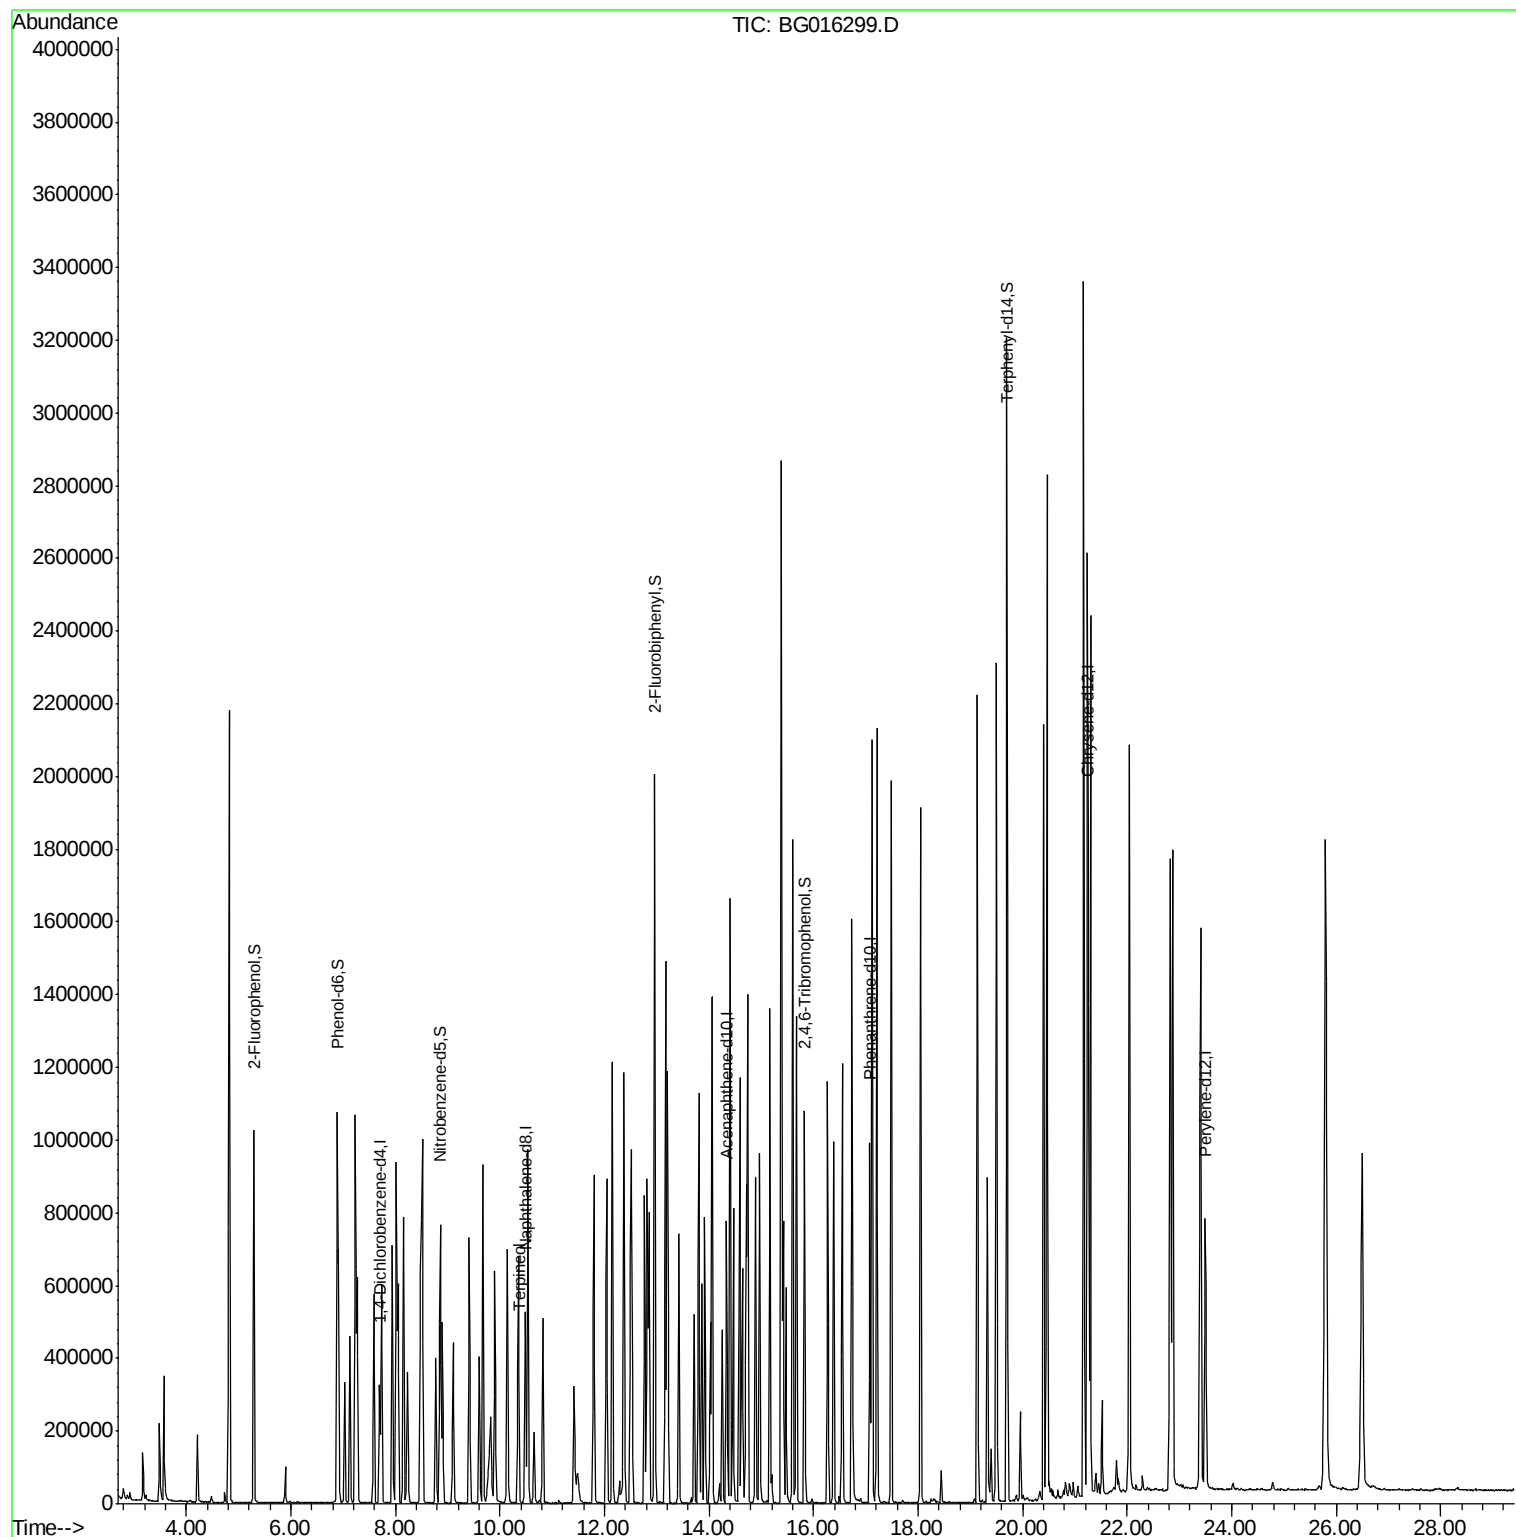

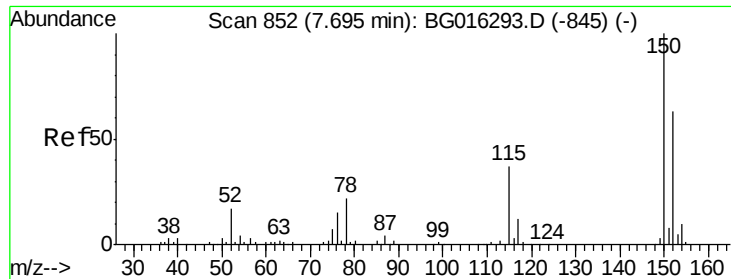

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.70 min Scan# 853

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion:152 Resp: 87752

Ion Ratio Lower Upper

152 100

150 157.5 139.4 209.0




115 57.5 44.6 67.0

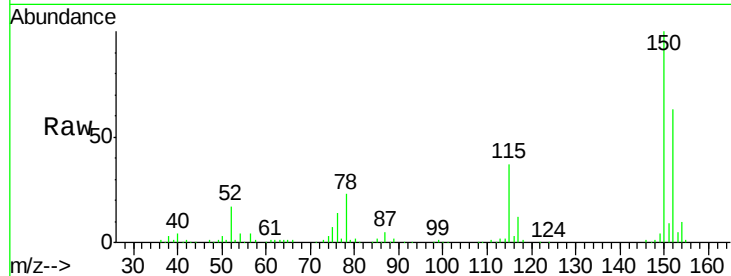

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

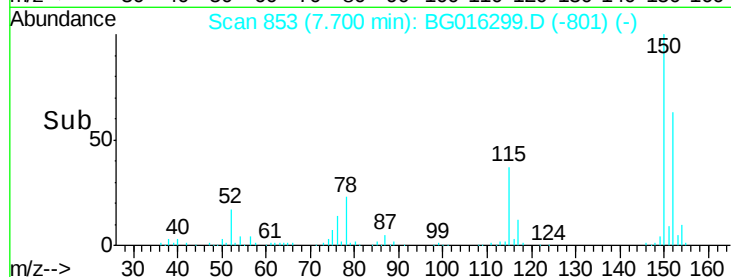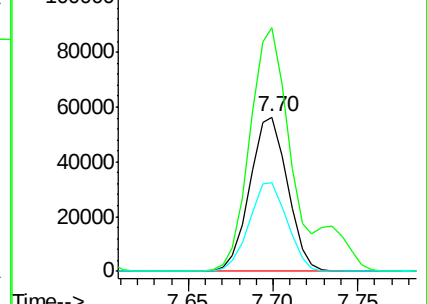

#2

2-Fluorophenol

Concen: 84.39 ng

RT: 5.29 min Scan# 443

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51


Tgt Ion:112 Resp: 474729

Ion Ratio Lower Upper

112 100

64 51.6 38.3 57.5



63 24.6 24.2 36.4




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

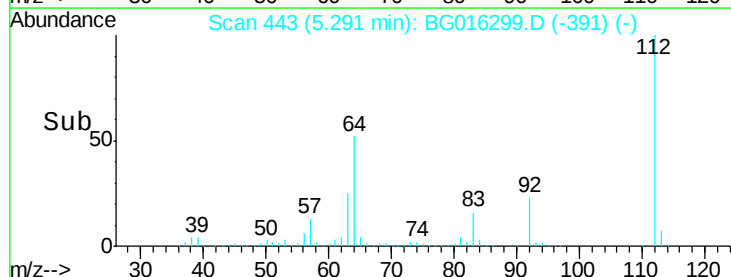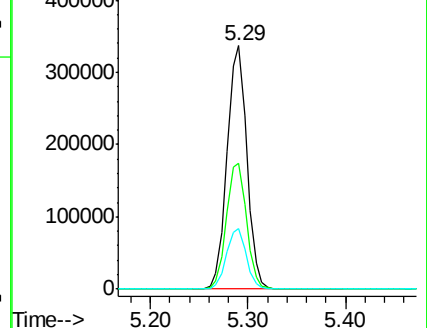

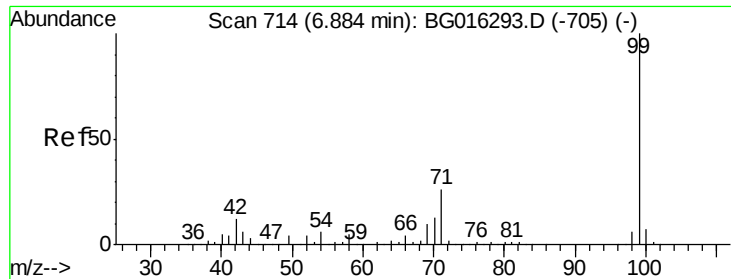

#3

Phenol-d6

Concen: 80.29 ng

RT: 6.89 min Scan# 715

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion: 99 Resp: 696469

Ion Ratio Lower Upper




99 100

42 12.6 16.5 24.7#

71 25.8 40.0 60.0#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

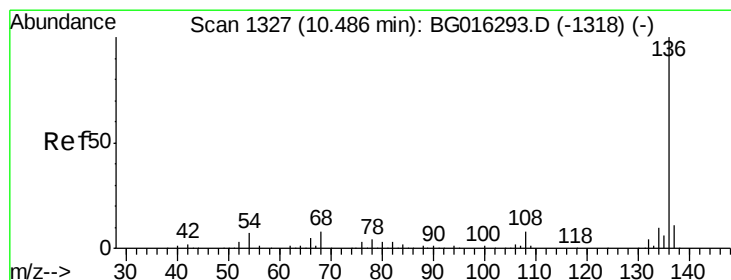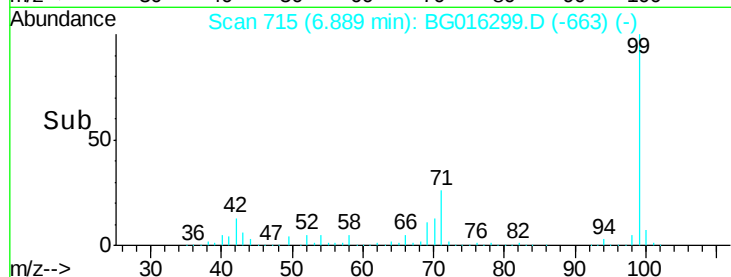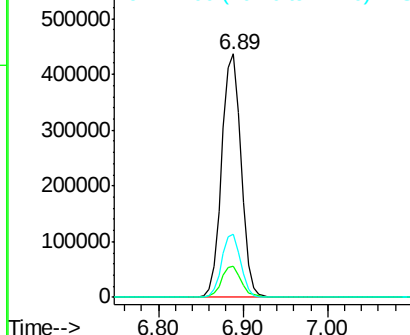

#4

Naphthalene-d8

Concen: 20.00 ng

RT: 10.48 min Scan# 1327

Delta R.T. -0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Tgt Ion: 136 Resp: 427043


Ion Ratio Lower Upper

136 100



137 11.3 9.7 14.5


54 7.4 3.2 4.8#

68 7.4 1.6 2.4#



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

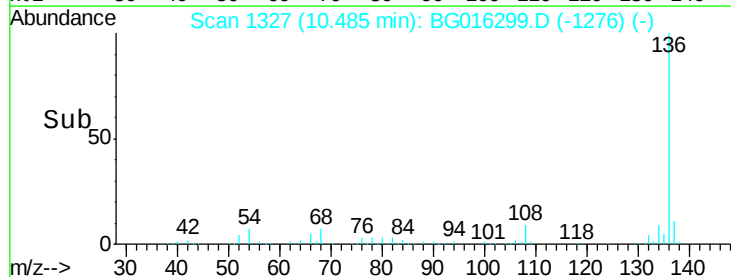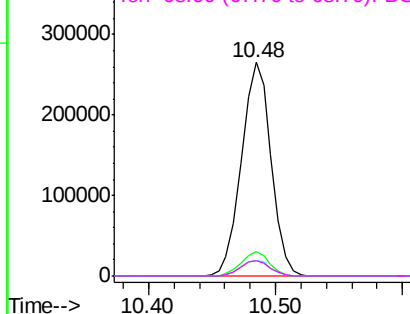

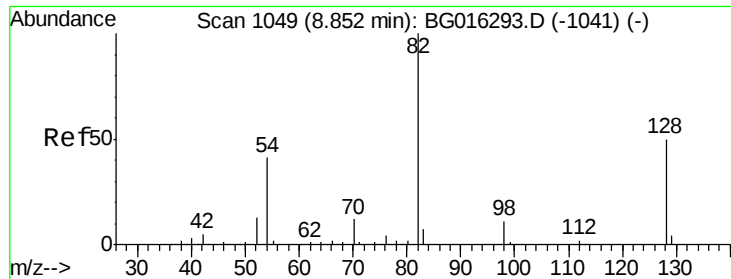

#5

Nitrobenzene-d5

Concen: 75.75 ng

RT: 8.86 min Scan# 1050

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion: 82 Resp: 461294

Ion Ratio Lower Upper




82 100

128 52.5 37.5 56.3

54 40.5 41.0 61.4#

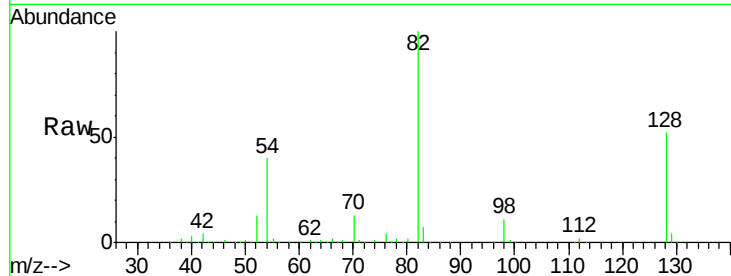

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

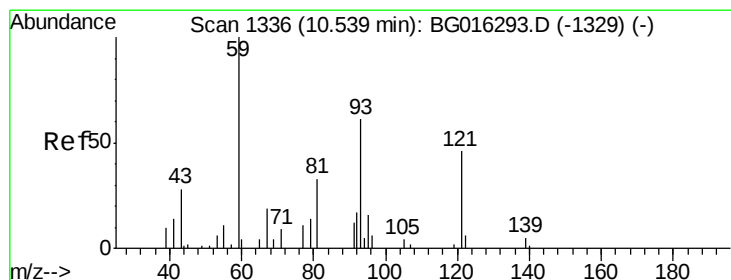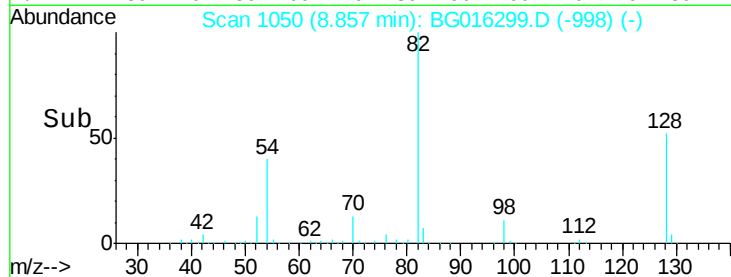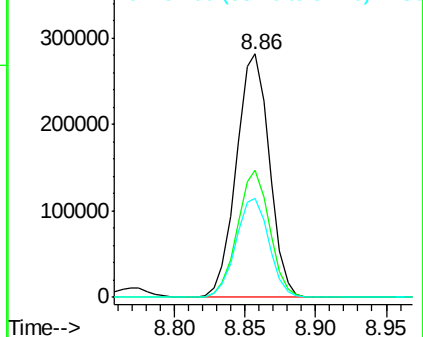

#6

Terpineol

Concen: 2.58 ng

RT: 10.37 min Scan# 1307

Delta R.T. -0.17 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51


Tgt Ion: 59 Resp: 1275

Ion Ratio Lower Upper



59 100


93 0.0 66.9 100.3#

121 60.9 72.0 108.0#



Abundance Ion 59.00 (58.70 to 59.70): BGC
Ion 93.00 (92.70 to 93.70): BGC
Ion 121.00 (120.70 to 121.70): BGC

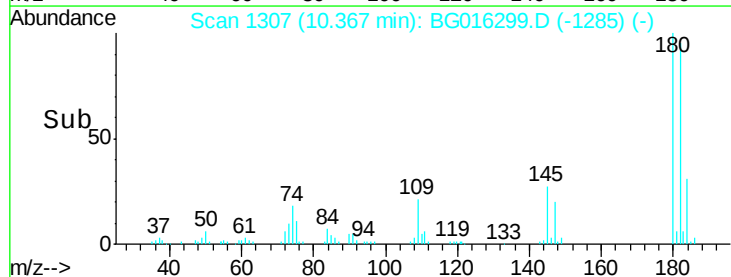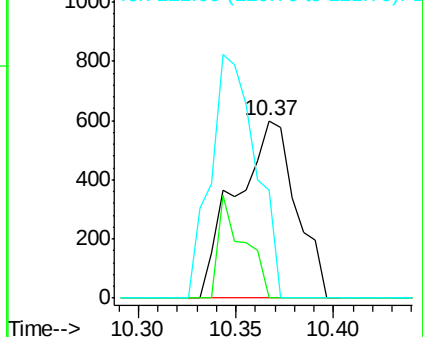

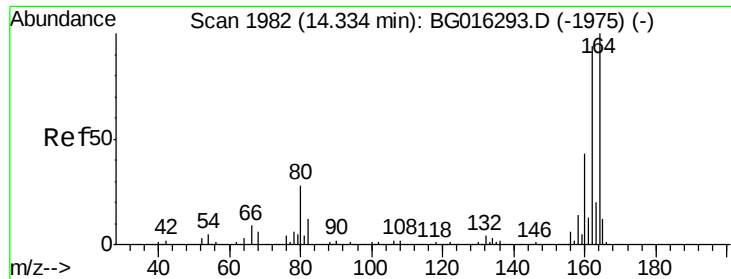

#7

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.34 min Scan# 1983

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion:164 Resp: 255348

Ion Ratio Lower Upper

164 100

162 96.7 72.8 109.2




160 42.1 31.9 47.9



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

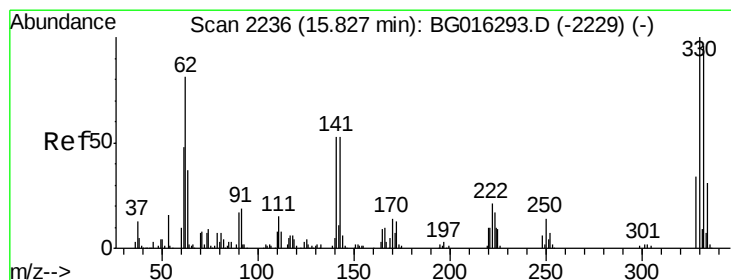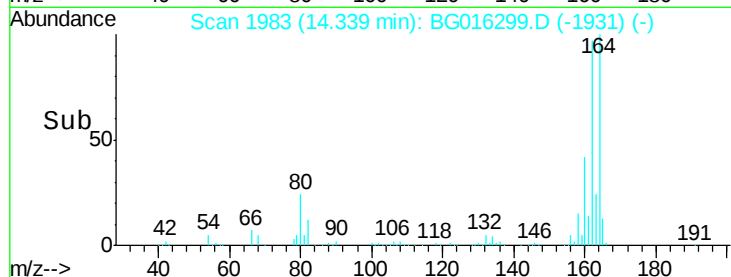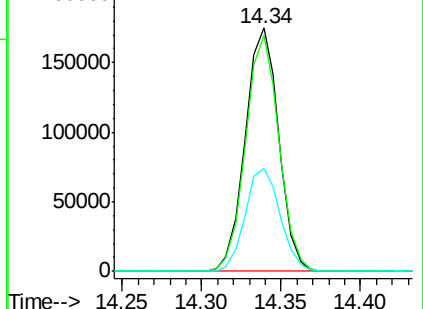

#8

2,4,6-Tribromophenol

Concen: 96.76 ng

RT: 15.83 min Scan# 2237

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51


Tgt Ion:330 Resp: 148033

Ion Ratio Lower Upper

330 100

332 95.6 79.6 119.4



141 55.6 27.3 40.9#

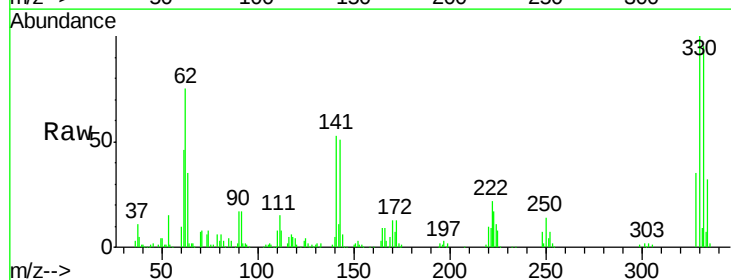


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

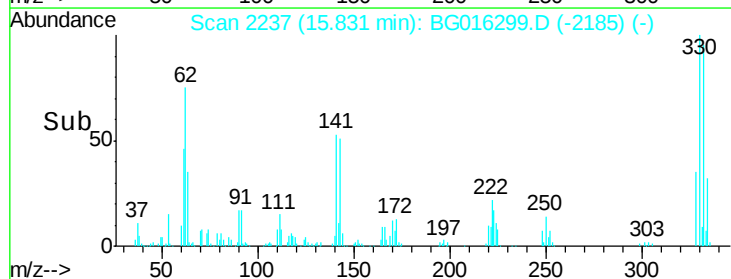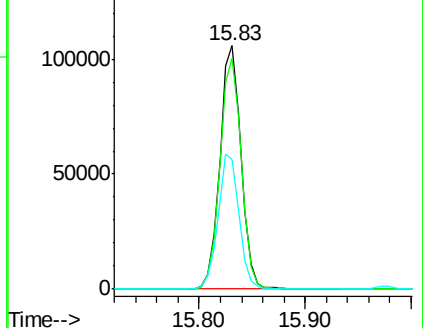

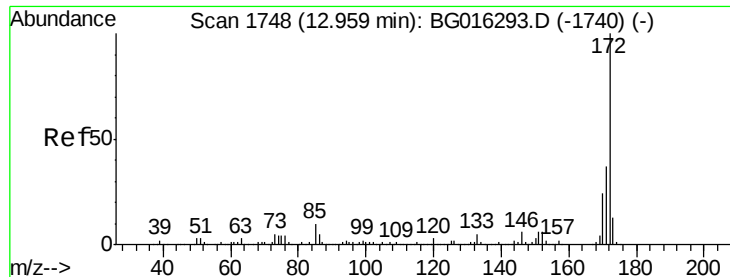

#9

2-Fluorobiphenyl

Concen: 75.08 ng

RT: 12.96 min Scan# 1748

Delta R.T. -0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion:172 Resp: 986368

Ion Ratio Lower Upper

172 100

171 37.9 31.1 46.7




170 24.5 19.8 29.8

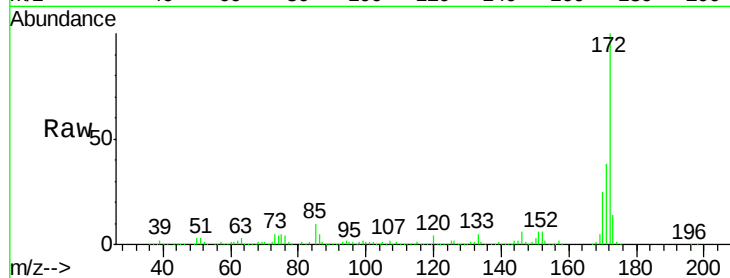

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

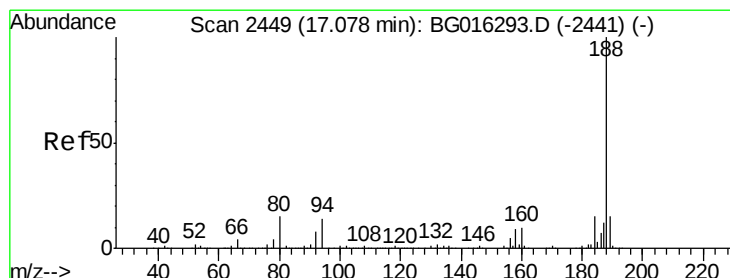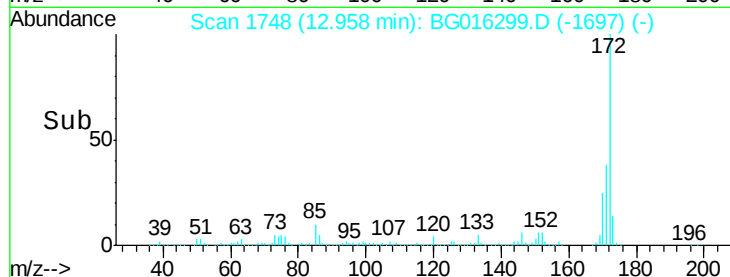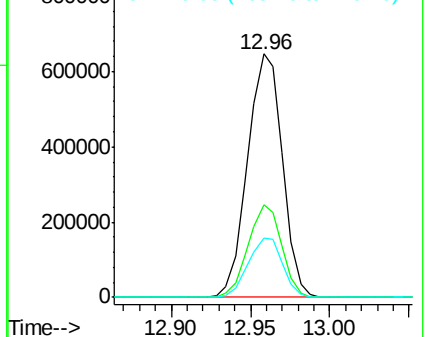

#10

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.08 min Scan# 2449

Delta R.T. -0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51


Tgt Ion:188 Resp: 530694

Ion Ratio Lower Upper

188 100

94 15.8 4.0 6.0#



80 15.6 3.4 5.2#

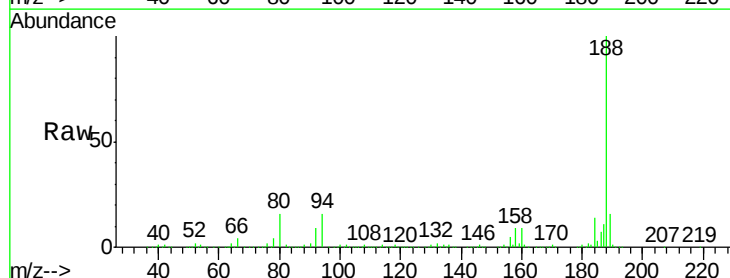


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

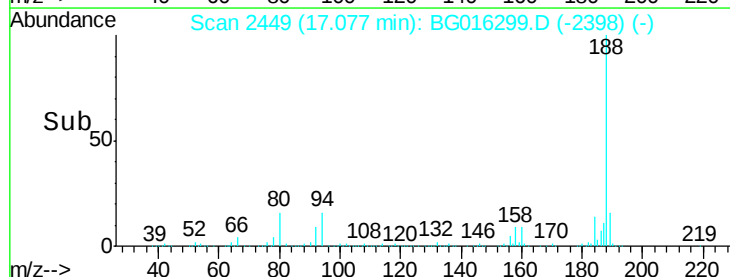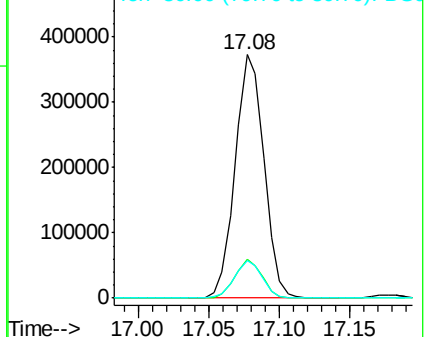

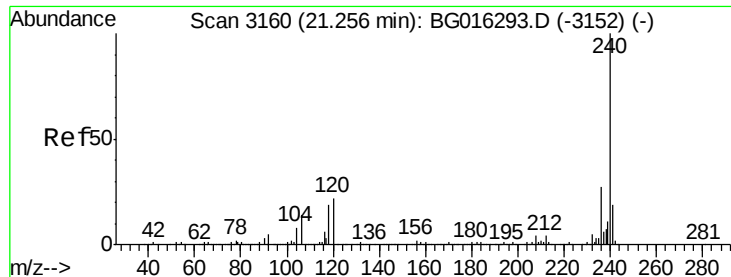

#11

Chrysene-d12

Concen: 20.00 ng

RT: 21.26 min Scan# 3161

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS


Tgt Ion:240 Resp: 449160

Ion Ratio Lower Upper

240 100

120 20.8 4.9 7.3#




236 27.1 18.8 28.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

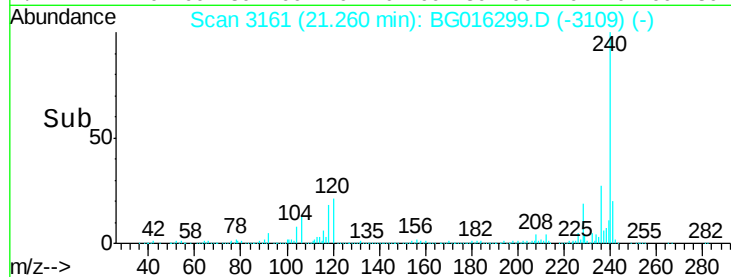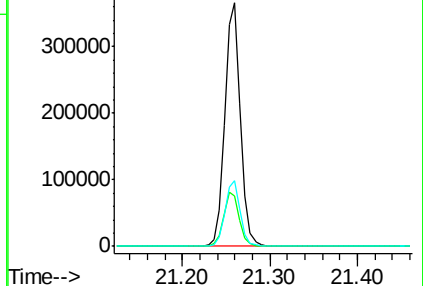

#12

Terphenyl-d14

Concen: 73.90 ng

RT: 19.70 min Scan# 2896

Delta R.T. 0.00 min

Lab File: BG016299.D

Acq: 9 Apr 2015 20:51


Tgt Ion:244 Resp: 1205518

Ion Ratio Lower Upper

244 100

212 8.1 5.7 8.5



122 24.4 5.4 8.2#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

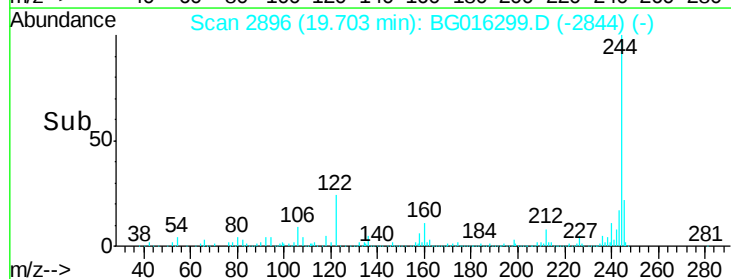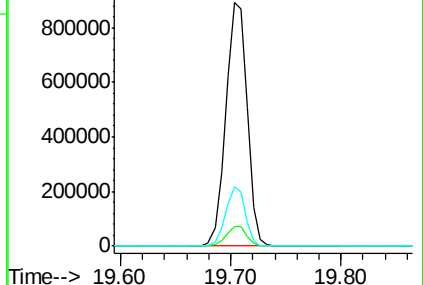

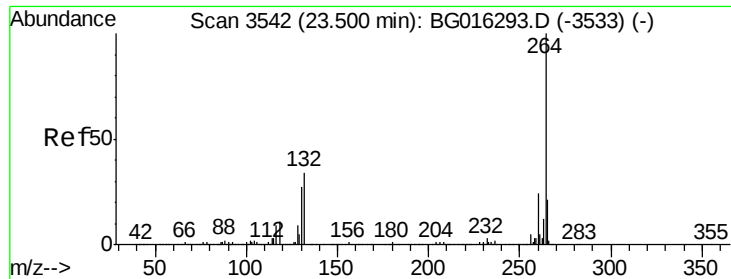

#13

Perylene-d12

Concen: 20.00 ng

RT: 23.50 min Scan# 3543

Delta R.T. 0.00 min

Lab File: BG016299.D


Acq: 9 Apr 2015 20:51

Instrument :

BNA_G

ClientSampleId :

PB82381BS



Tgt Ion: 264 Resp: 425686

Ion Ratio Lower Upper

264 100

260 24.4 17.5 26.3

265 21.5 17.0 25.4

