
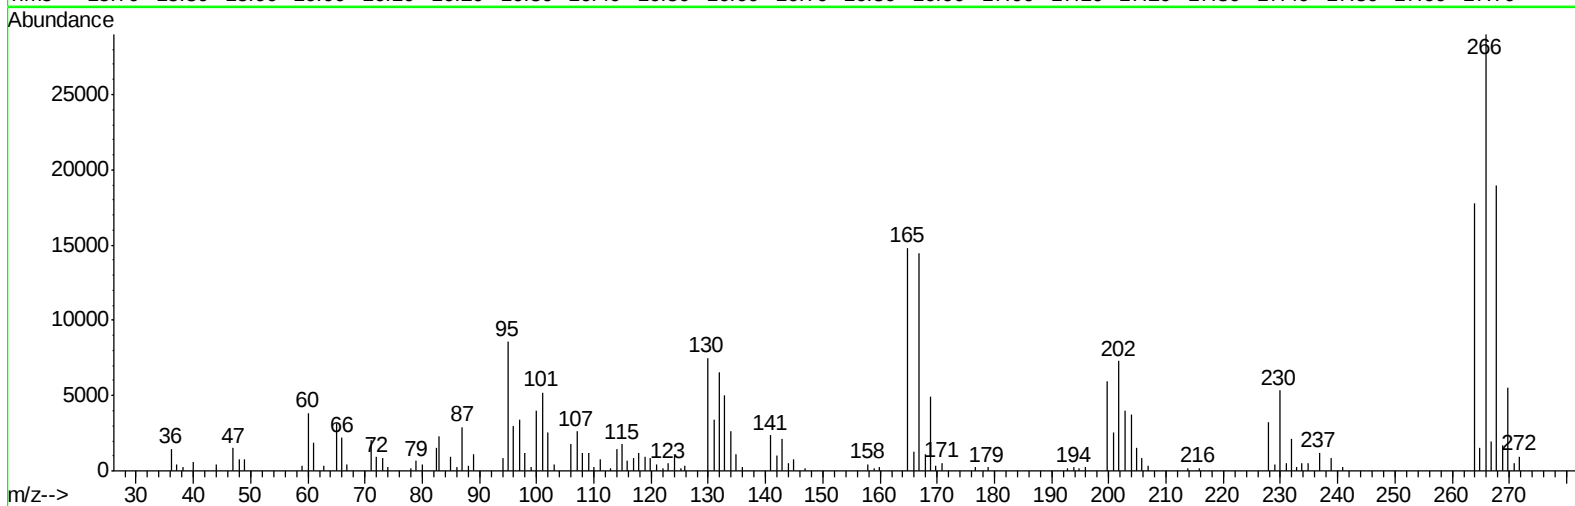


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040915\
Data File : BG016303.D
Acq On : 9 Apr 2015 23:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:53:22 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

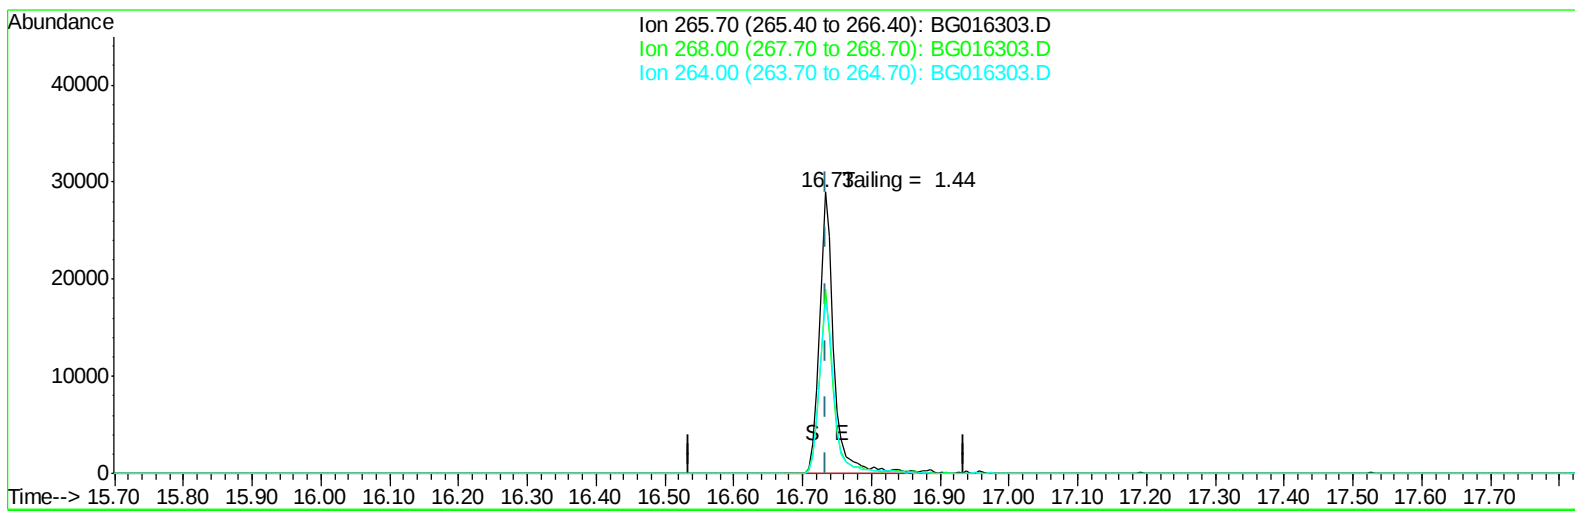

TIC: BG016303.D

(69) Pentachlorophenol (C)



16.733min (-0.002) 2557.95ng

response 41542

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	65.37
264.00	66.00	61.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040915\
Data File : BG016303.D
Acq On : 9 Apr 2015 23:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:53:22 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

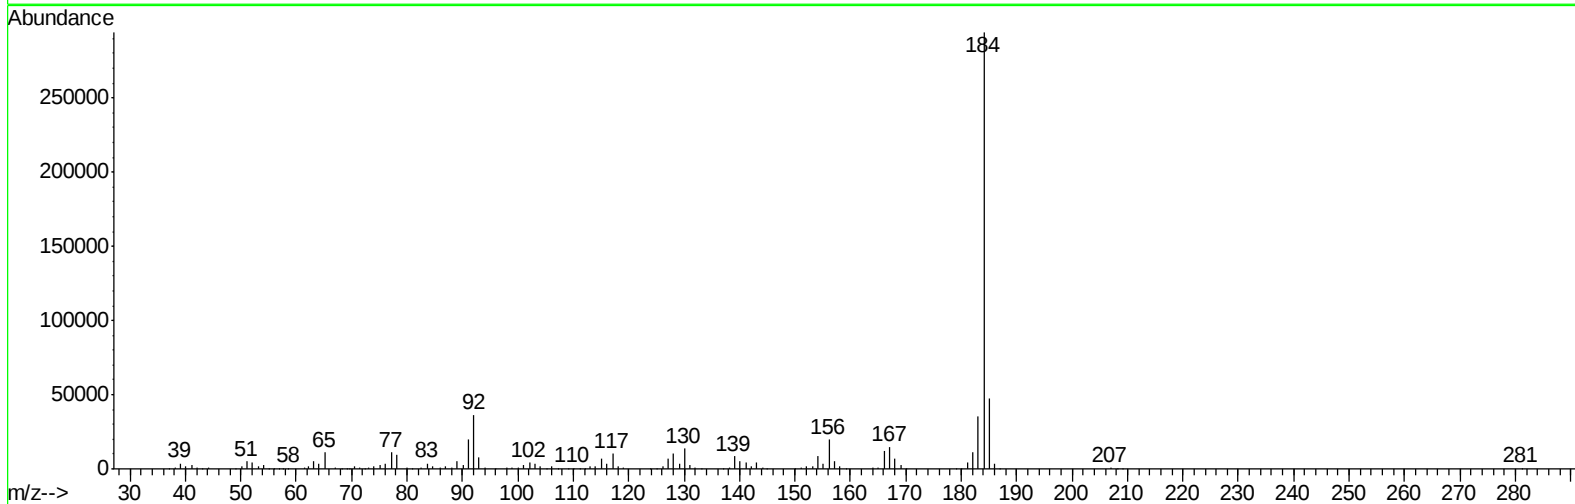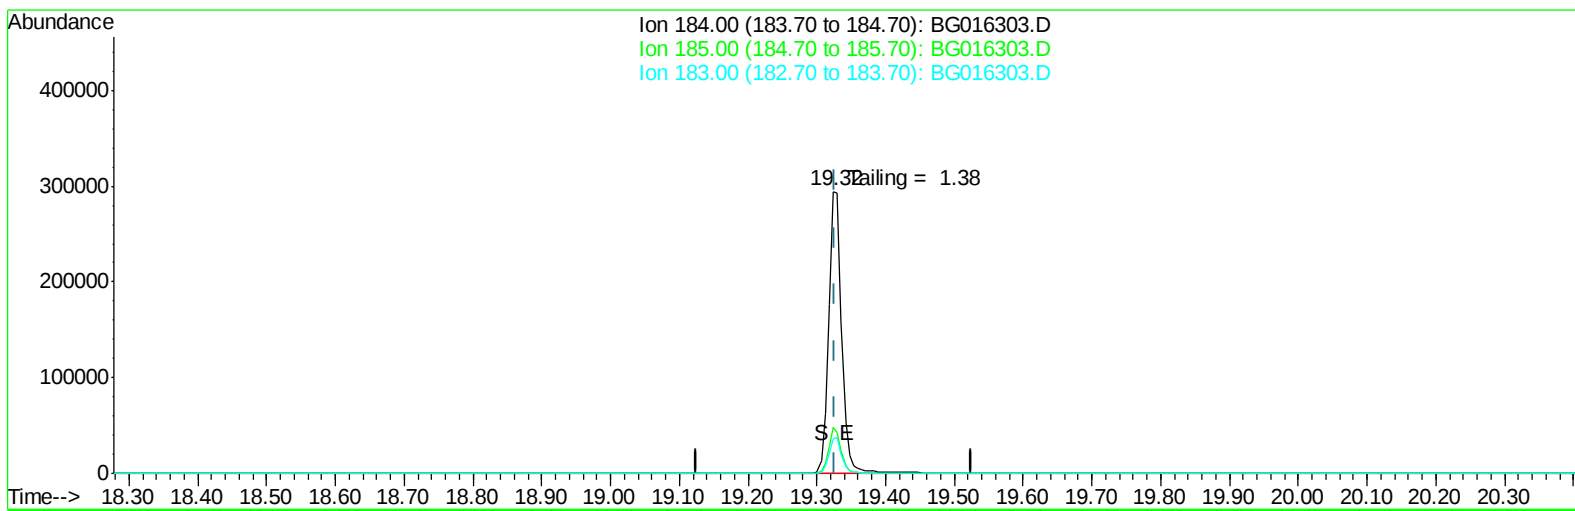

TIC: BG016303.D

(76) Benzidine

19.324min (-0.003) 3623.12ng

response 389802

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.22
183.00	13.00	12.09
0.00	0.00	0.00