


Data Path : Z:\HPCHEM1\BNA G\Data\BG040915\
Data File : BG016289.D
Acq On : 9 Apr 2015 15:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\625-TERPINEOL-BG040915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 09 19:35:19 2015

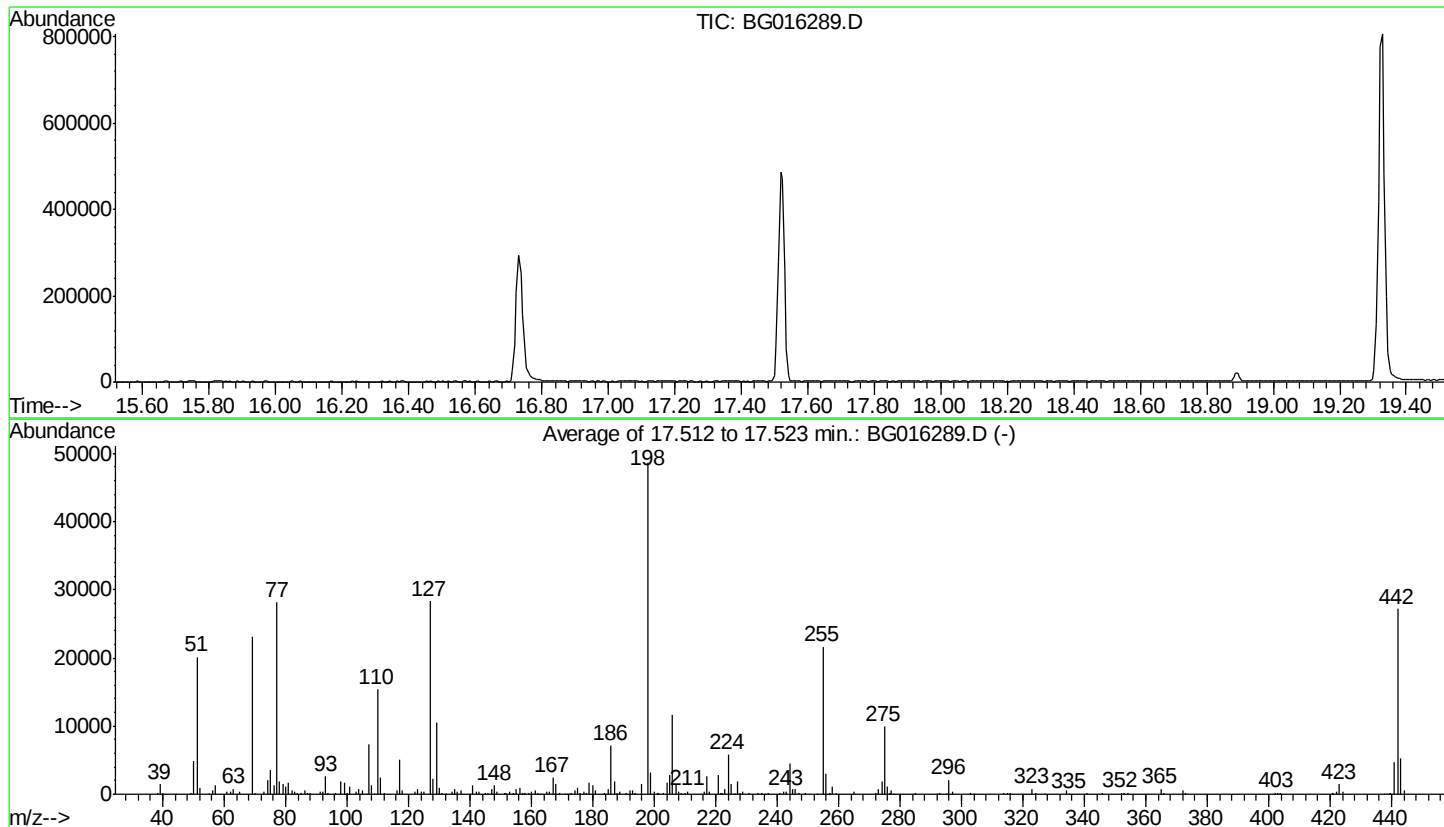

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.5	20191	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.4	23064	PASS
70	69	0.00	2	0.6	136	PASS
127	198	40	60	58.1	28280	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	48656	PASS
199	198	5	9	6.5	3145	PASS
275	198	10	30	20.3	9894	PASS
365	198	1	100	1.6	784	PASS
441	443	0.01	100	88.5	4657	PASS
442	198	40	100	55.8	27163	PASS
443	442	17	23	19.4	5264	PASS