
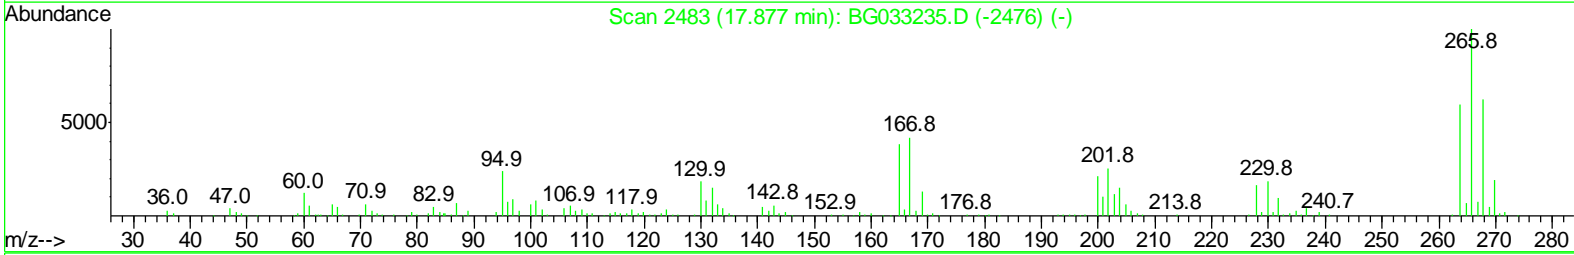
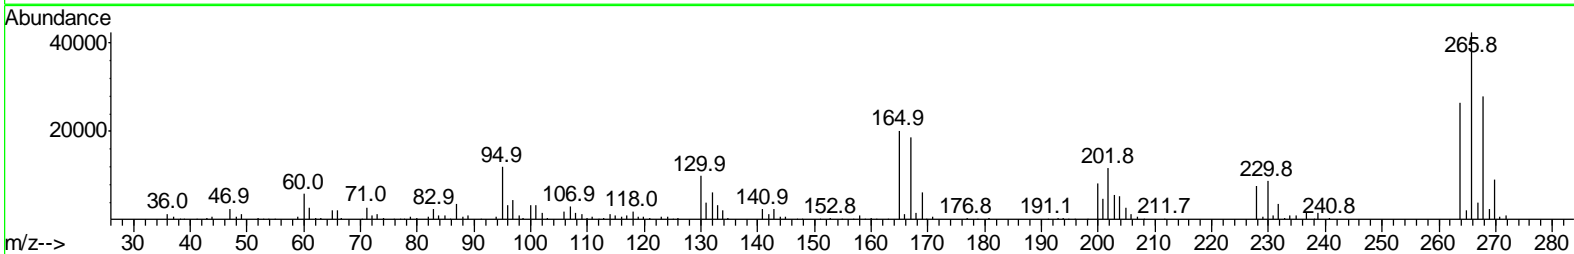


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
 Data File : BG033672.D
 Acq On : 9 Apr 2018 9:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 08:14:46 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 05 17:36:07 2018
 Response via : Initial Calibration

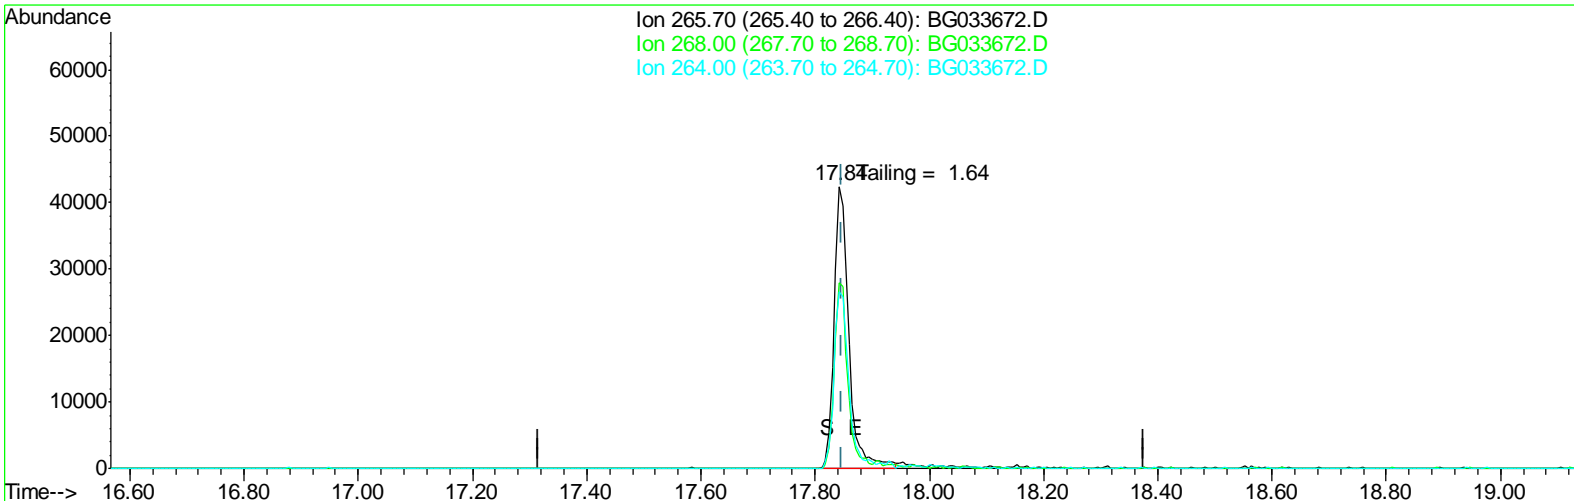




TIC: BG033672.D

(69) Pentachlorophenol (C)
 17.842min (-0.006) 92971.51ng
 response 75926

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.91
264.00	62.00	62.72
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
 Data File : BG033672.D
 Acq On : 9 Apr 2018 9:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 08:14:46 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 05 17:36:07 2018
 Response via : Initial Calibration

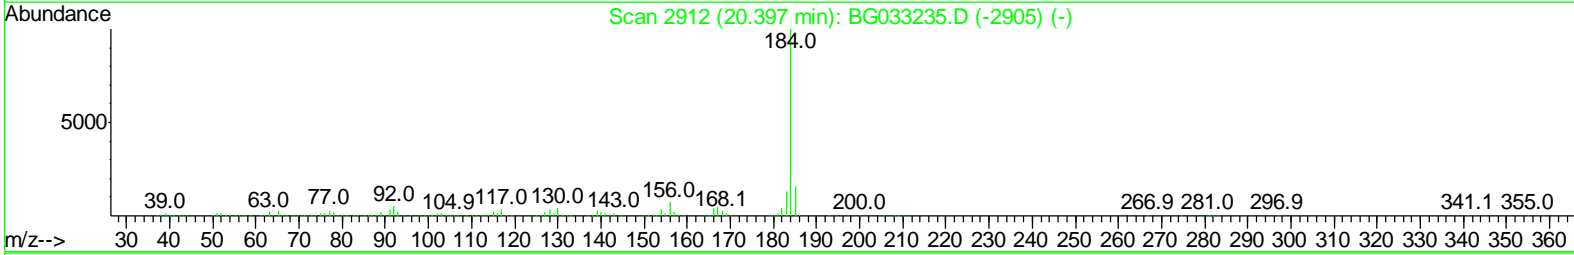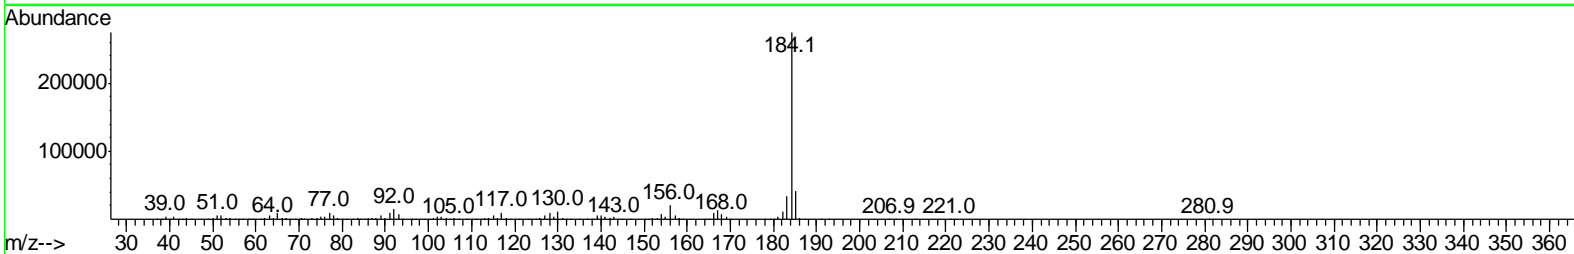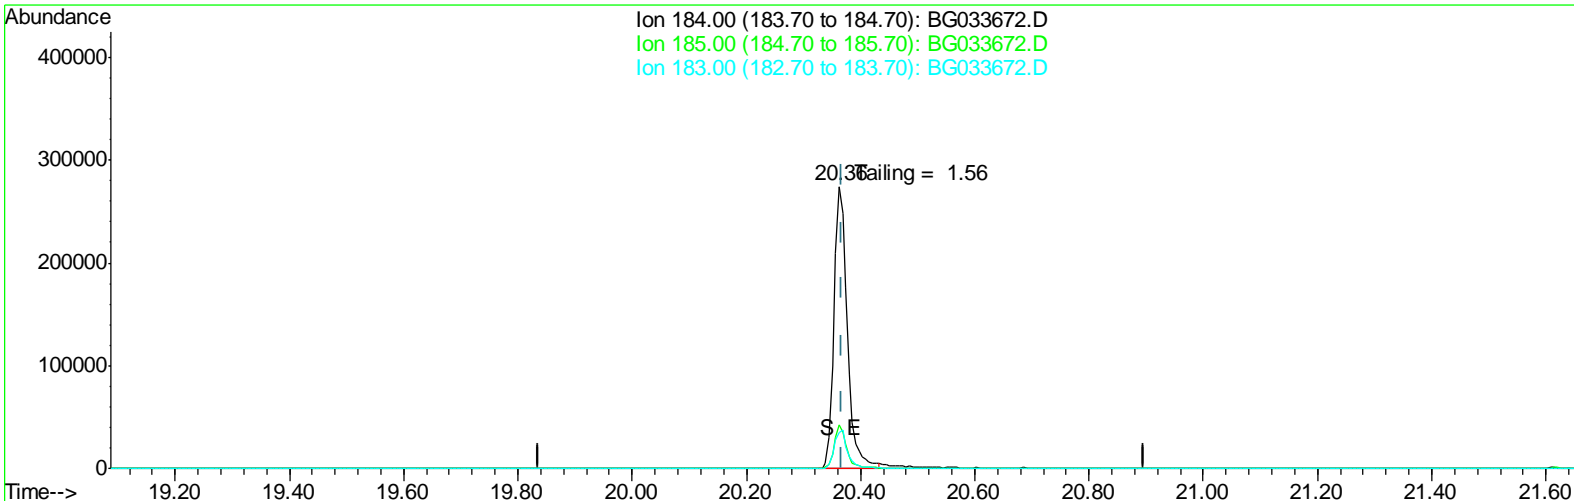

TIC: BG033672.D

(76) Benzidine

20.362min (-0.005) 289728.79ng

response 455707

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.26
183.00	13.30	12.62
0.00	0.00	0.00