
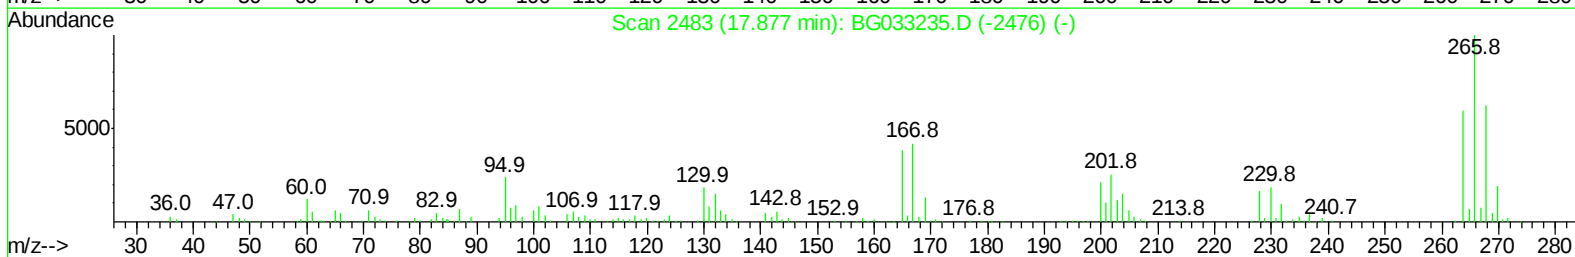
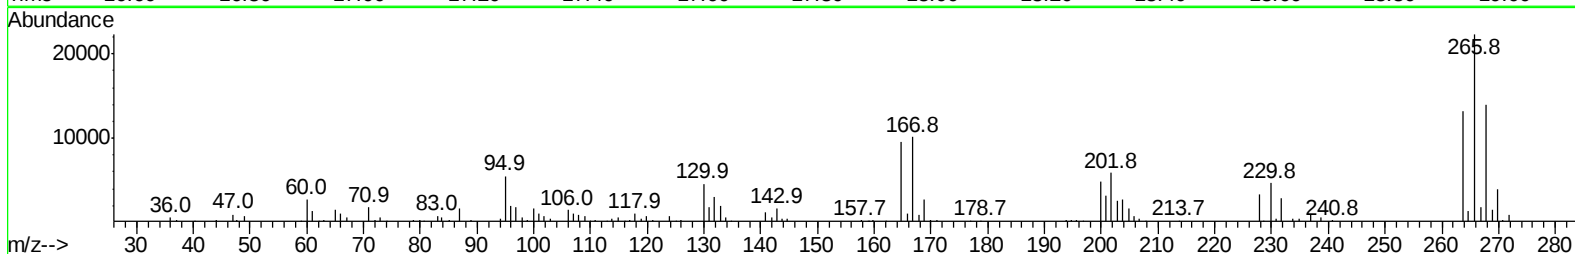


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
Data File : BG033690.D
Acq On : 9 Apr 2018 22:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 08:27:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

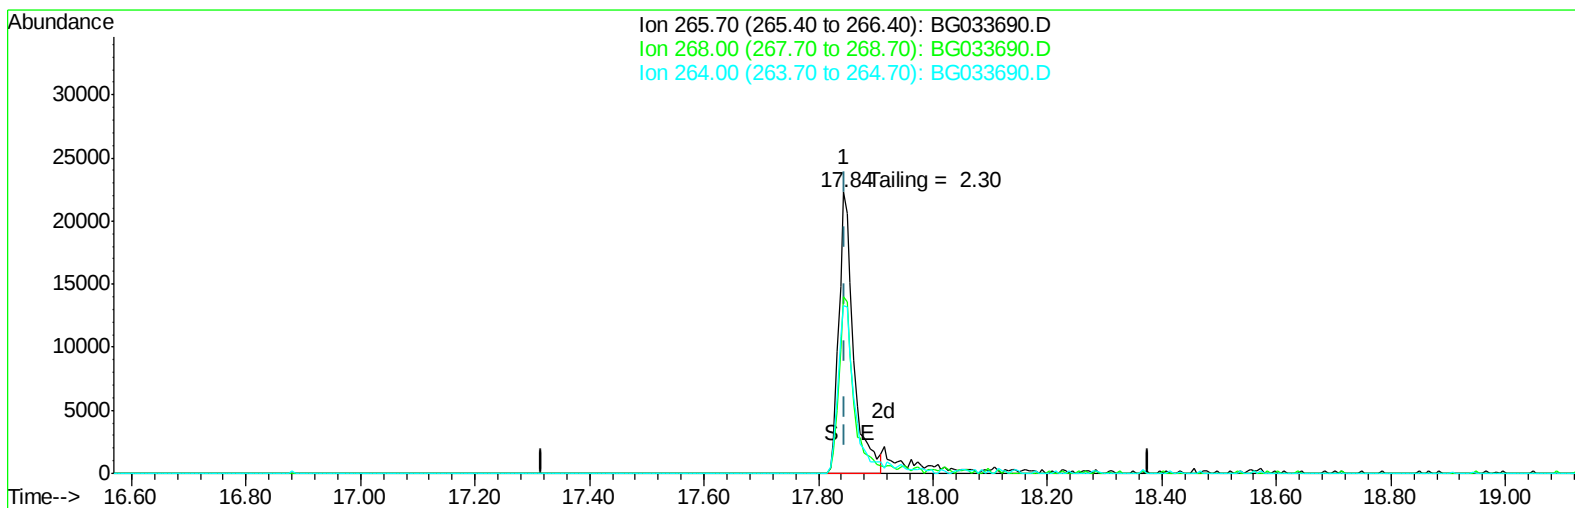

TIC: BG033690.D

(69) Pentachlorophenol (C)




17.844min (-0.003) 50741.64ng

response 39712

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.83
264.00	62.00	65.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
Data File : BG033690.D
Acq On : 9 Apr 2018 22:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 08:27:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

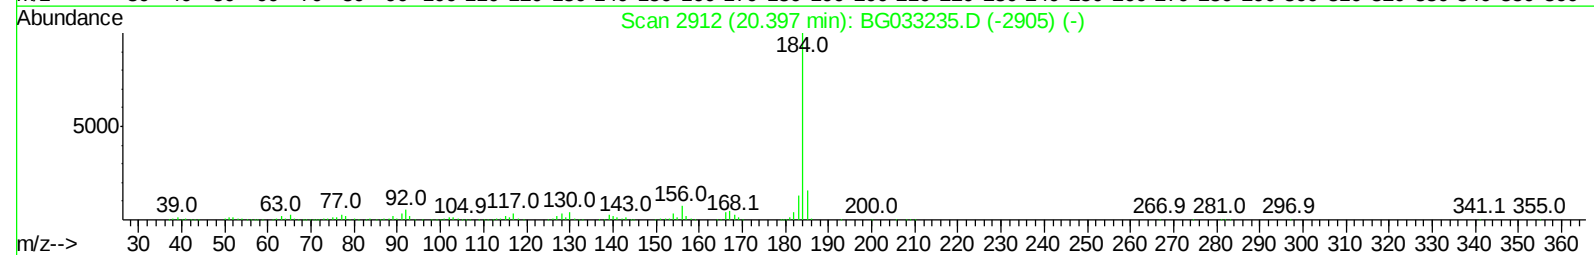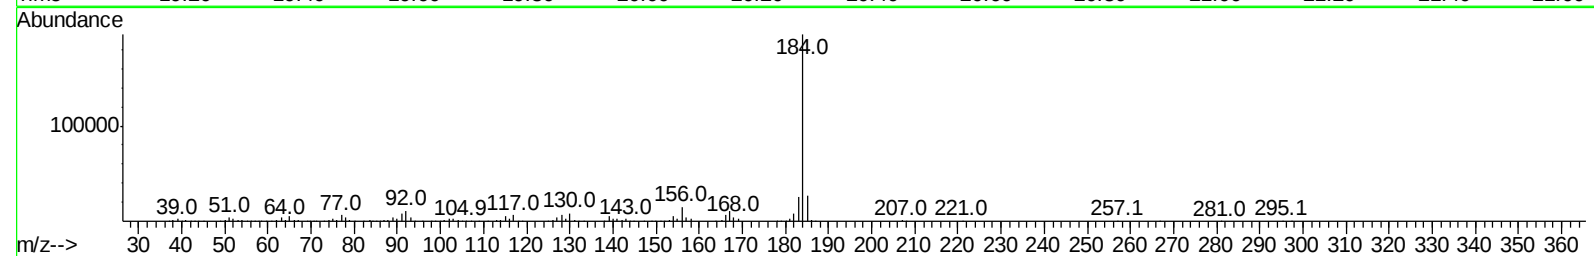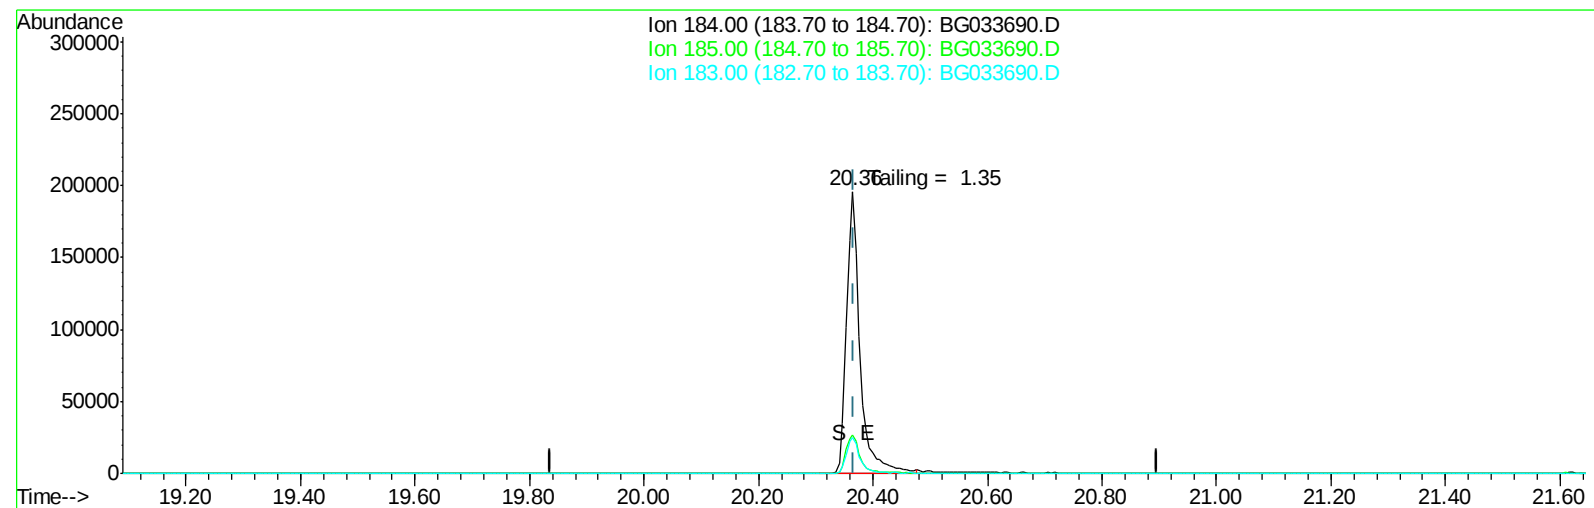

TIC: BG033690.D

(76) Benzidine

20.364min (-0.003) 177520.89ng

response 322545

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.82
183.00	13.30	12.86
0.00	0.00	0.00