

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
 Data File : BG033701.D
 Acq On : 10 Apr 2018 5:10
 Operator : SJ/JU
 Sample : J2157-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-040618-A

Quant Time: Apr 10 07:52:42 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 05 17:36:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.86	152	37173	20.00	ng	0.00
21) Naphthalene-d8	11.74	136	157479	20.00	ng	0.00
38) Acenaphthene-d10	15.47	164	115446	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	308615	20.00	ng	0.00
75) Chrysene-d12	22.55	240	316518	20.00	ng	-0.01
86) Perylene-d12	26.31	264	336955	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	363557	183.39	ng	0.00
7) Phenol-d6	7.97	99	506772	148.78	ng	0.00
23) Nitrobenzene-d5	10.06	82	376198	109.75	ng	0.00
41) 2,4,6-Tribromophenol	16.95	330	262931	152.28	ng	0.00
44) 2-Fluorobiphenyl	14.10	172	849868	106.27	ng	0.00
78) Terphenyl-d14	20.73	244	1637524	110.64	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
Data File : BG033701.D
Acq On : 10 Apr 2018 5:10
Operator : SJ/JU
Sample : J2157-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-040618-A

Quant Time: Apr 10 07:52:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

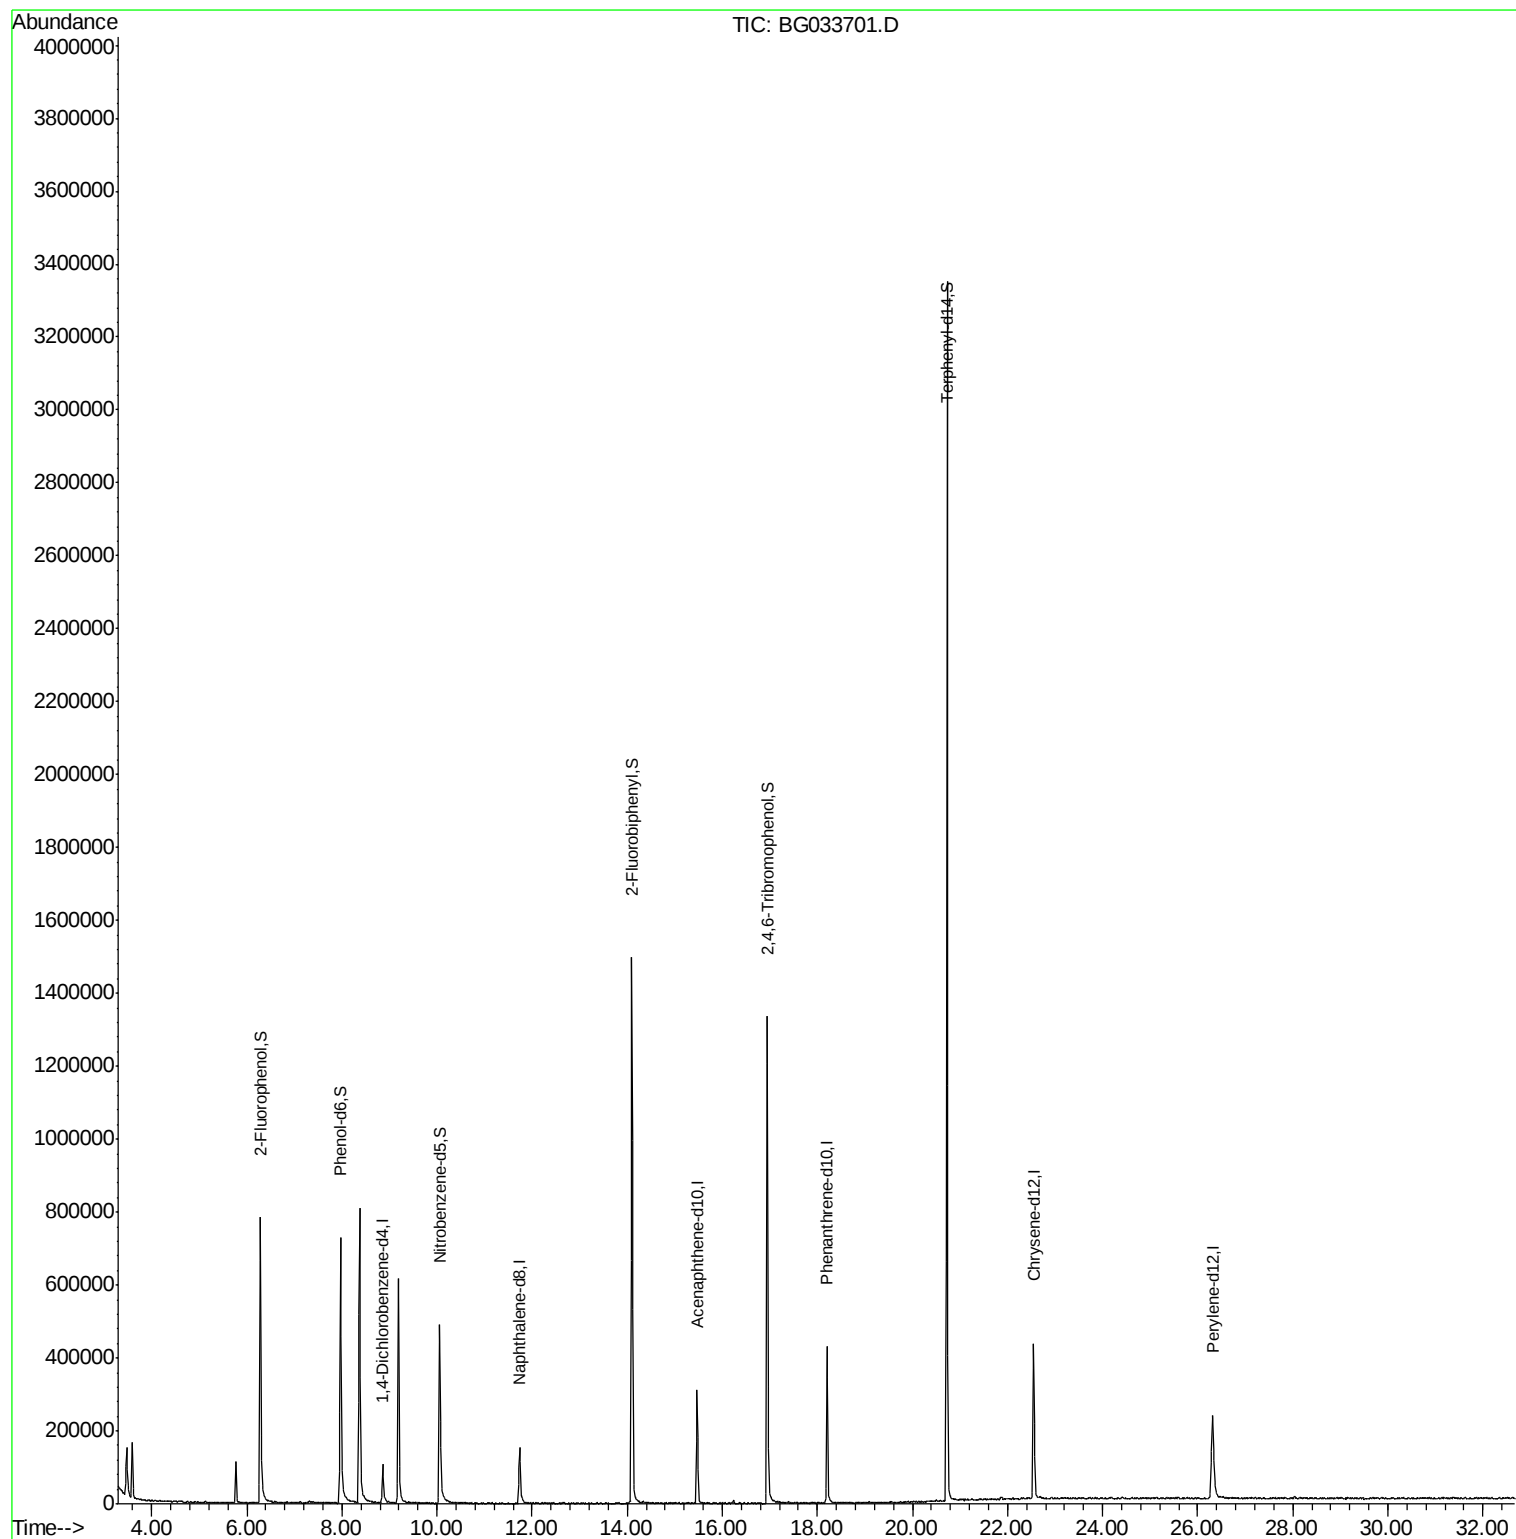

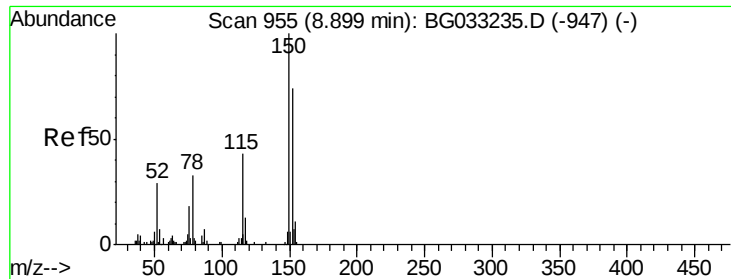


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.86 min Scan# 948
Delta R.T. -0.01 min
Lab File: BG033701.D
Acq: 10 Apr 2018 5:10

Instrument :
BNA_G
ClientSampleId :
CL-01-040618-A

Tot Ion:152 Resp: 37173
Ion Ratio Lower Upper
152 100
150 152.3 126.6 189.8
115 61.7 53.0 79.4

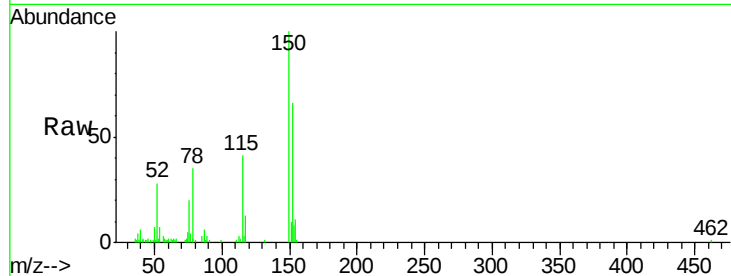


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

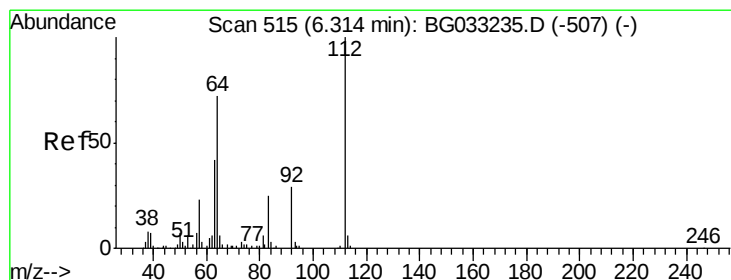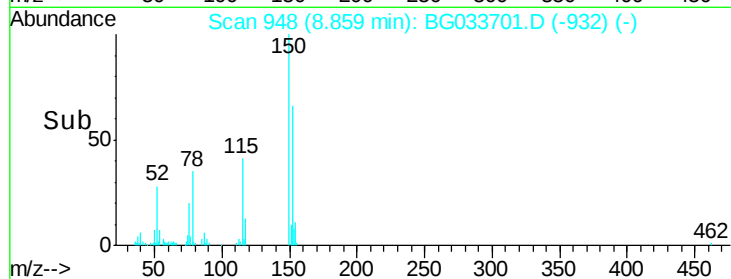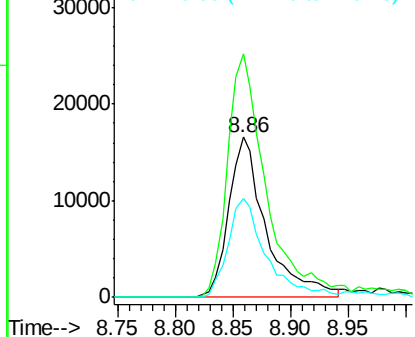



#5


2-Fluorophenol
Concen: 183.389 ng
RT: 6.29 min Scan# 510
Delta R.T. -0.00 min
Lab File: BG033701.D
Acq: 10 Apr 2018 5:10

Tgt Ion:112 Resp: 363557
Ion Ratio Lower Upper
112 100
64 74.6 56.3 84.5
63 42.6 30.1 45.1

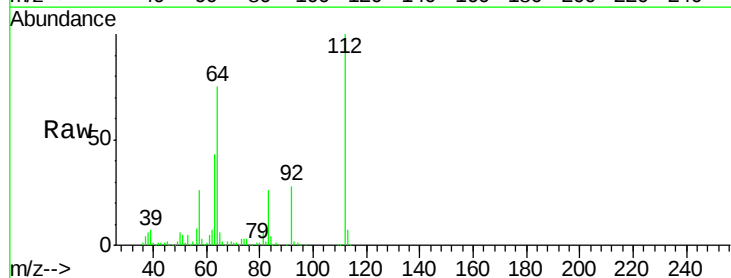

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

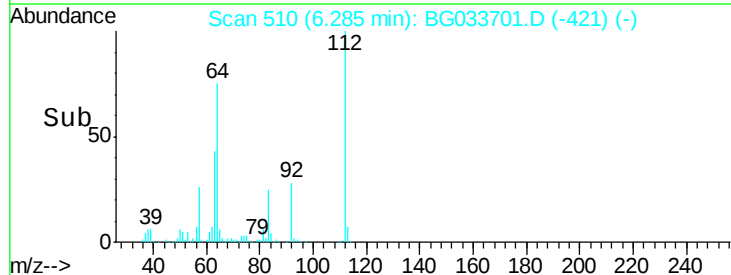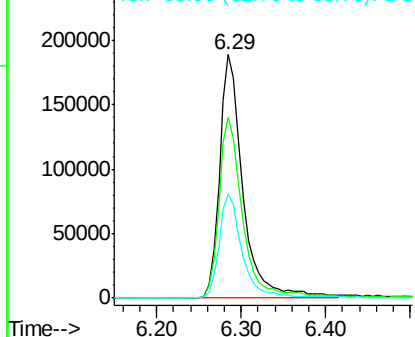

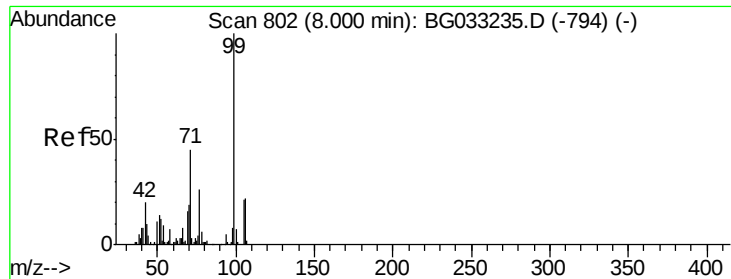

#7

Phenol-d6

Concen: 148.778 ng

RT: 7.97 min Scan# 797

Delta R.T. 0.00 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10

Instrument :

BNA_G

ClientSampleId :

CL-01-040618-A





Tot Ion: 99 Resp: 506772

Ion Ratio Lower Upper

99 100

42 20.7 14.1 21.1

71 41.9 26.1 39.1#

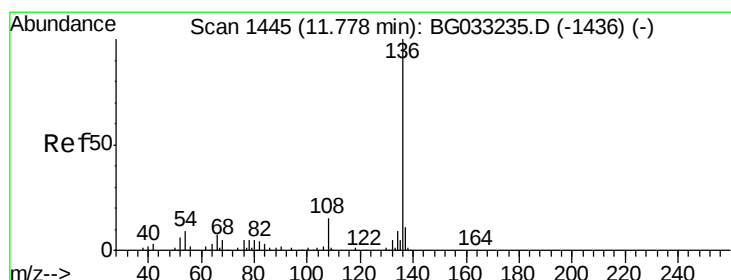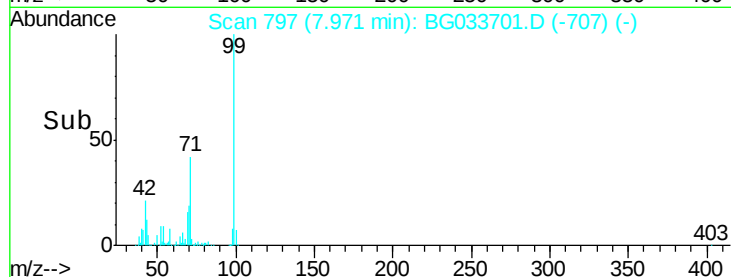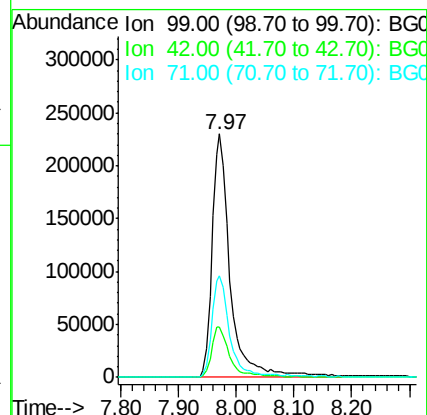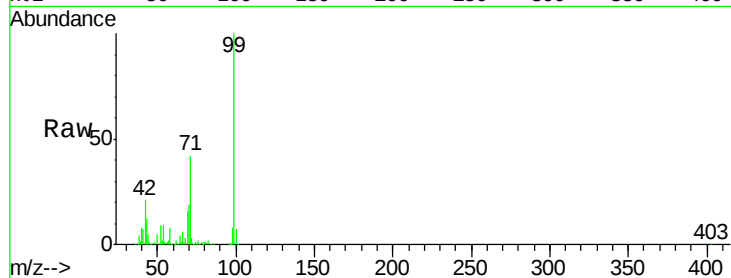

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.74 min Scan# 1438

Delta R.T. -0.00 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10

Tgt Ion: 136 Resp: 157479




Ion Ratio Lower Upper


136 100

137 11.2 9.2 13.8

54 11.0 10.3 15.5

68 5.4 4.5 6.7


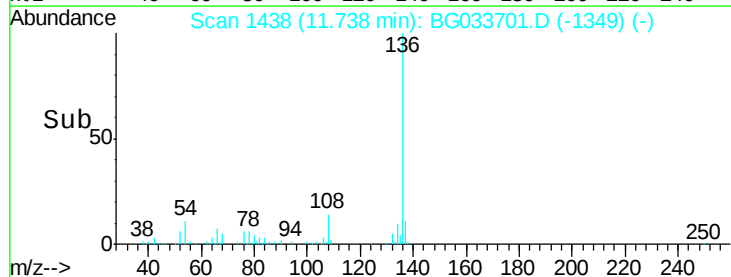
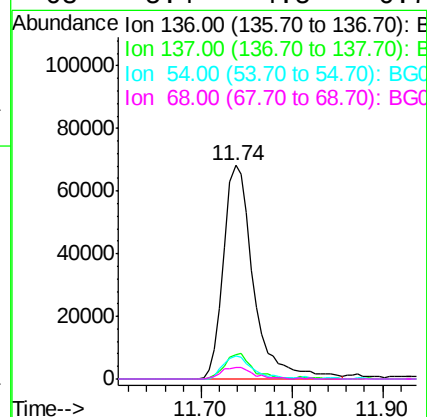
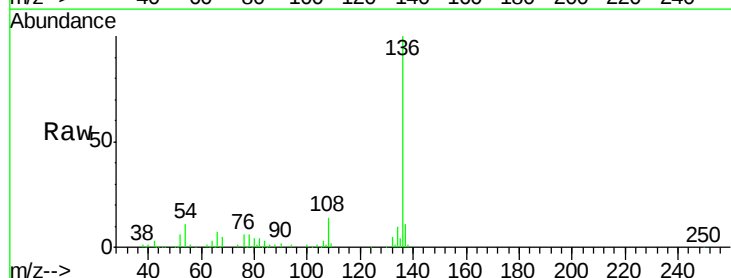


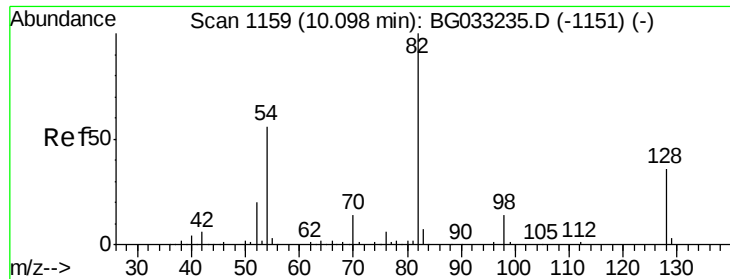

#23
 Nitrobenzene-d5
 Concen: 109.755 ng
 RT: 10.06 min Scan# 1152
 Delta R.T. -0.00 min
 Lab File: BG033701.D
 Acq: 10 Apr 2018 5:10




Instrument :
 BNA_G
 ClientSampleId :
 CL-01-040618-A


Tot Ion	82	Resp	376198
Ion Ratio	Lower	Upper	
82	100		
128	36.5	29.7	44.5
54	56.1	43.1	64.7

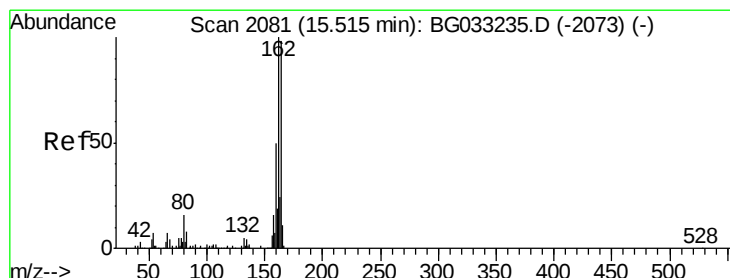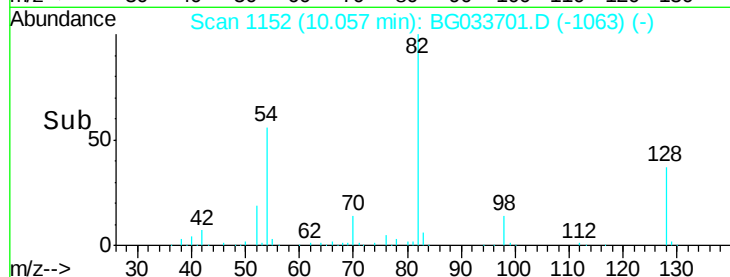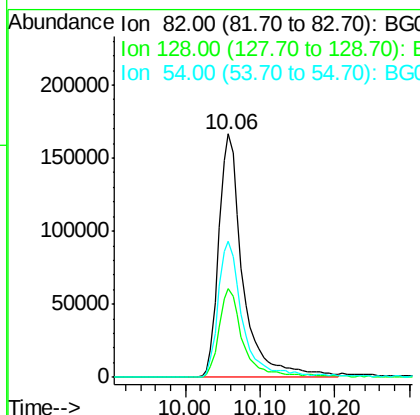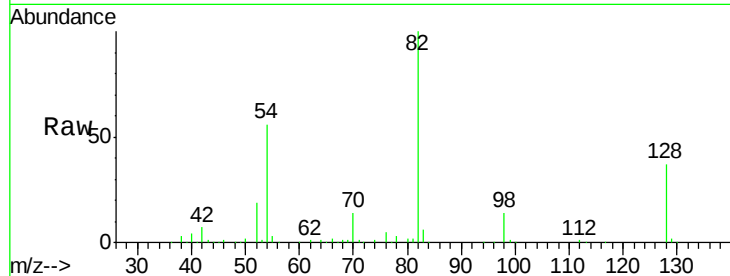

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2074
 Delta R.T. -0.00 min
 Lab File: BG033701.D
 Acq: 10 Apr 2018 5:10

Tgt Ion	164	Resp	115446
Ion Ratio	Lower	Upper	
164	100		
162	97.3	78.8	118.2
160	44.1	35.4	53.0

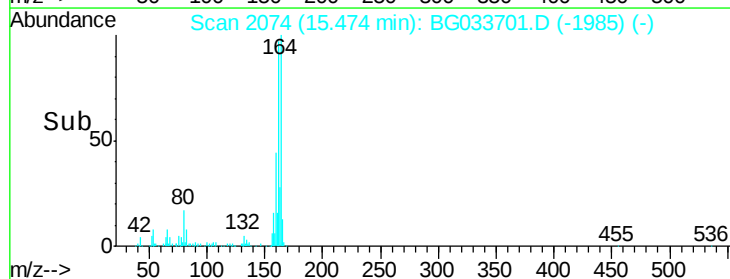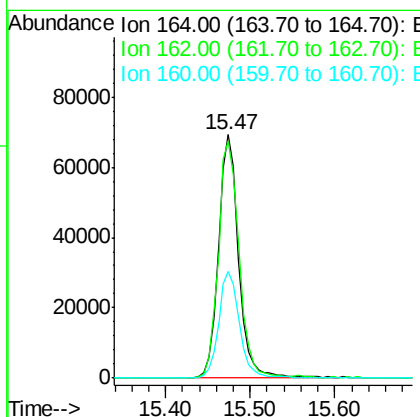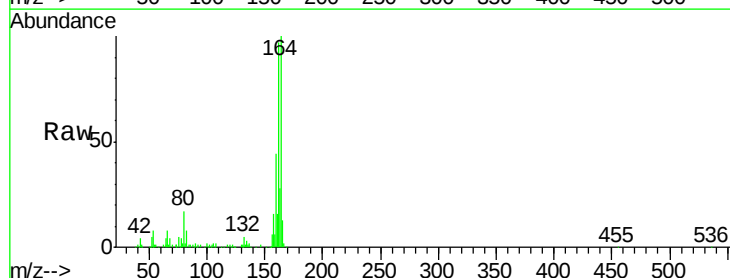


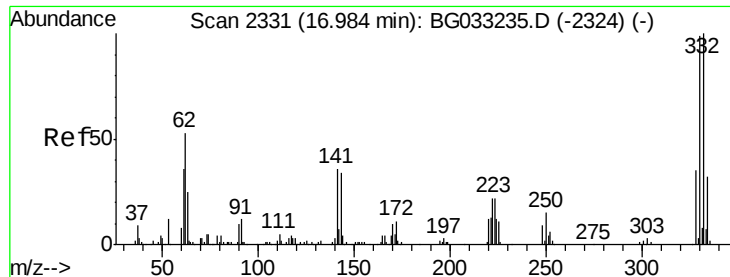



#41
 2,4,6-Tribromophenol
 Concen: 152.280 ng
 RT: 16.95 min Scan# 2325
 Delta R.T. -0.01 min
 Lab File: BG033701.D
 Acq: 10 Apr 2018 5:10

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-040618-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.9	77.0	115.6
141	38.6	25.2	37.8#

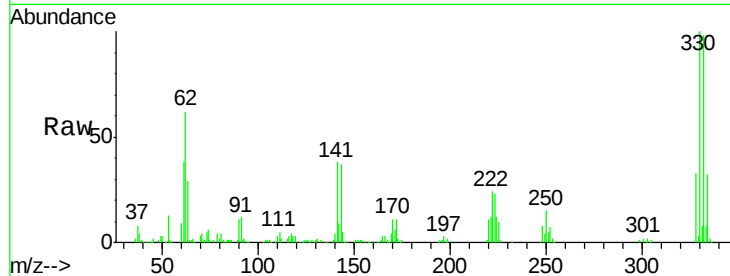


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

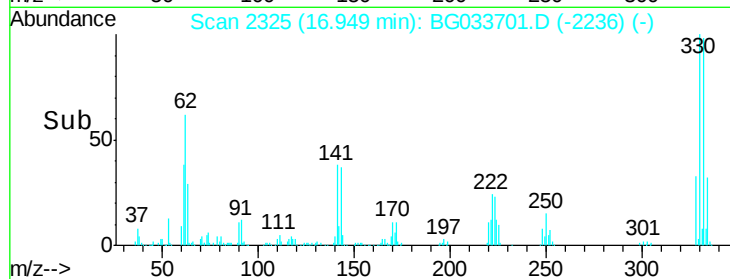
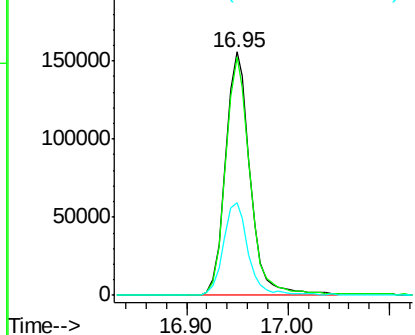



#44
 2-Fluorobiphenyl
 Concen: 106.275 ng
 RT: 14.10 min Scan# 1840
 Delta R.T. -0.00 min
 Lab File: BG033701.D
 Acq: 10 Apr 2018 5:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.2	30.0	45.0
170	25.6	19.5	29.3

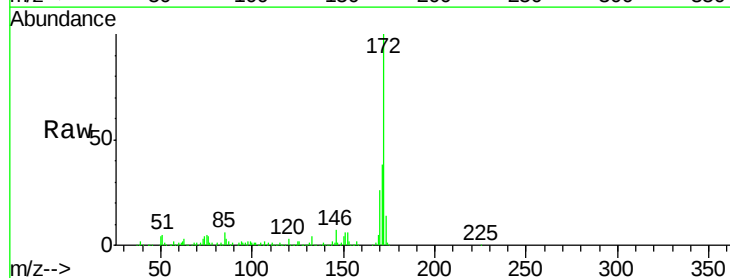

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

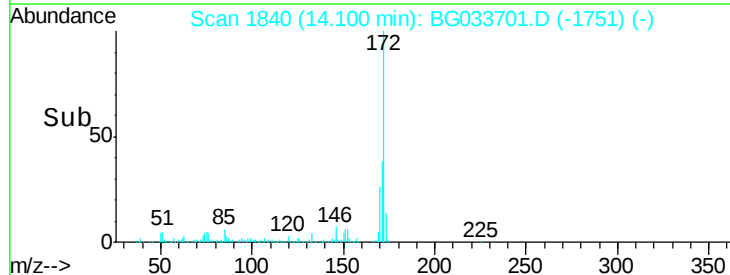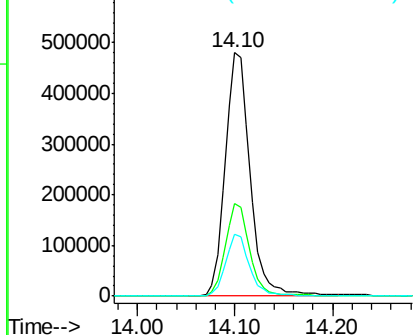

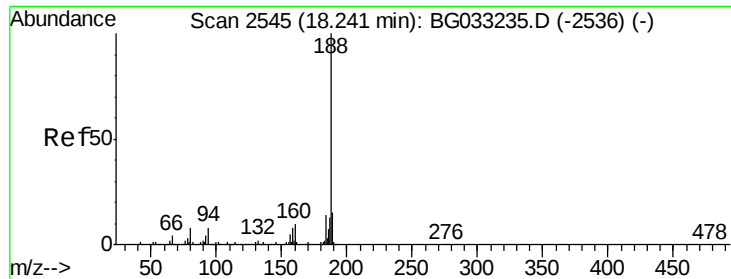

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.21 min Scan# 2539

Delta R.T. -0.00 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10

Instrument :

BNA_G

ClientSampleId :

CL-01-040618-A


Tot Ion:188 Resp: 308615

Ion Ratio Lower Upper

188 100

94 6.2 6.9 10.3#




80 8.6 7.7 11.5

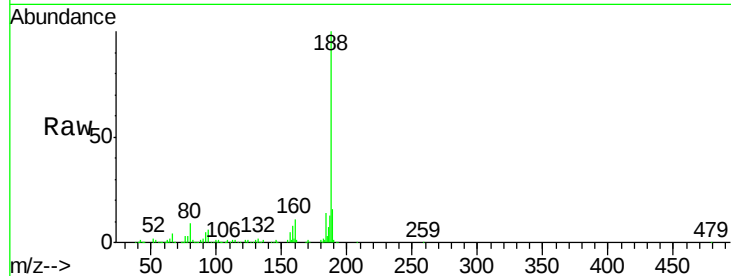

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

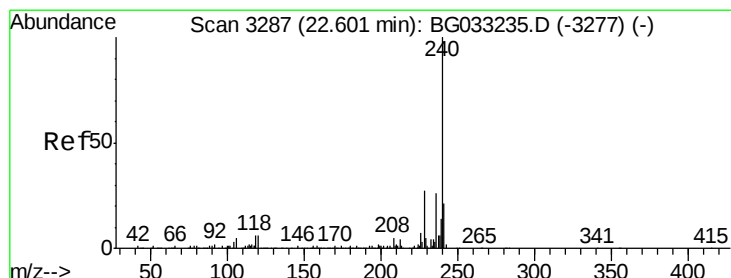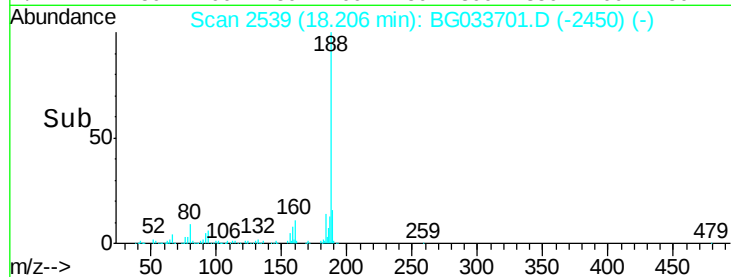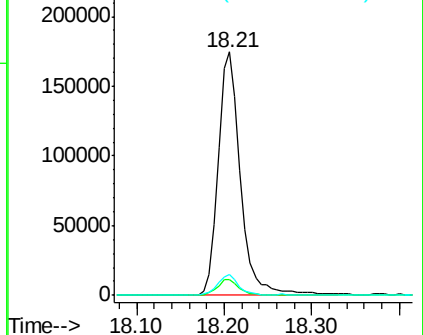

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.55 min Scan# 3278

Delta R.T. -0.01 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10


Tgt Ion:240 Resp: 316518

Ion Ratio Lower Upper

240 100

120 7.3 6.8 10.2



236 26.5 20.9 31.3

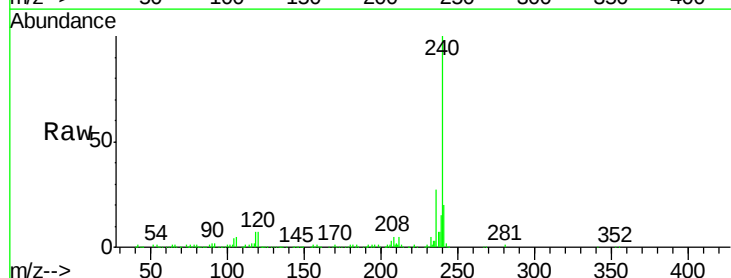


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

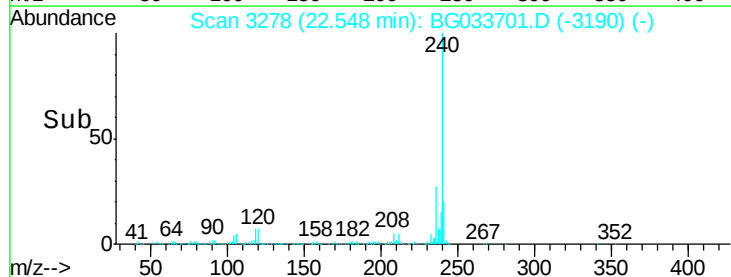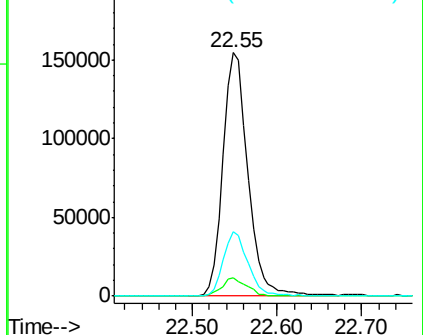

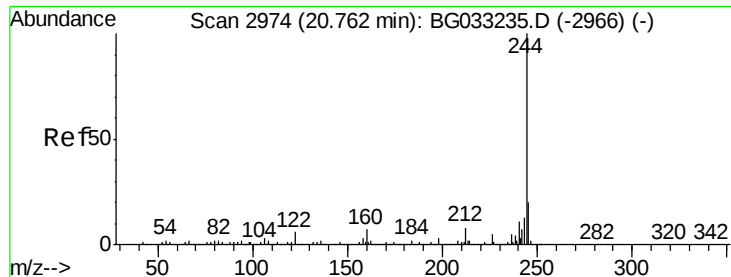

#78

Terphenyl-d14

Concen: 110.642 ng

RT: 20.73 min Scan# 2968

Delta R.T. 0.00 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10

Instrument :

BNA_G

ClientSampleId :

CL-01-040618-A


Tot Ion:244 Resp: 1637524

Ion Ratio Lower Upper

244 100

212 9.0 5.8 8.8#




122 7.5 7.0 10.4

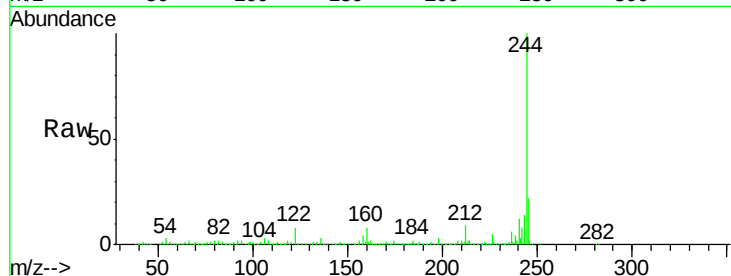

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

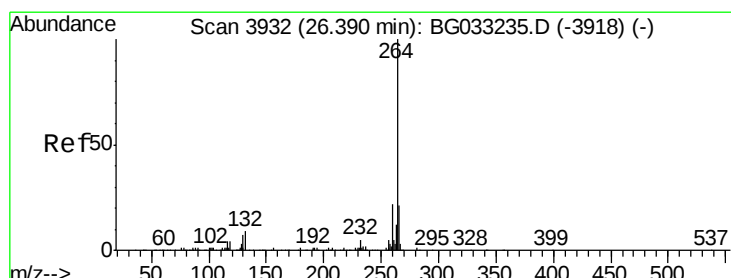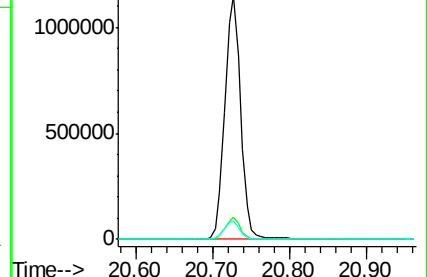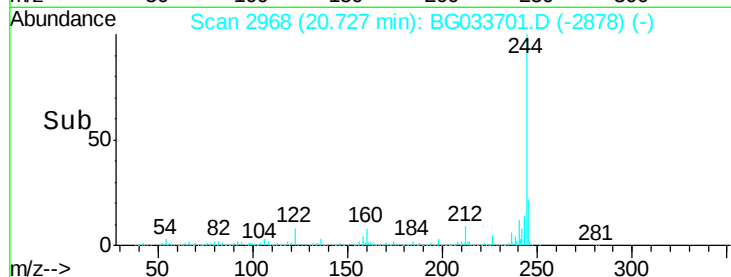

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.31 min Scan# 3919

Delta R.T. -0.00 min

Lab File: BG033701.D

Acq: 10 Apr 2018 5:10


Tgt Ion:264 Resp: 336955

Ion Ratio Lower Upper

264 100

260 25.2 17.4 26.0

265 21.1 17.7 26.5

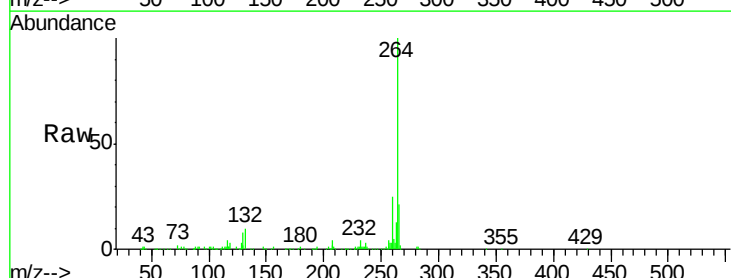

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

