

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
 Data File : BG033708.D
 Acq On : 10 Apr 2018 9:33
 Operator : SJ/JU
 Sample : PB108084BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB108084BL

Quant Time: Apr 10 11:02:46 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 05 17:36:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.85	152	40270	20.00	ng	0.00
21) Naphthalene-d8	11.74	136	169994	20.00	ng	0.00
38) Acenaphthene-d10	15.47	164	119999	20.00	ng	0.00
63) Phenanthrene-d10	18.20	188	326436	20.00	ng	0.00
75) Chrysene-d12	22.54	240	333509	20.00	ng	-0.02
86) Perylene-d12	26.30	264	354861	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	362947	169.00	ng	0.00
7) Phenol-d6	7.97	99	518168	140.42	ng	0.00
23) Nitrobenzene-d5	10.06	82	334029	90.28	ng	0.00
41) 2,4,6-Tribromophenol	16.95	330	204498	113.94	ng	0.00
44) 2-Fluorobiphenyl	14.10	172	744745	89.60	ng	0.00
78) Terphenyl-d14	20.72	244	1365174	87.54	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040918\
Data File : BG033708.D
Acq On : 10 Apr 2018 9:33
Operator : SJ/JU
Sample : PB108084BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB108084BL

Quant Time: Apr 10 11:02:46 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

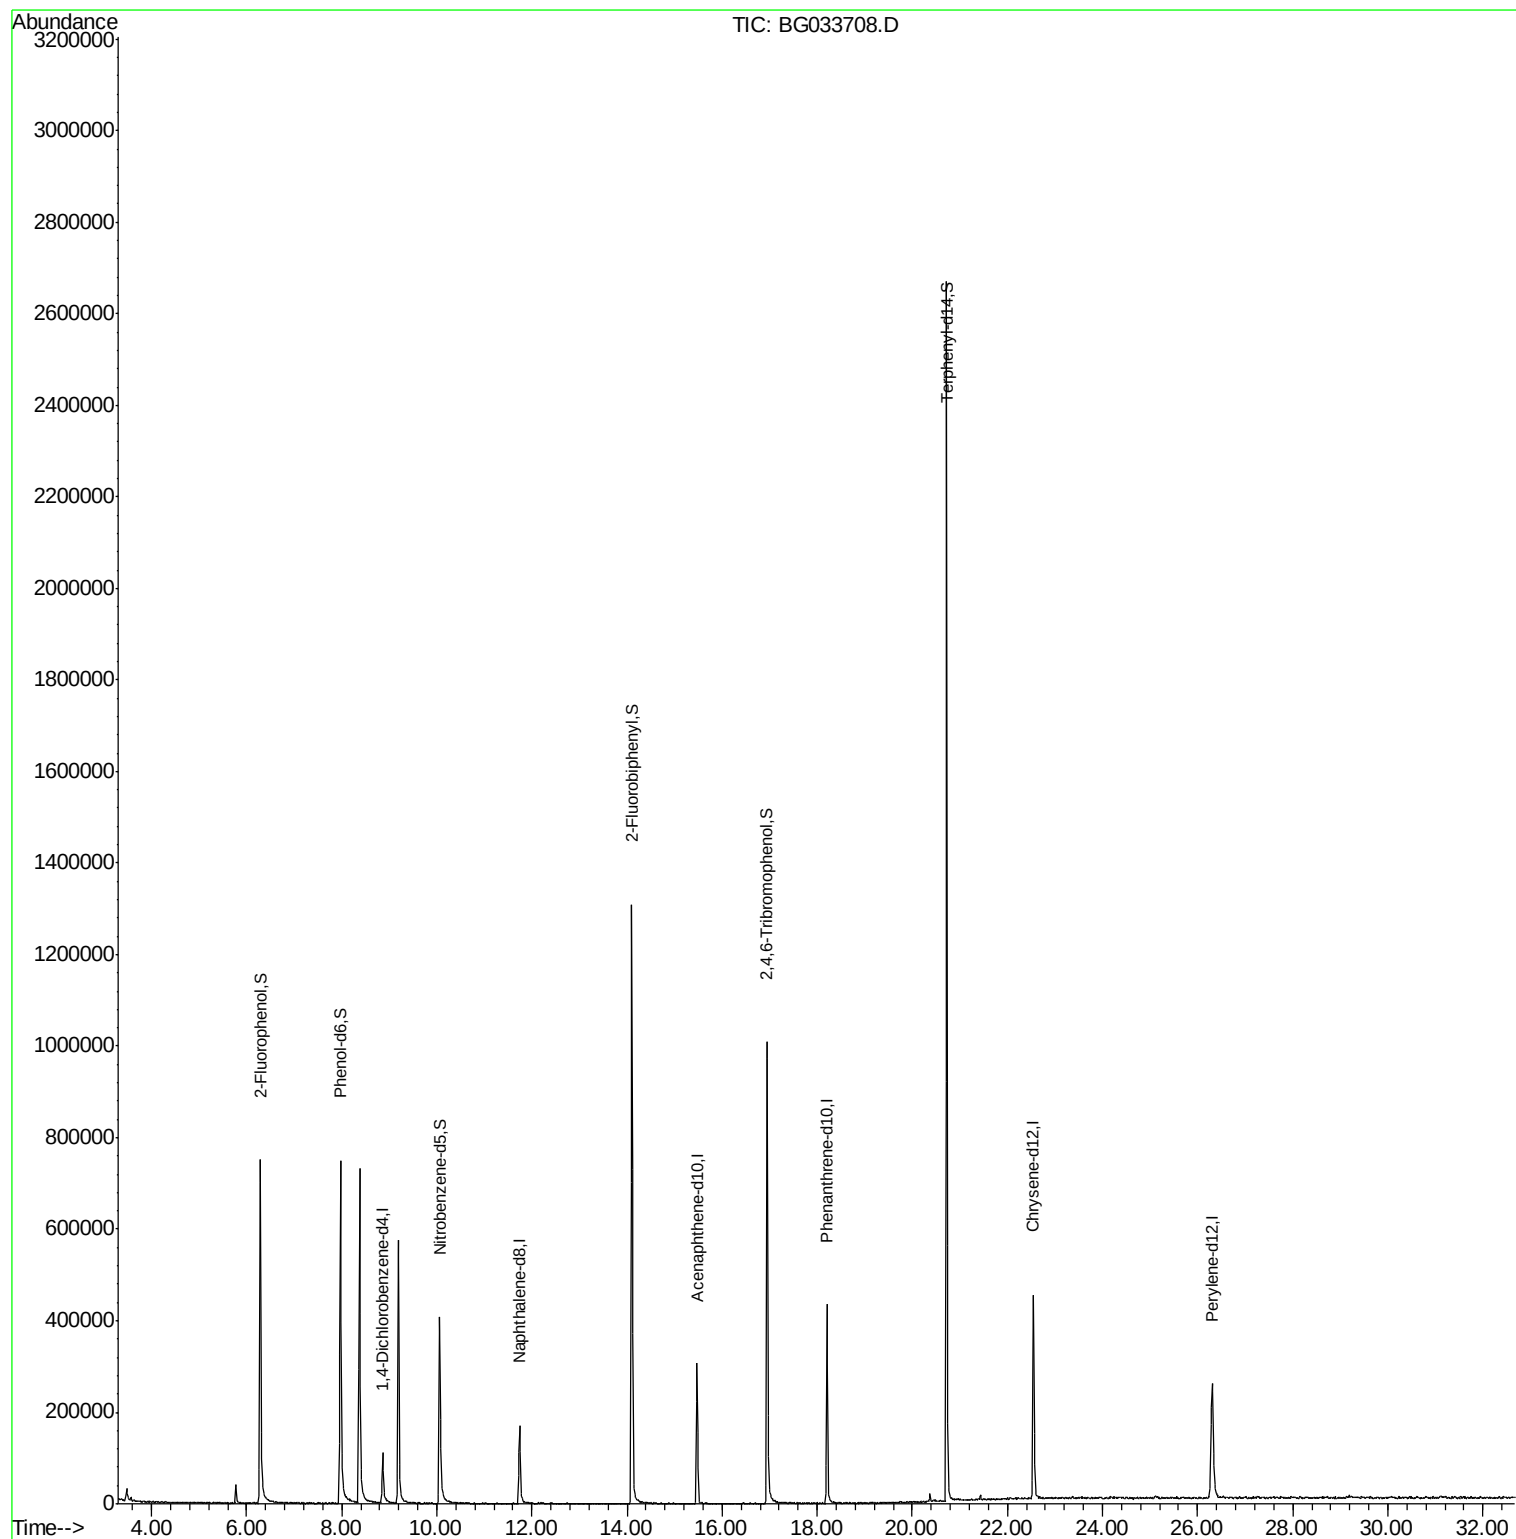

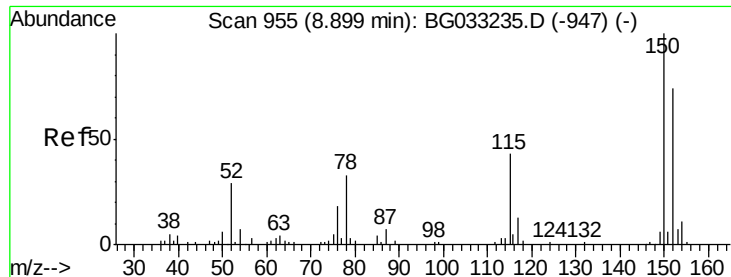


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.85 min Scan# 947
 Delta R.T. -0.01 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33

Instrument :
 BNA_G
 ClientSampleId :
 PB108084BL

Tot Ion:152 Resp: 40270
 Ion Ratio Lower Upper
 152 100
 150 153.7 126.6 189.8
 115 56.1 53.0 79.4

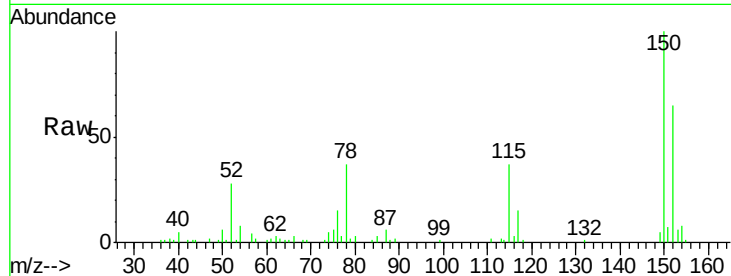


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

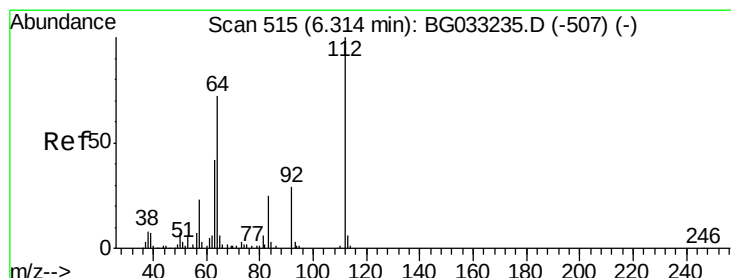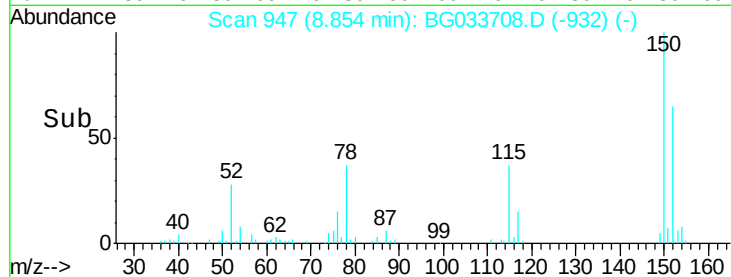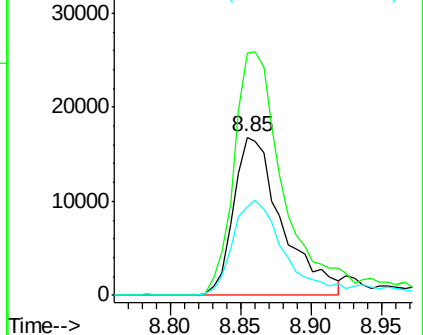



#5


2-Fluorophenol
 Concen: 169.002 ng
 RT: 6.29 min Scan# 510
 Delta R.T. -0.00 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33

Tgt Ion:112 Resp: 362947
 Ion Ratio Lower Upper
 112 100
 64 75.8 56.3 84.5
 63 44.2 30.1 45.1

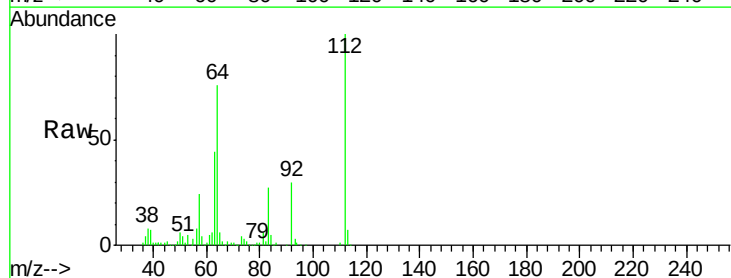

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

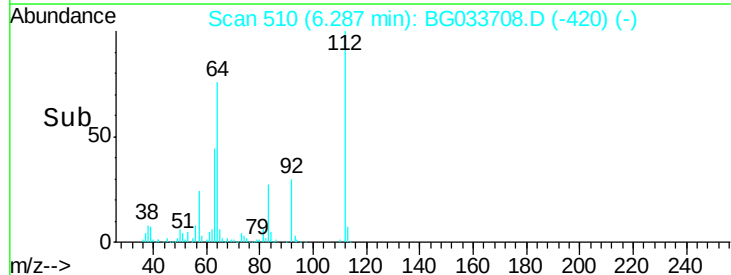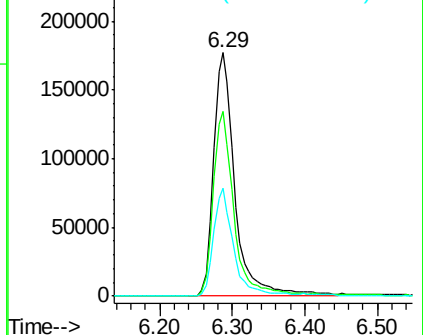

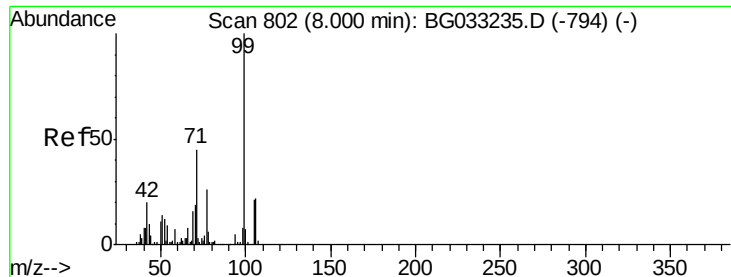

#7

Phenol-d6

Concen: 140.425 ng

RT: 7.97 min Scan# 796

Delta R.T. -0.00 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33

Instrument :

BNA_G

ClientSampleId :

PB108084BL


Tot Ion: 99 Resp: 518168

Ion Ratio Lower Upper




99 100

42 20.4 14.1 21.1

71 42.8 26.1 39.1#

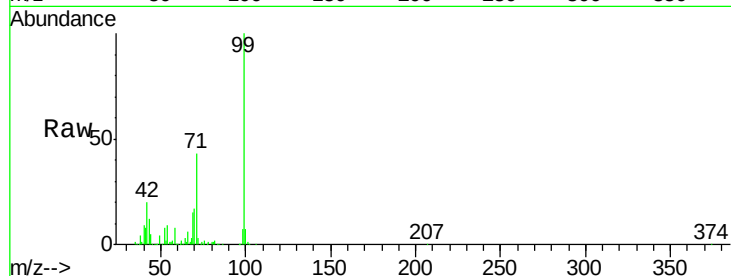

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

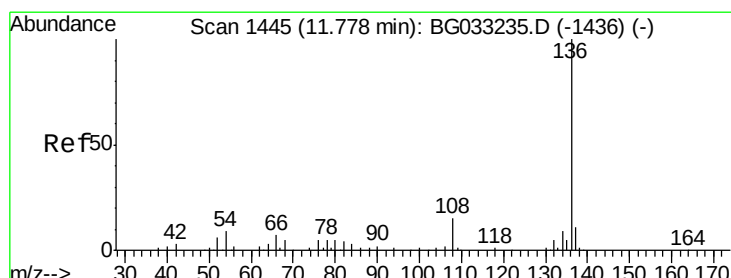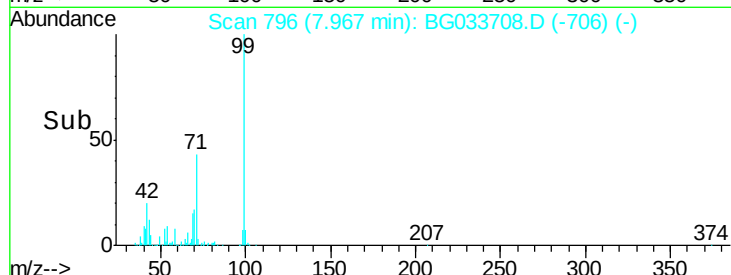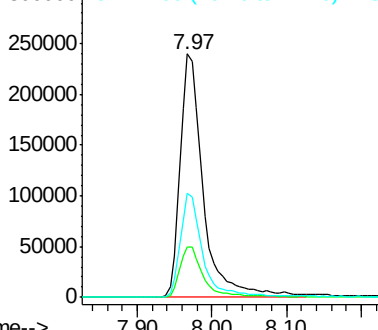

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.74 min Scan# 1438

Delta R.T. -0.00 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33

Tgt Ion: 136 Resp: 169994


Ion Ratio Lower Upper

136 100



137 10.7 9.2 13.8


54 10.9 10.3 15.5

68 5.7 4.5 6.7

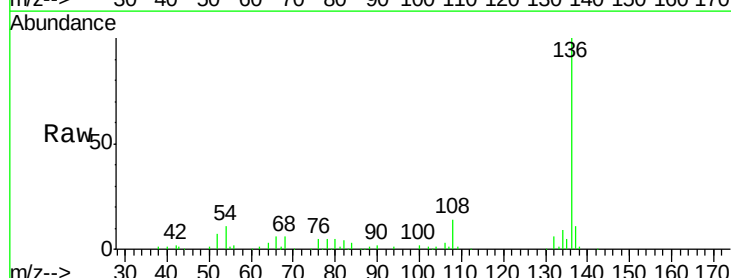

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



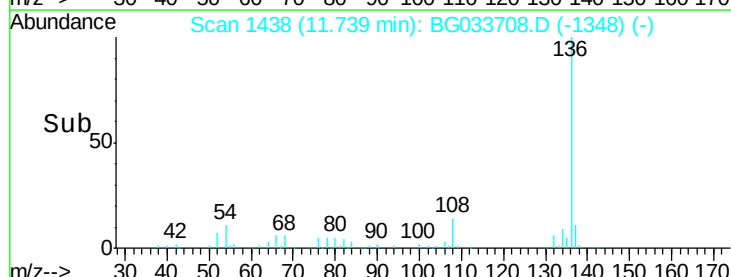
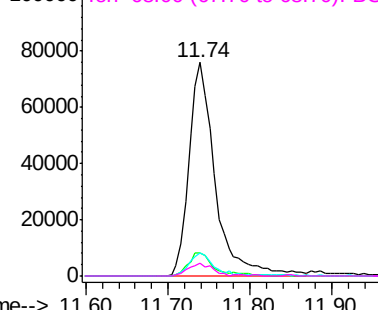


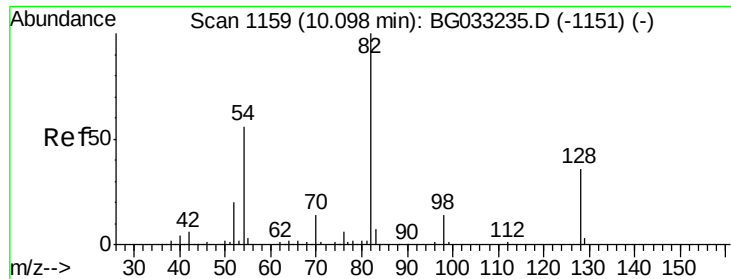

#23
 Nitrobenzene-d5
 Concen: 90.278 ng
 RT: 10.06 min Scan# 1152
 Delta R.T. -0.00 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33




Instrument :
 BNA_G
 ClientSampleId :
 PB108084BL


Tot Ion: 82 Resp: 334029
 Ion Ratio Lower Upper
 82 100
 128 35.2 29.7 44.5
 54 56.7 43.1 64.7

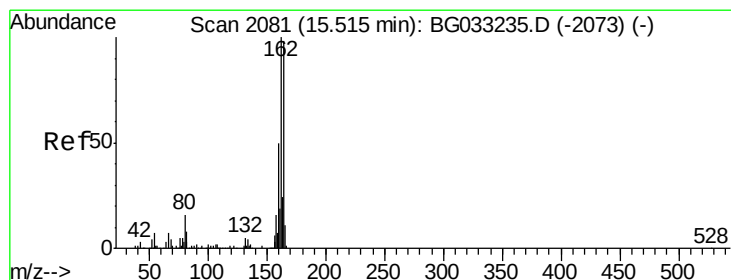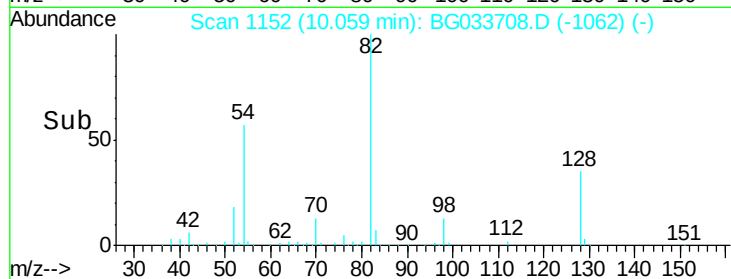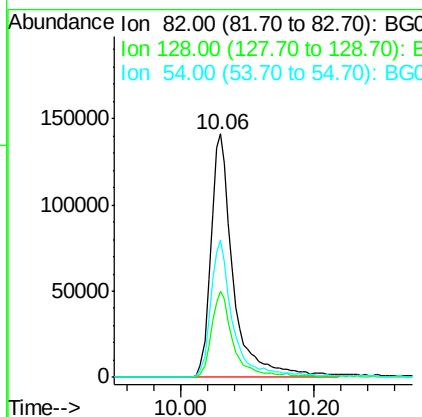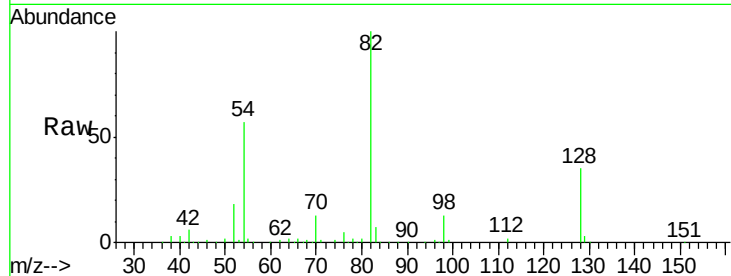

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2073
 Delta R.T. -0.01 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33

Tgt Ion:164 Resp: 119999
 Ion Ratio Lower Upper
 164 100
 162 96.8 78.8 118.2
 160 44.1 35.4 53.0

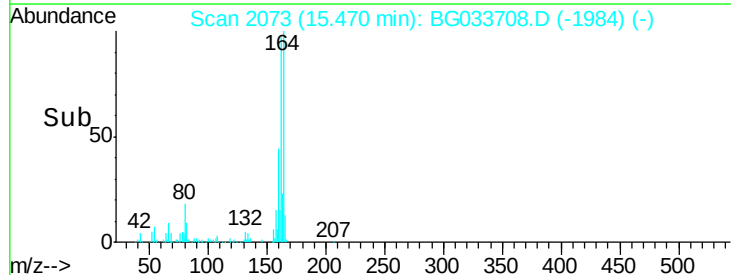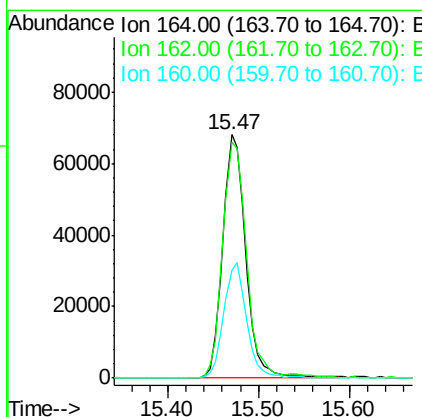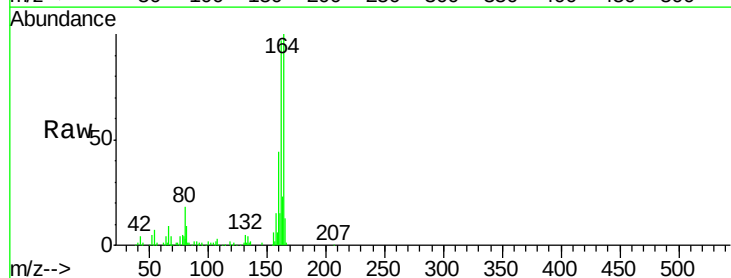


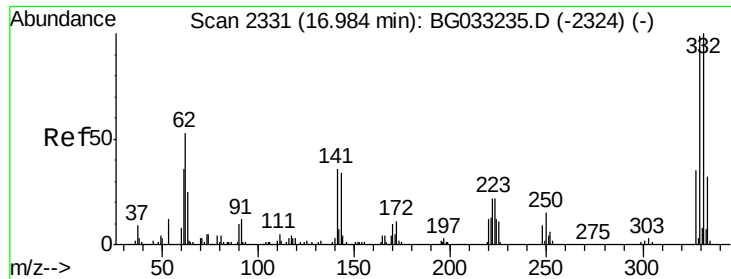

#41
 2,4,6-Tribromophenol
 Concen: 113.944 ng
 RT: 16.95 min Scan# 2325
 Delta R.T. -0.00 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33

Instrument :
 BNA_G
 ClientSampleId :
 PB108084BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.7	77.0	115.6
141	38.2	25.2	37.8#



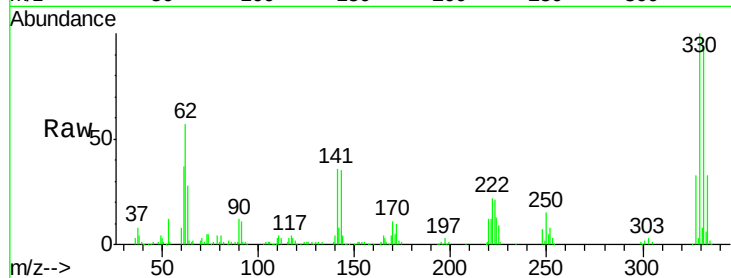


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

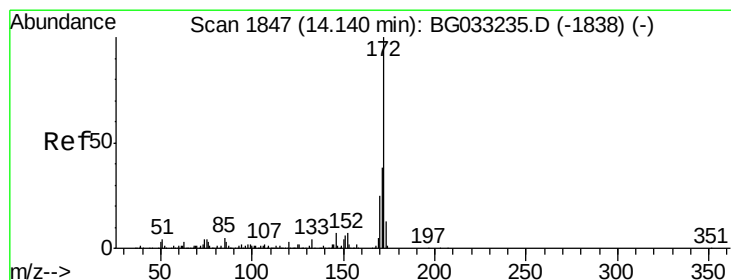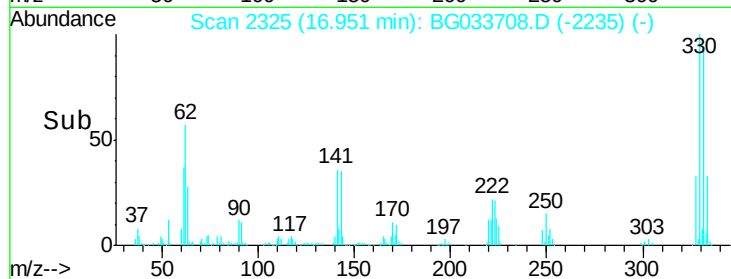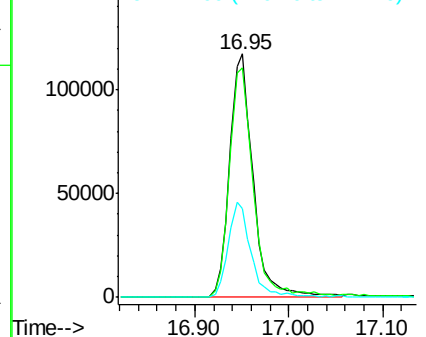

#44
 2-Fluorobiphenyl
 Concen: 89.596 ng
 RT: 14.10 min Scan# 1840
 Delta R.T. -0.00 min
 Lab File: BG033708.D
 Acq: 10 Apr 2018 9:33

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.4	30.0	45.0
170	24.8	19.5	29.3


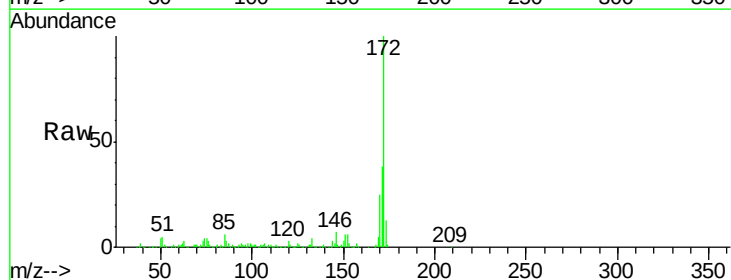



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

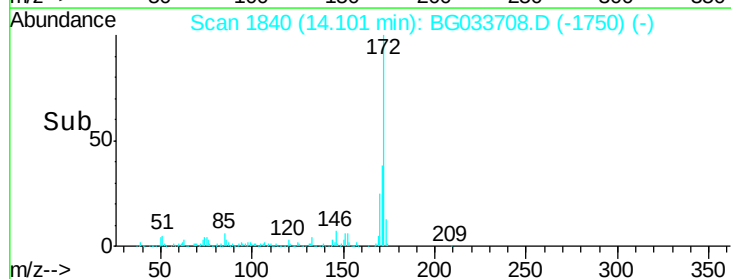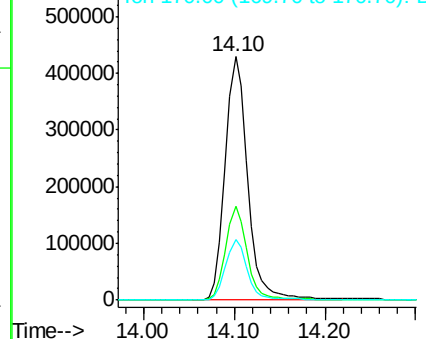

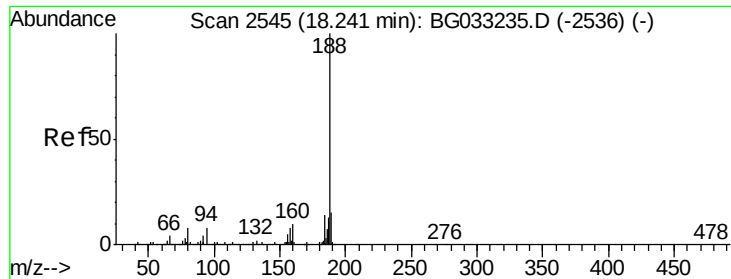

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.20 min Scan# 2538

Delta R.T. -0.01 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33

Instrument :

BNA_G

ClientSampleId :

PB108084BL


Tot Ion:188 Resp: 326436

Ion Ratio Lower Upper

188 100

94 7.4 6.9 10.3




80 8.4 7.7 11.5

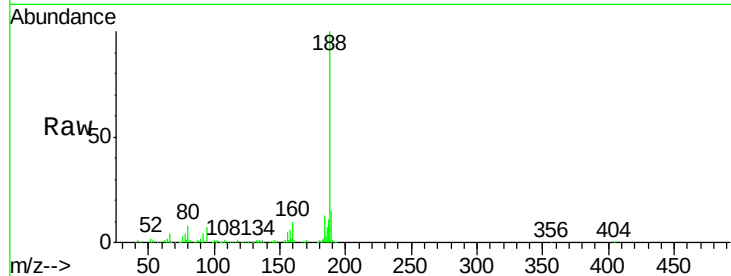

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

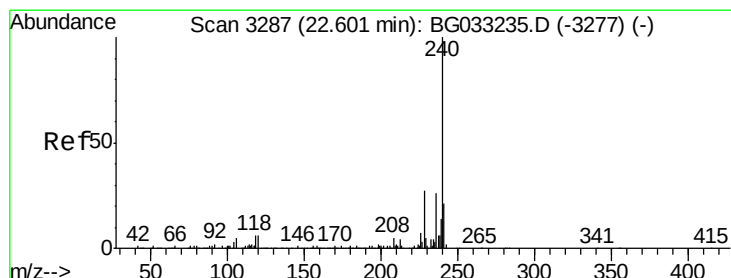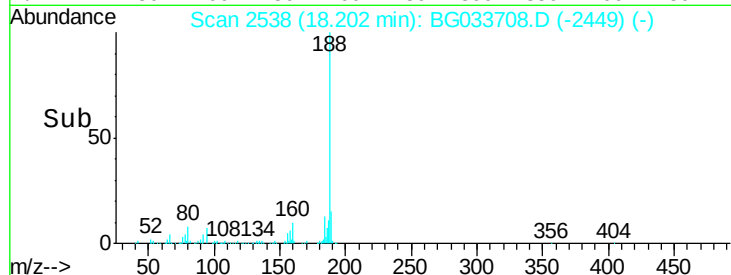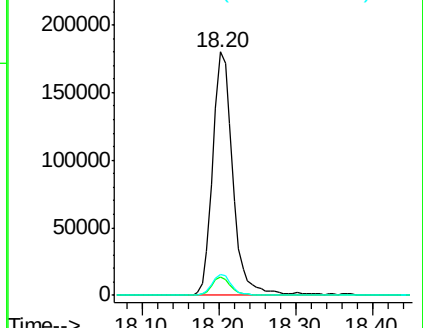

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.54 min Scan# 3277

Delta R.T. -0.02 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33


Tgt Ion:240 Resp: 333509

Ion Ratio Lower Upper

240 100

120 6.8 6.8 10.2



236 26.5 20.9 31.3

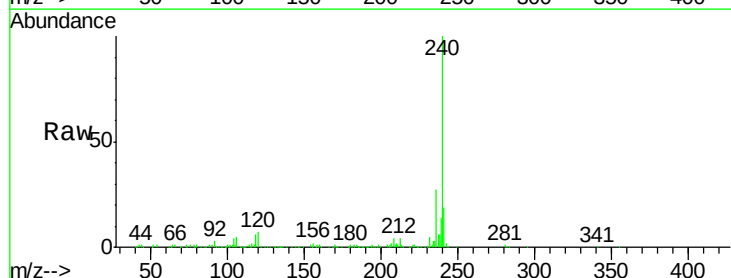


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

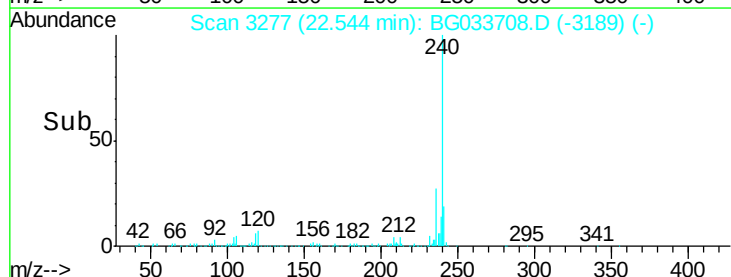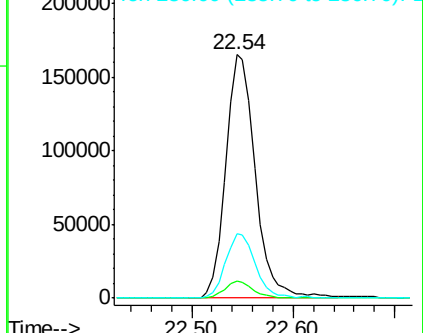

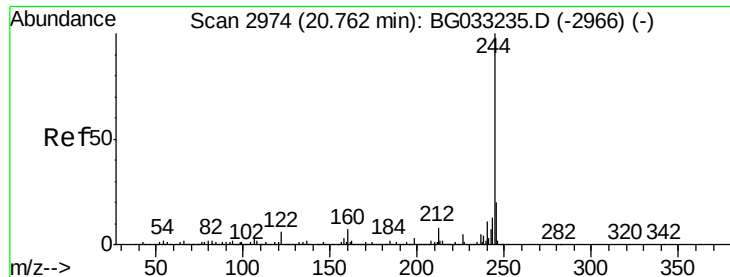

#78

Terphenyl-d14

Concen: 87.541 ng

RT: 20.72 min Scan# 2967

Delta R.T. -0.00 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33

Instrument :

BNA_G

ClientSampleId :

PB108084BL


Tot Ion:244 Resp: 1365174

Ion Ratio Lower Upper

244 100

212 8.7 5.8 8.8




122 7.8 7.0 10.4

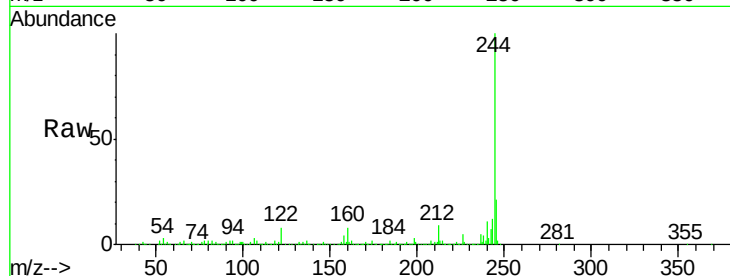

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

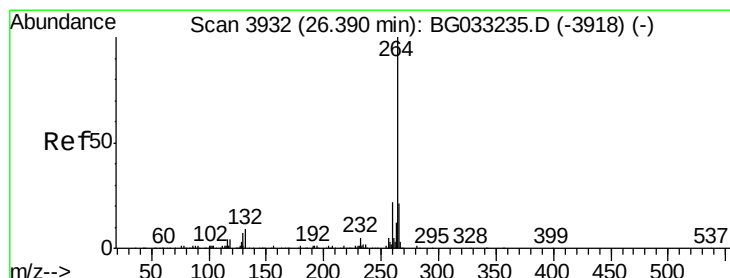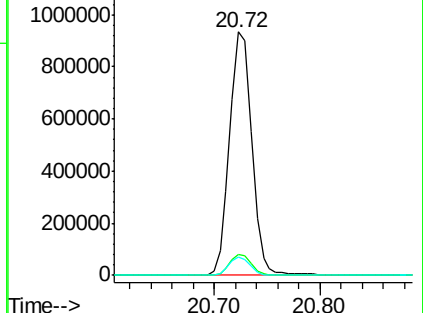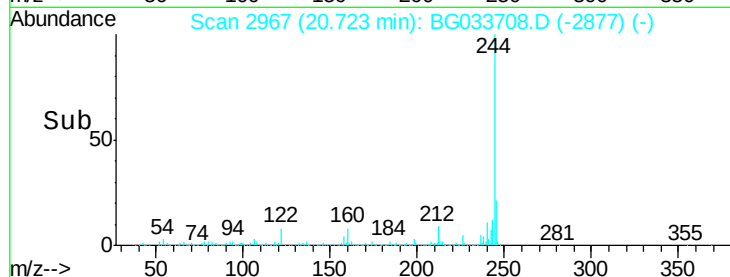

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.30 min Scan# 3917

Delta R.T. -0.02 min

Lab File: BG033708.D

Acq: 10 Apr 2018 9:33


Tgt Ion:264 Resp: 354861

Ion Ratio Lower Upper

264 100

260 20.6 17.4 26.0

265 23.3 17.7 26.5

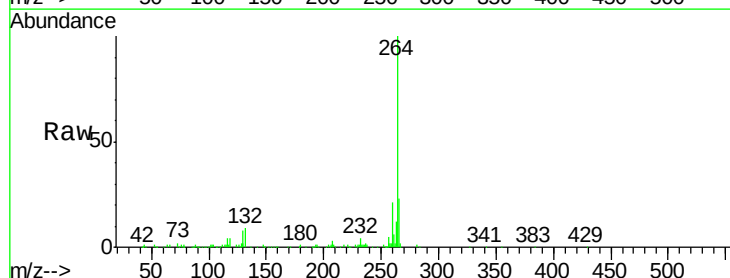

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

