


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040919\
 Data File : BG040393.D
 Acq On : 9 Apr 2019 11:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

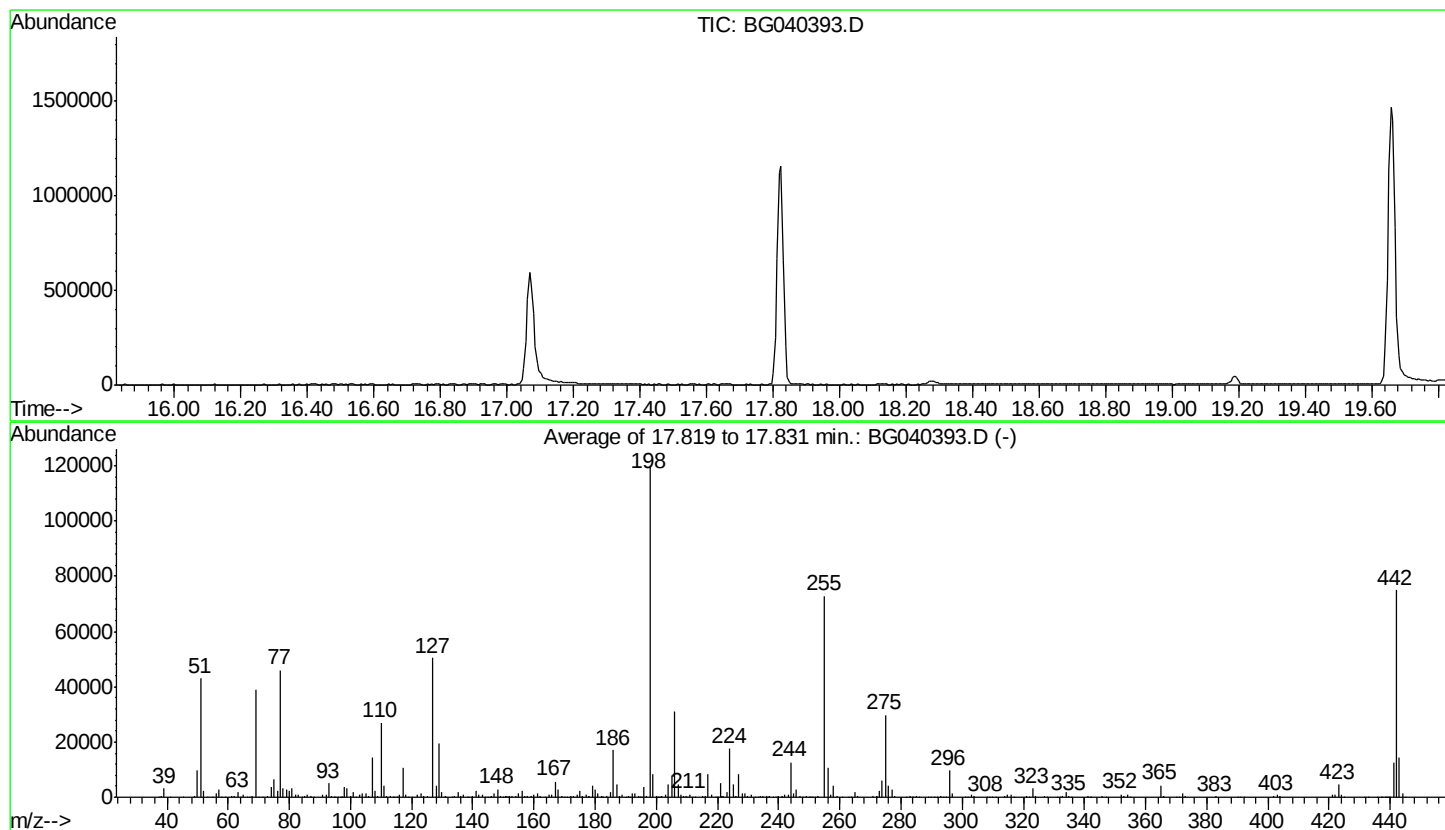

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	43098	PASS
68	69	0.00	2	0.7	284	PASS
69	198	0.00	100	32.3	38752	PASS
70	69	0.00	2	0.5	201	PASS
127	198	10	80	41.9	50320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120101	PASS
199	198	5	9	7.1	8562	PASS
275	198	10	60	24.8	29730	PASS
365	198	1	100	3.6	4320	PASS
441	198	0.01	100	10.5	12576	PASS
442	198	50	100	62.5	75016	PASS
443	442	15	24	19.1	14346	PASS