
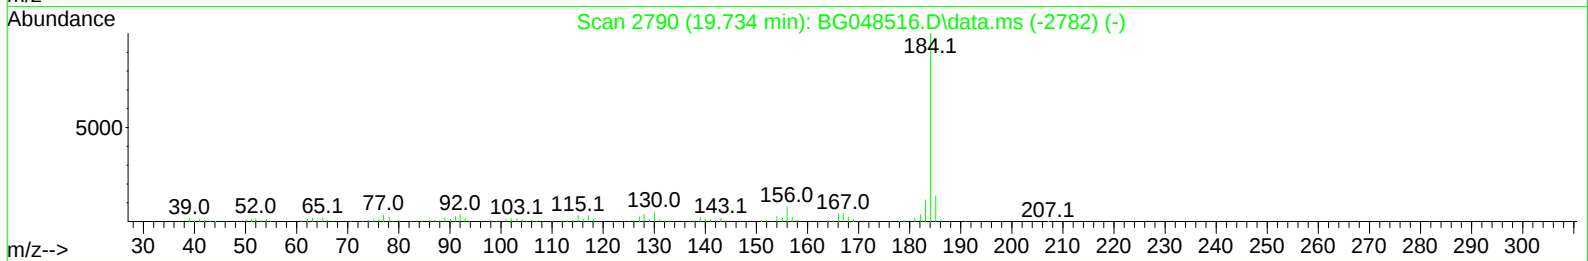
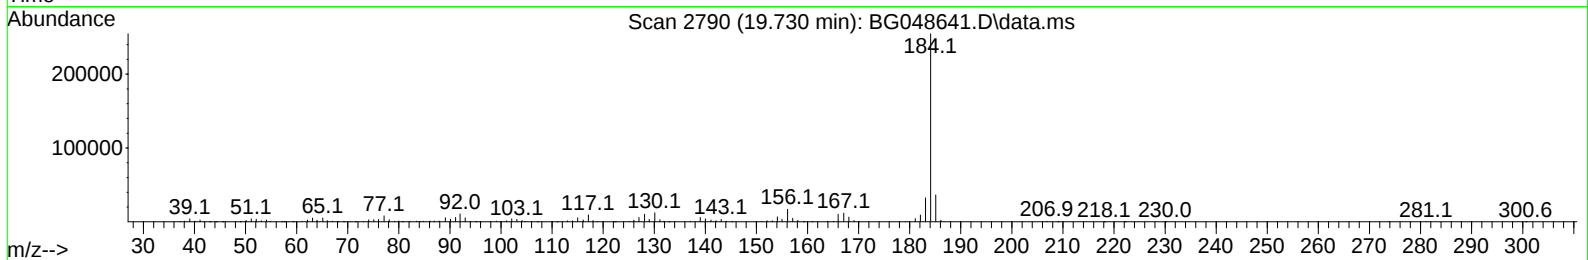


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040921\
Data File : BG048641.D
Acq On : 9 Apr 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 12:48:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

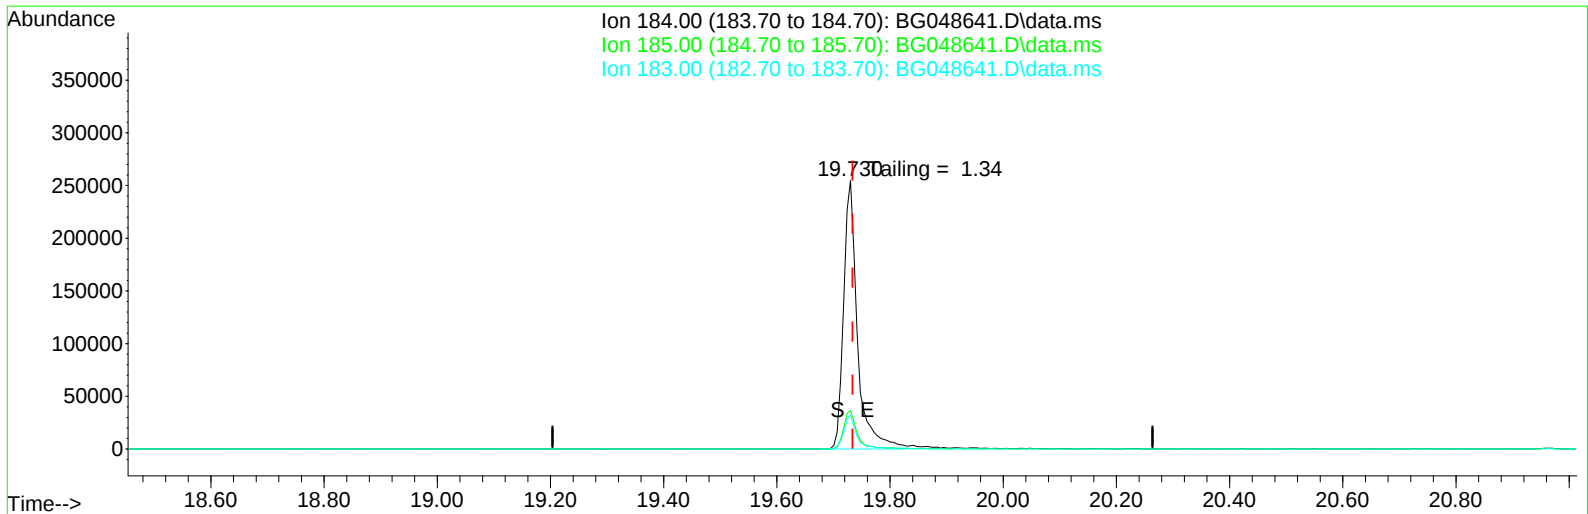

TIC: BG048641.D\data.ms

(77) Benzidine




19.730min (-0.004) 206613.75 ng

response 433787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.34
183.00	11.50	12.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040921\
Data File : BG048641.D
Acq On : 9 Apr 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 12:48:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

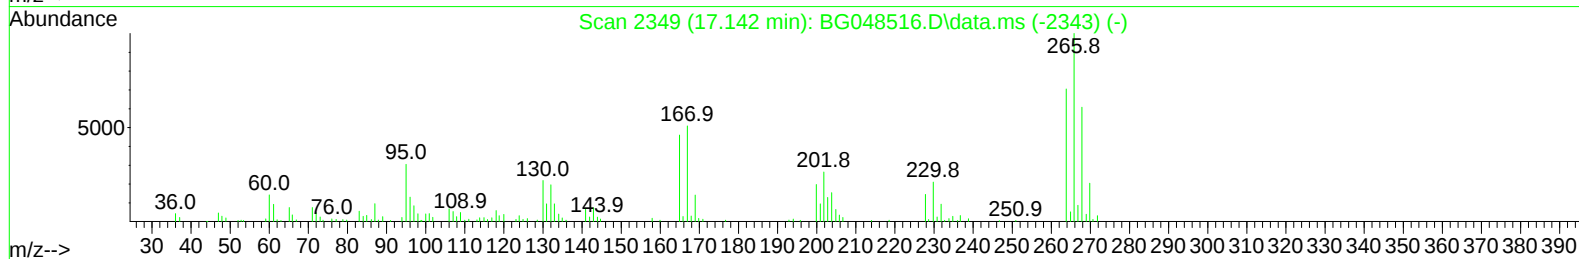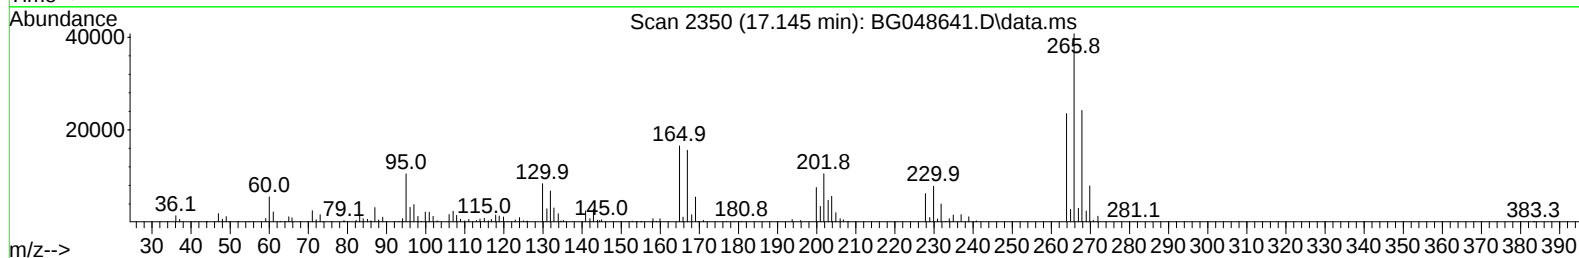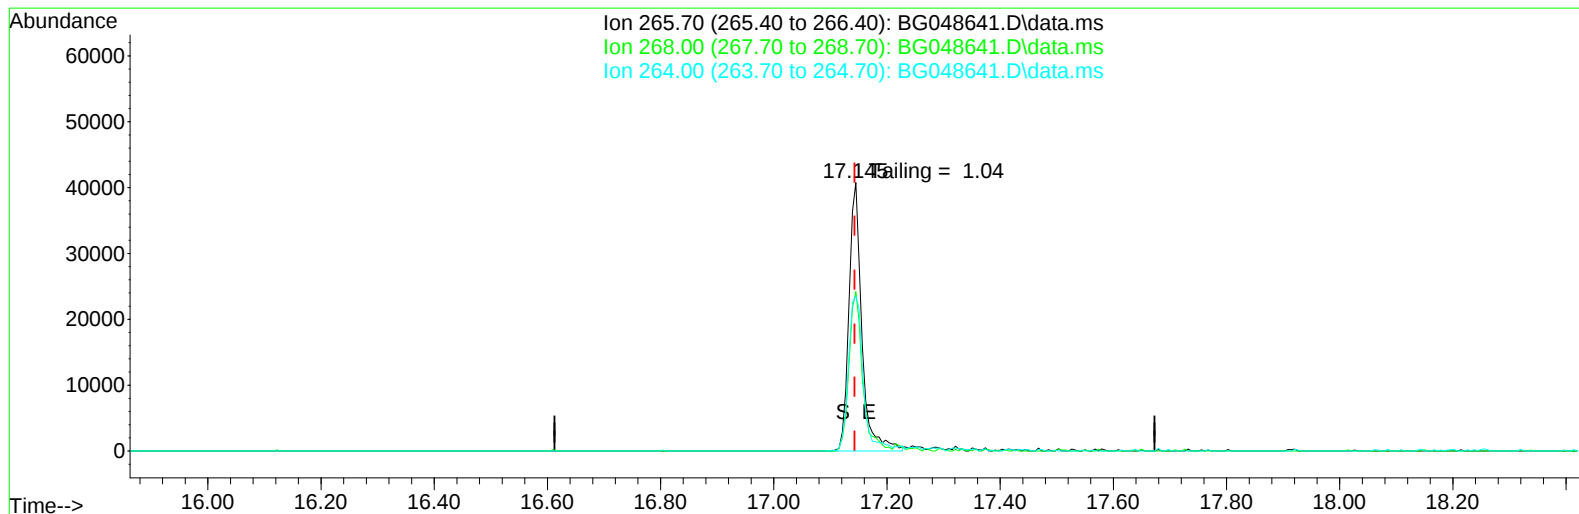

TIC: BG048641.D\data.ms

(70) Pentachlorophenol (C)

17.145min (+ 0.002) 92995.02 ng

response 64896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.39
264.00	70.50	57.70
0.00	0.00	0.00