

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040921\  
 Data File : BG048643.D  
 Acq On : 9 Apr 2021 13:15  
 Operator : CG/JU  
 Sample : PB135641BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB135641BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048643.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.633       | 382           | 390         | 403          | rVB      | 398275         | 635881        | 27.44%          | 8.422%        |
| 2         | 7.242       | 656           | 664         | 672          | rBV      | 398904         | 662295        | 28.58%          | 8.772%        |
| 3         | 8.088       | 801           | 808         | 815          | rBV      | 78613          | 132420        | 5.72%           | 1.754%        |
| 4         | 9.258       | 999           | 1007        | 1019         | rBV      | 244752         | 441193        | 19.04%          | 5.843%        |
| 5         | 10.915      | 1282          | 1289        | 1298         | rBV      | 99260          | 171945        | 7.42%           | 2.277%        |
| 6         | 13.359      | 1698          | 1705        | 1715         | rBV      | 606070         | 962731        | 41.55%          | 12.751%       |
| 7         | 14.739      | 1934          | 1940        | 1947         | rBV      | 130826         | 217883        | 9.40%           | 2.886%        |
| 8         | 16.232      | 2187          | 2194        | 2208         | rBV      | 508821         | 861384        | 37.18%          | 11.409%       |
| 9         | 17.495      | 2403          | 2409        | 2419         | rBV      | 205047         | 336696        | 14.53%          | 4.459%        |
| 10        | 20.104      | 2847          | 2853        | 2870         | rBV      | 1741606        | 2317049       | 100.00%         | 30.689%       |
| 11        | 20.691      | 2945          | 2953        | 2954         | rBV5     | 15922          | 28081         | 1.21%           | 0.372%        |
| 12        | 21.790      | 3133          | 3140        | 3148         | rBV2     | 224077         | 417362        | 18.01%          | 5.528%        |
| 13        | 25.133      | 3697          | 3709        | 3721         | rBV2     | 103850         | 365231        | 15.76%          | 4.837%        |




Sum of corrected areas: 7550151

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040921\  
Data File : BG048643.D  
Acq On : 9 Apr 2021 13:15  
Operator : CG/JU  
Sample : PB135641BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135641BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

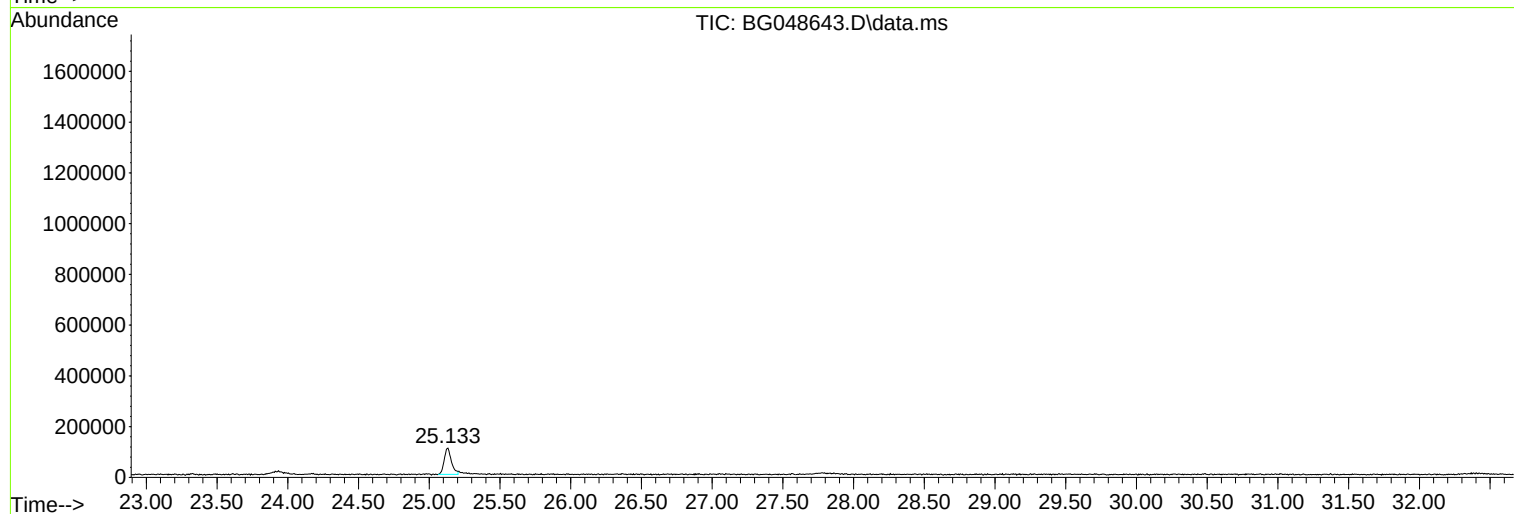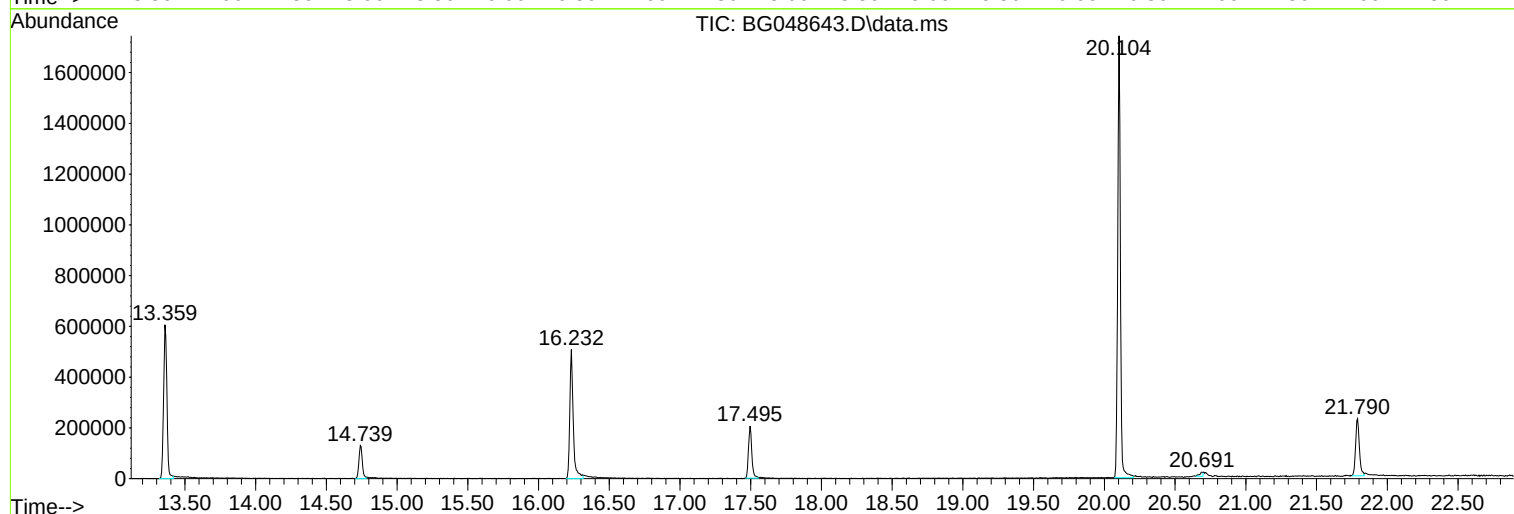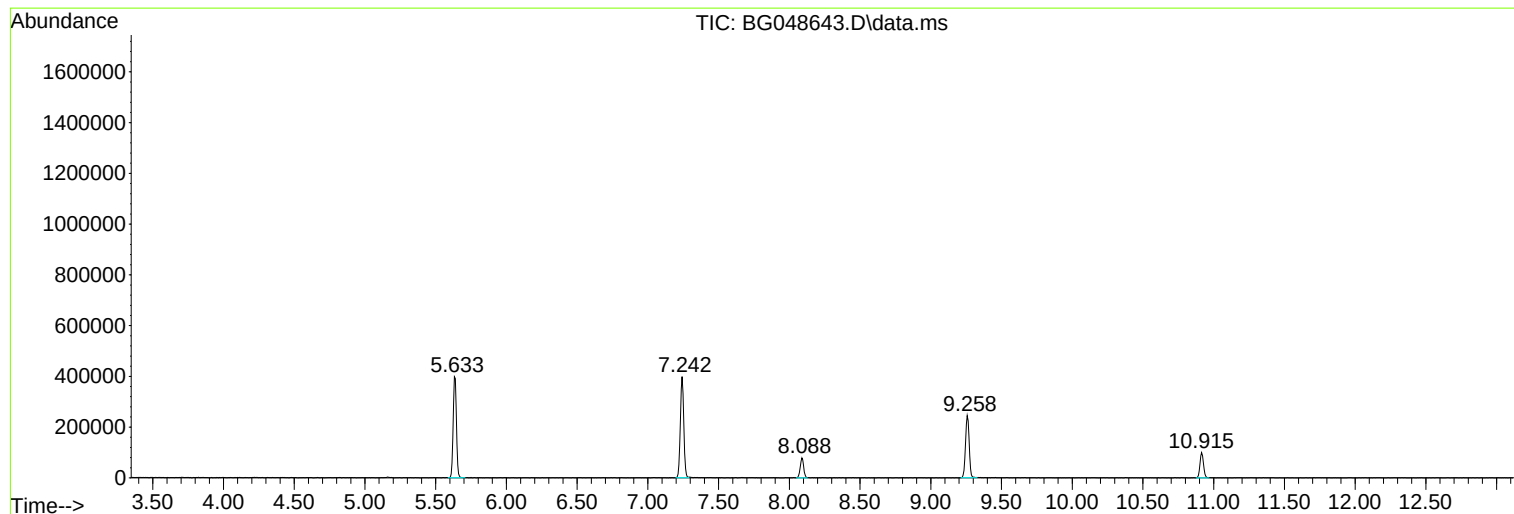

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040921\  
Data File : BG048643.D  
Acq On : 9 Apr 2021 13:15  
Operator : CG/JU  
Sample : PB135641BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135641BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040921\  
Data File : BG048643.D  
Acq On : 9 Apr 2021 13:15  
Operator : CG/JU  
Sample : PB135641BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135641BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|