
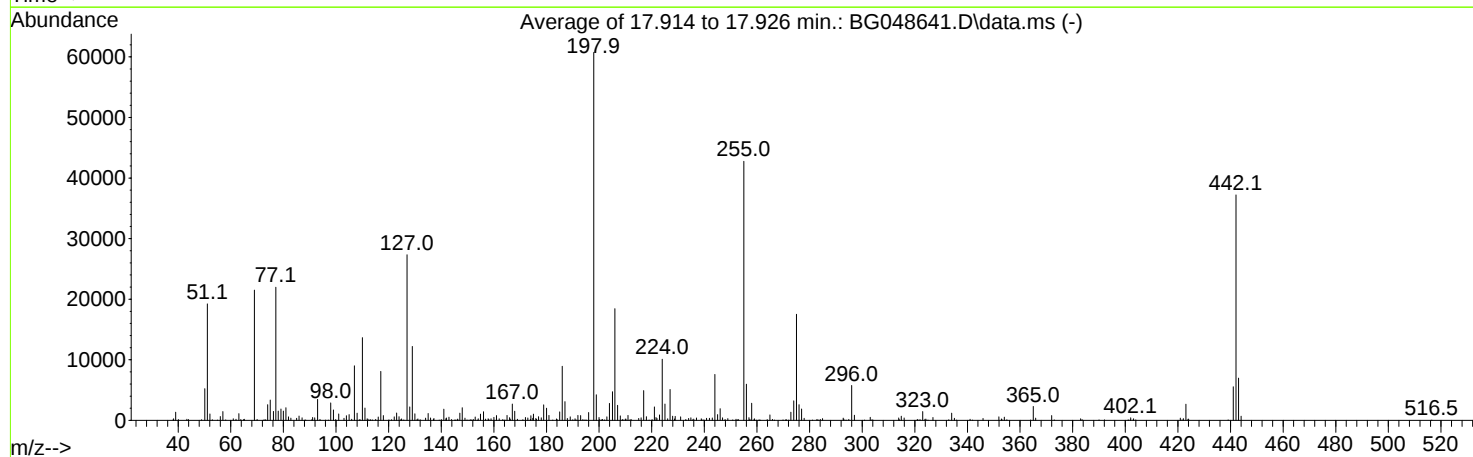


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040921\
 Data File : BG048641.D
 Acq On : 9 Apr 2021 11:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:06:00 2021

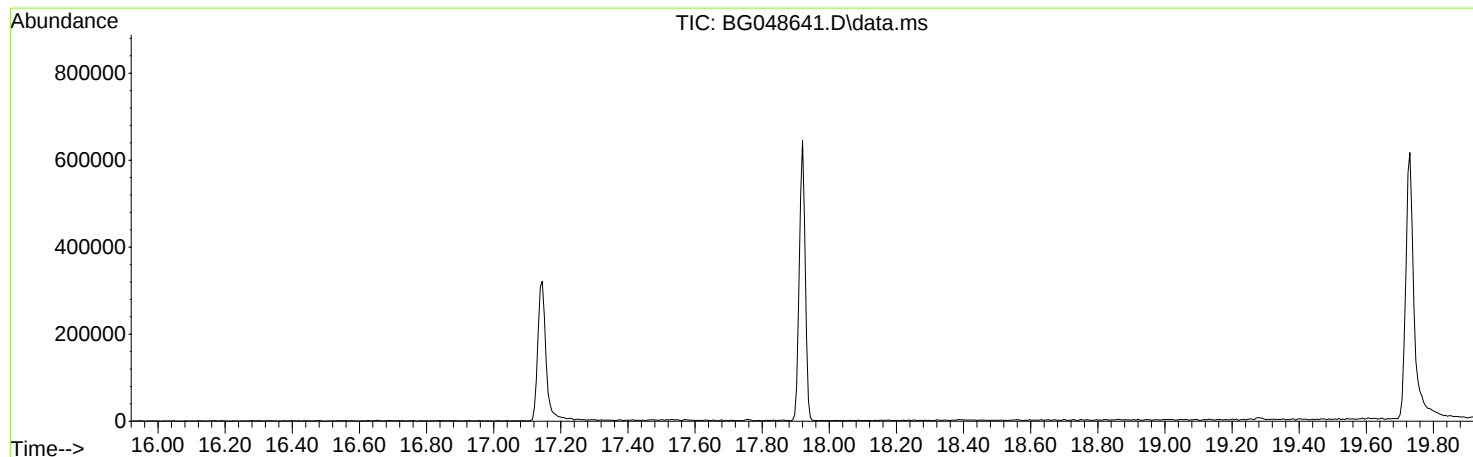

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	19224	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	21493	PASS
70	69	0.00	2	0.8	173	PASS
127	198	10	80	45.0	27339	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60723	PASS
199	198	5	9	7.0	4239	PASS
275	198	10	60	28.9	17524	PASS
365	198	1	100	3.8	2300	PASS
441	198	0.01	100	9.1	5541	PASS
442	198	50	100	61.3	37203	PASS
443	442	15	24	18.8	6981	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/9/2021	BNA_G	<u>BG048641.D</u>
Compound Name	Response	Retention Time
DDT	220330	20.96
DDD	4552	20.51
DDE	685	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5237	225567	2.32

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040921\
Data File : BG048641.D
Acq On : 9 Apr 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 09 12:48:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

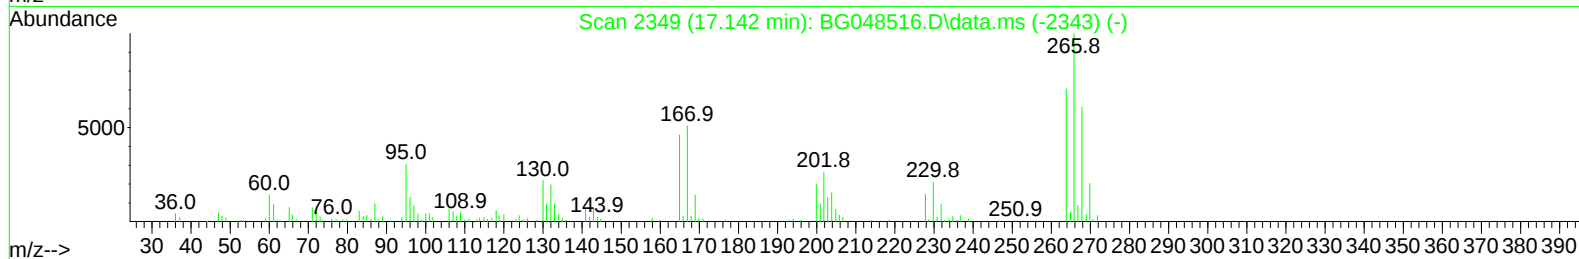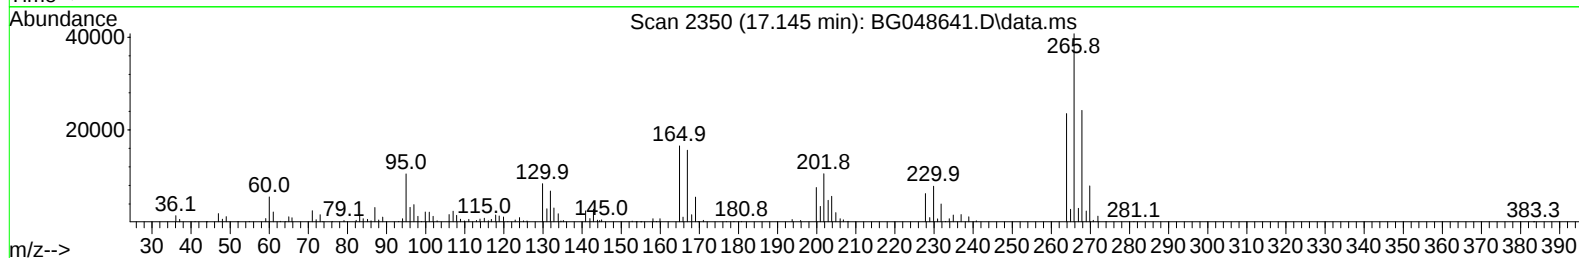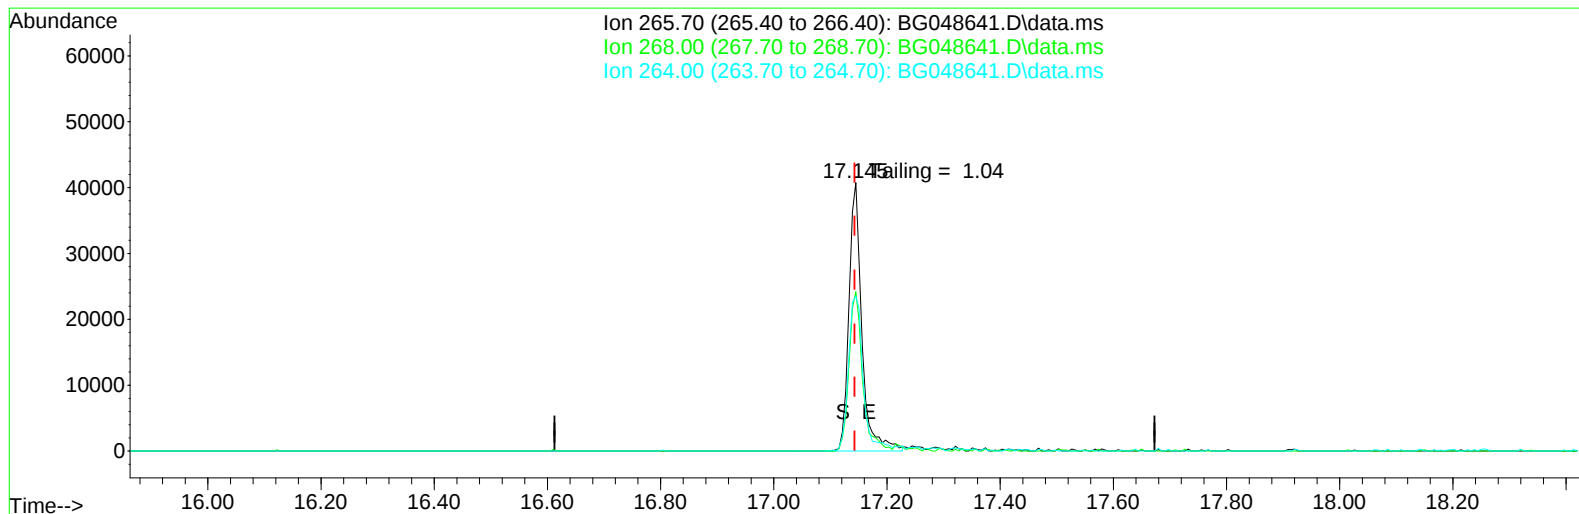

TIC: BG048641.D\data.ms

(70) Pentachlorophenol (C)

17.145min (+ 0.002) 92995.02 ng




response 64896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.39
264.00	70.50	57.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040921\
Data File : BG048641.D
Acq On : 9 Apr 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 09 12:48:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

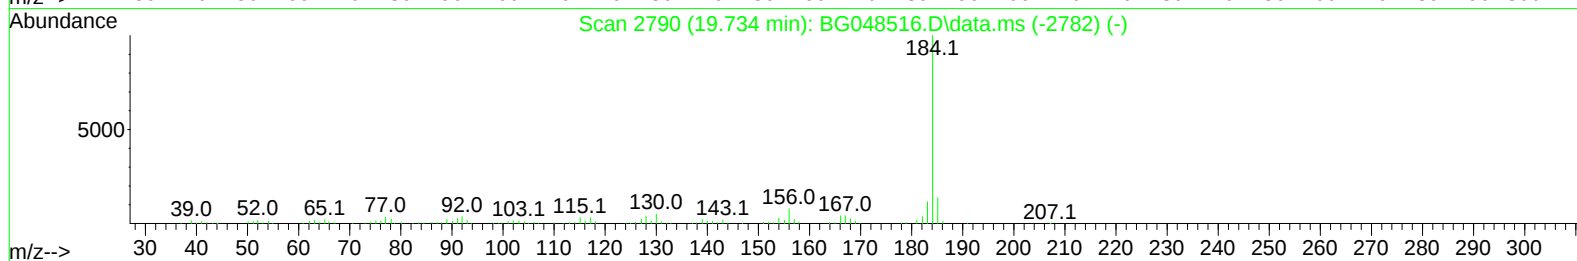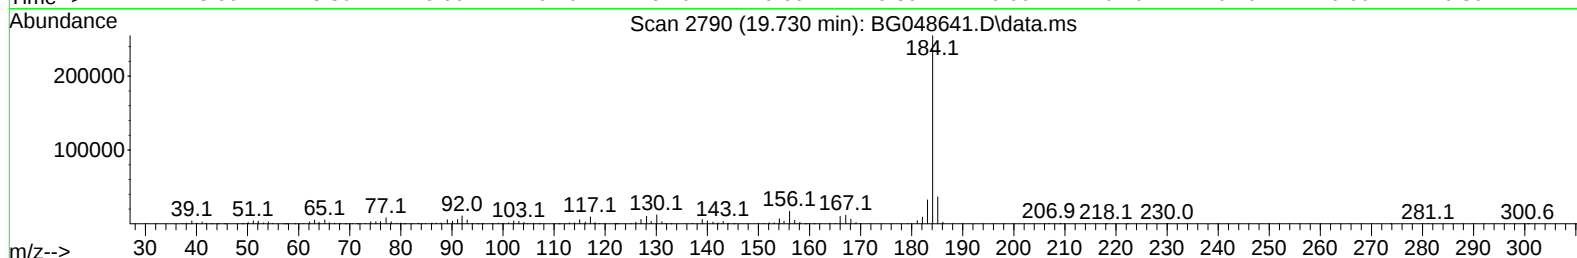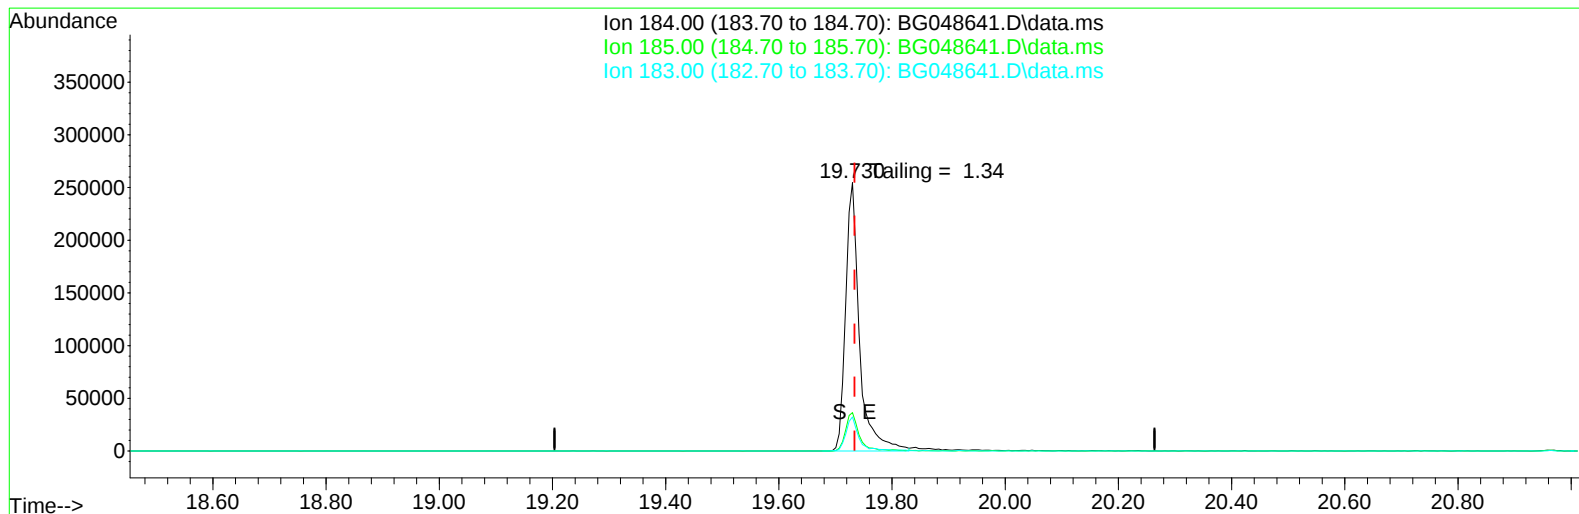

TIC: BG048641.D\data.ms

(77) Benzidine

19.730min (-0.004) 206613.75 ng

response 433787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.34
183.00	11.50	12.73
0.00	0.00	0.00