
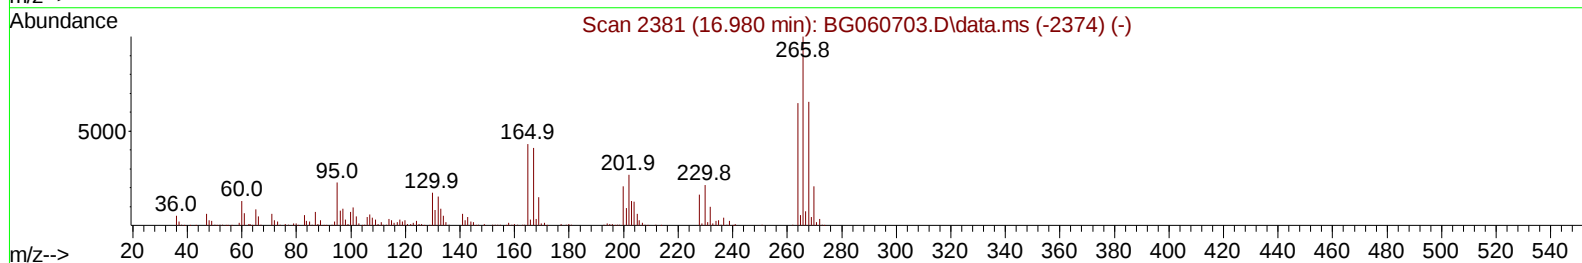
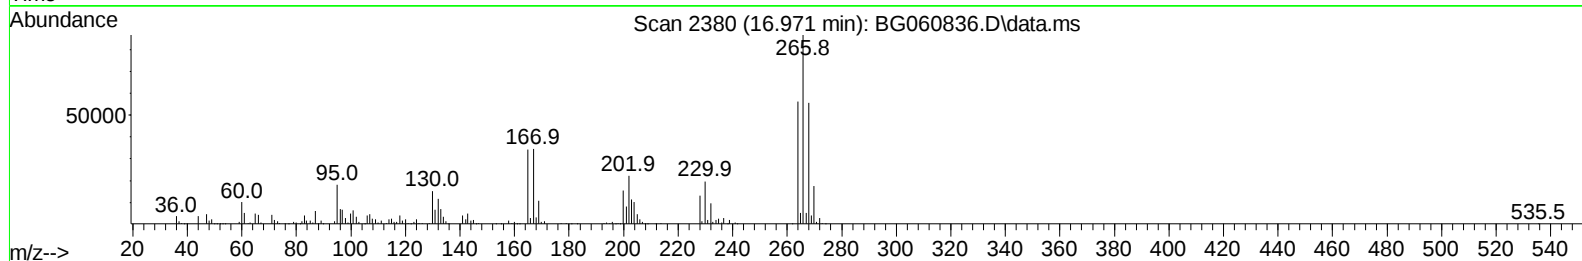


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040924\
Data File : BG060836.D
Acq On : 9 Apr 2024 8:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 23:47:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

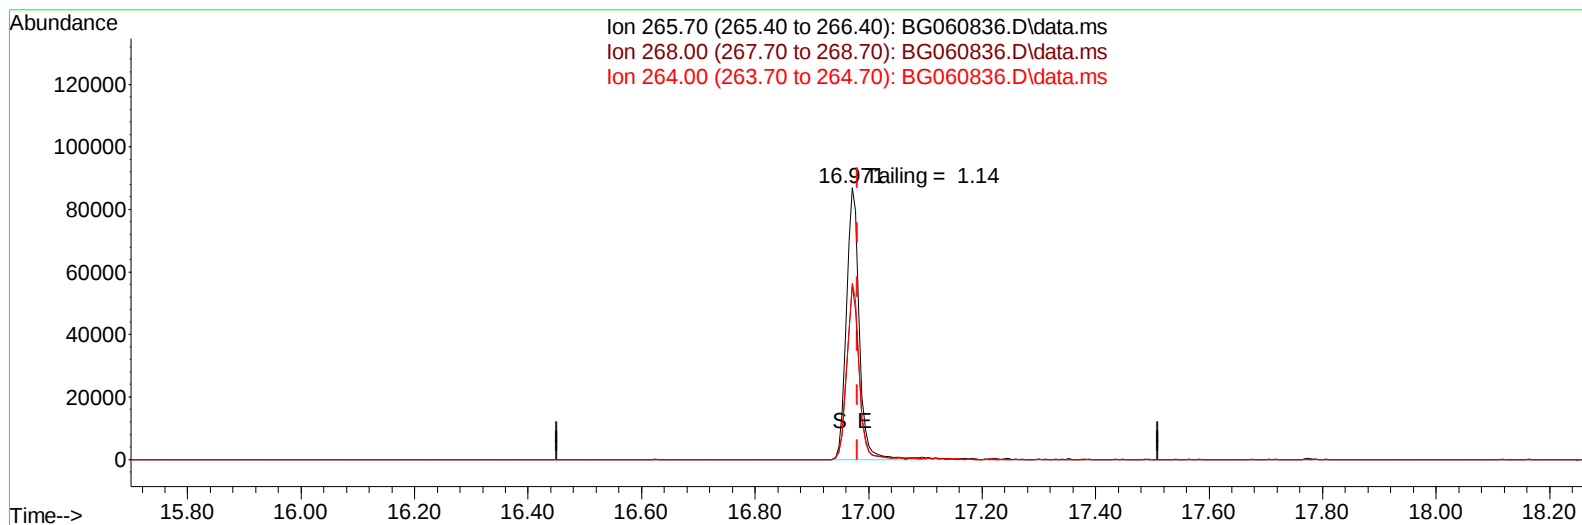

TIC: BG060836.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.009) 24008.43 ng

response 136579

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.13
264.00	64.70	64.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040924\
Data File : BG060836.D
Acq On : 9 Apr 2024 8:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 23:47:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

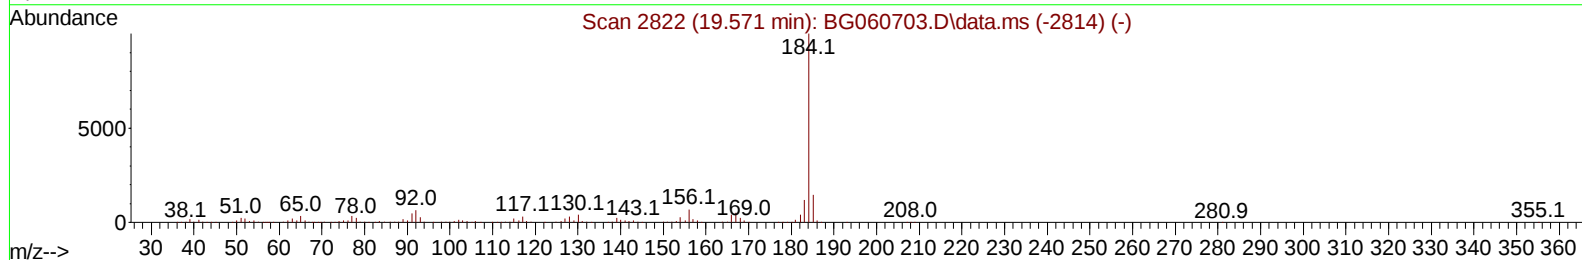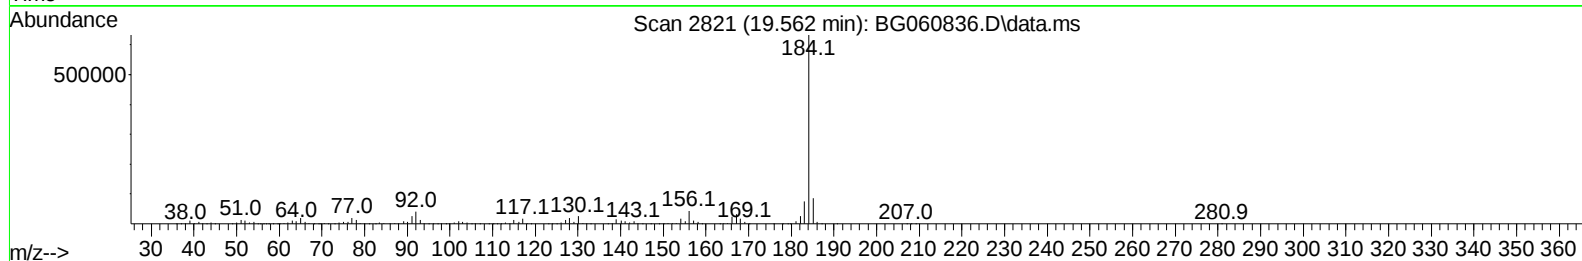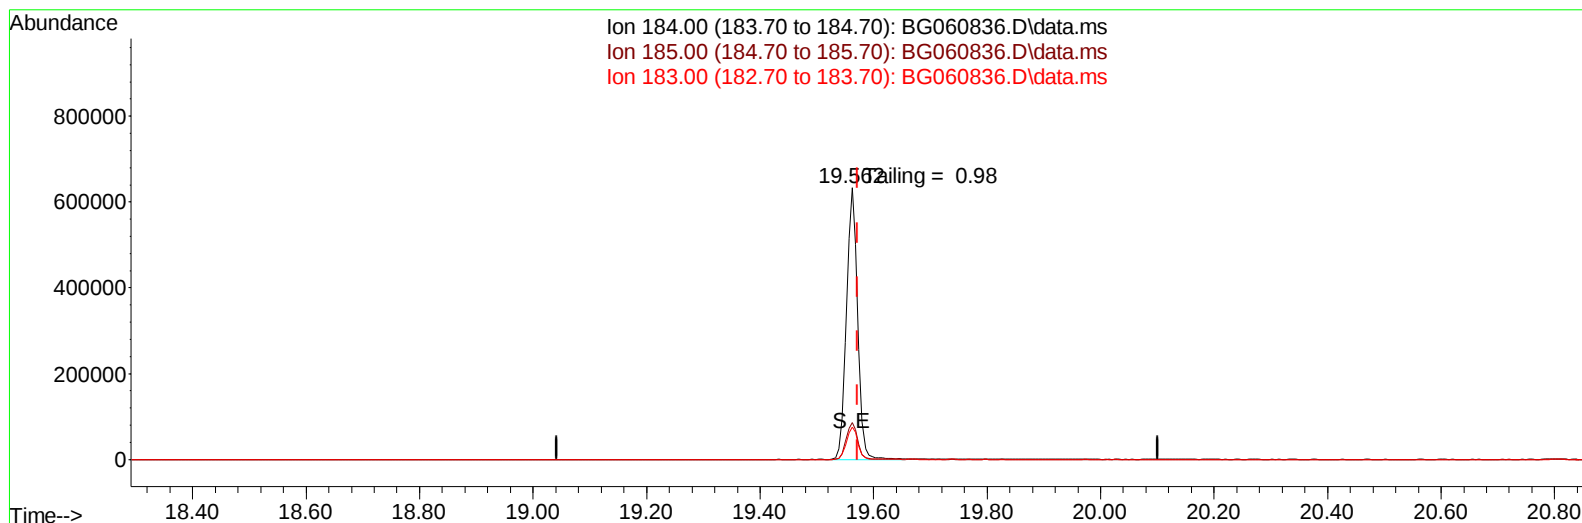

TIC: BG060836.D\data.ms

(77) Benzidine

19.562min (-0.009) 0.00 ng

response 868781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.68
183.00	11.90	11.85
0.00	0.00	0.00