


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040924\
Data File : BG060836.D
Acq On : 9 Apr 2024 8:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

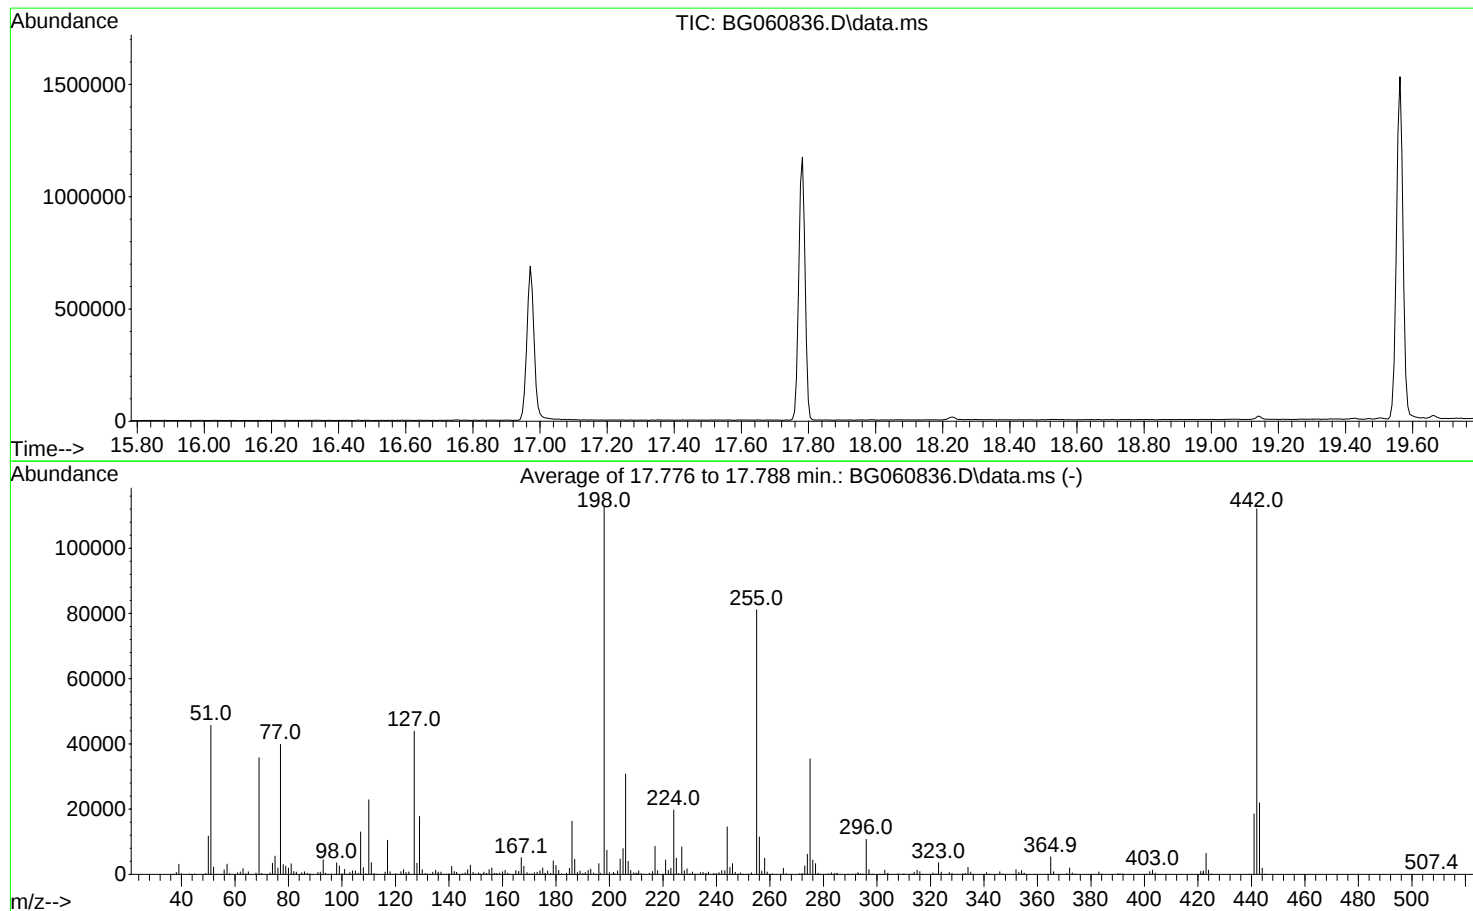




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	45696	PASS
68	69	0.00	2	1.2	421	PASS
69	198	0.00	100	31.7	35765	PASS
70	69	0.00	2	0.9	321	PASS
127	198	10	80	38.9	43912	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112789	PASS
199	198	5	9	6.6	7414	PASS
275	198	10	60	31.4	35443	PASS
365	198	1	100	4.8	5375	PASS
441	198	0.01	100	16.4	18533	PASS
442	442	50	100	100.0	112048	PASS
443	442	15	24	19.6	21933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040924\
 Data File : BG060836.D
 Acq On : 9 Apr 2024 8:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 09 23:47:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 30 03:12:26 2024
 Response via : Initial Calibration

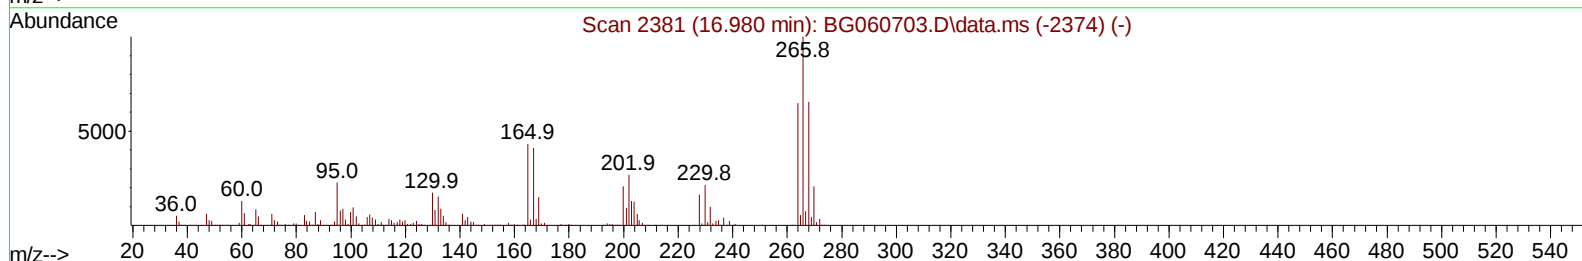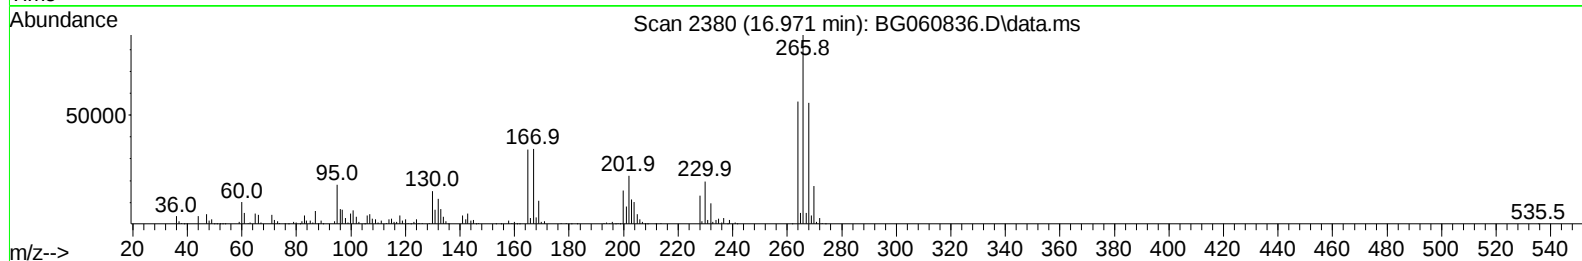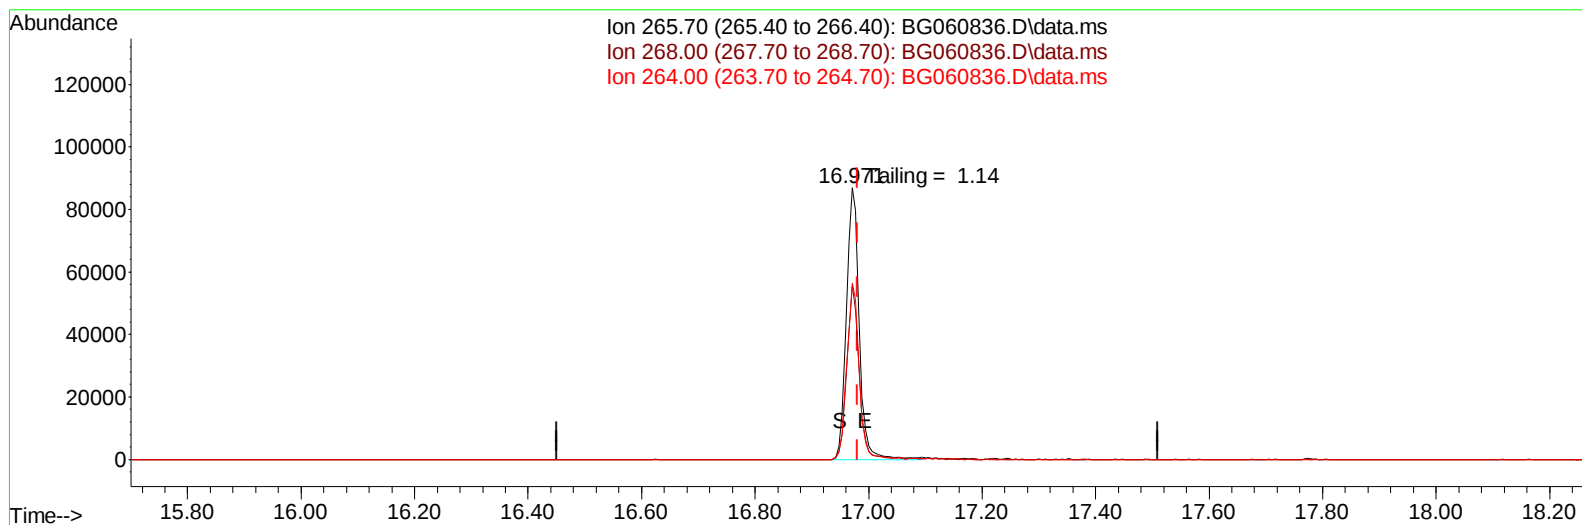

TIC: BG060836.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.009) 24008.43 ng




response 136579

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.13
264.00	64.70	64.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040924\
Data File : BG060836.D
Acq On : 9 Apr 2024 8:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 09 23:47:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

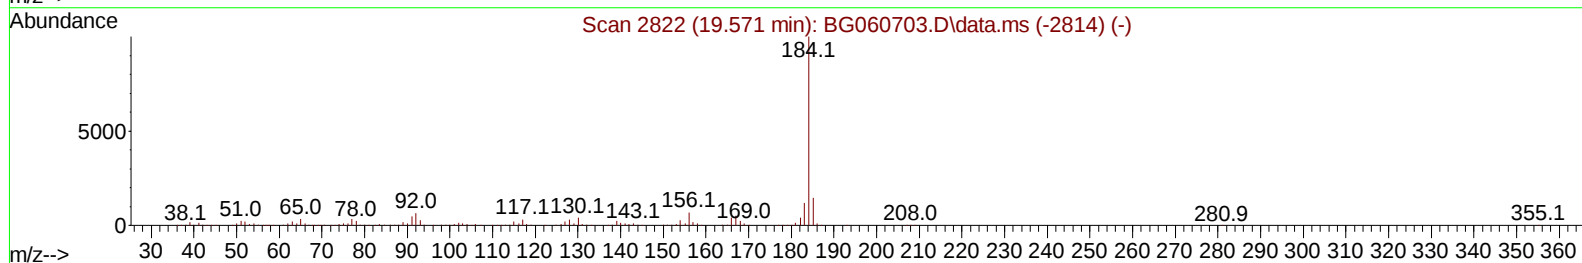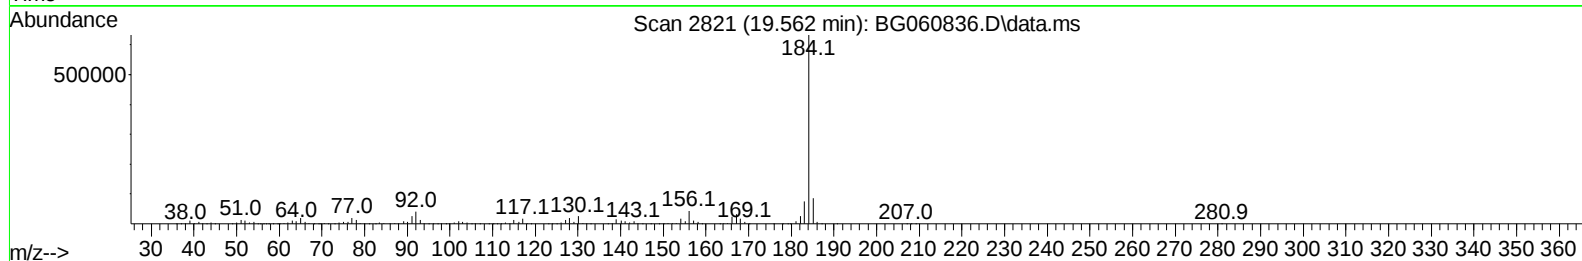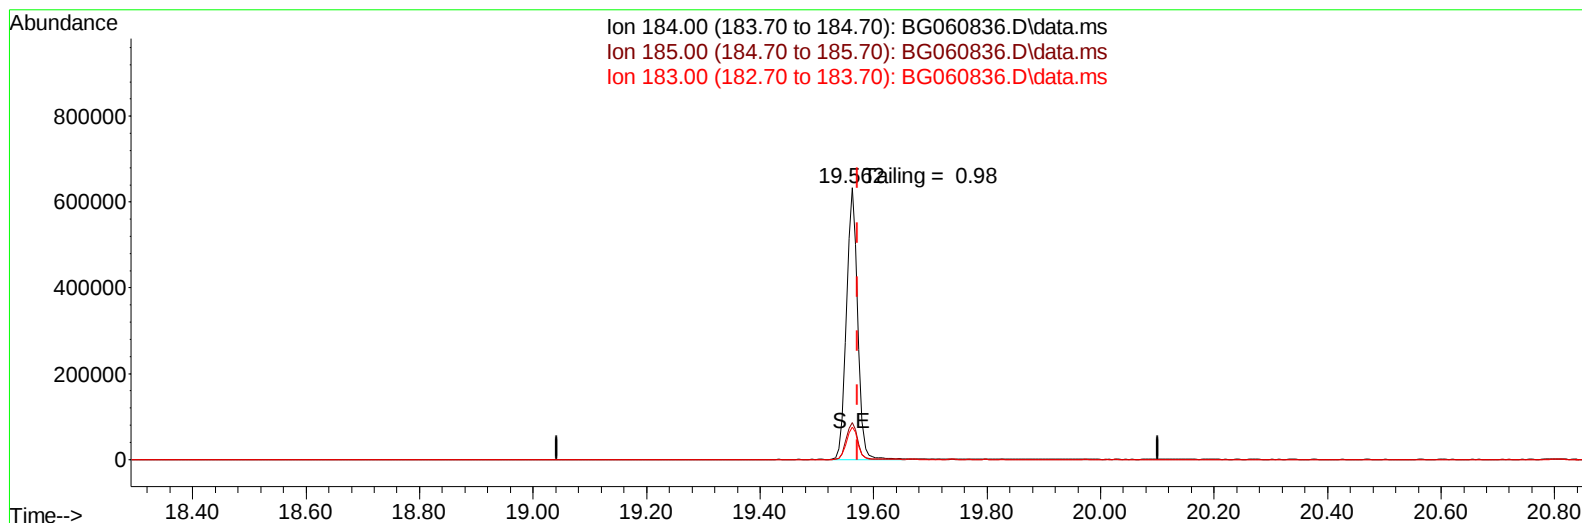

TIC: BG060836.D\data.ms

(77) Benzidine

19.562min (-0.009) 0.00 ng

response 868781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.68
183.00	11.90	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/9/2024	BNA_G	<u>BG060836.D</u>
Compound Name	Response	Retention Time
DDT	427917	20.802
DDD	11127	20.361
DDE	2258	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13385	441302	3.03

Instrument :
BNA_G
ClientSampleId :
DFTPP