

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041015\
 Data File : BG016325.D
 Acq On : 10 Apr 2015 18:55
 Operator : TP/IZ
 Sample : G1806-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GMW-02

Quant Time: Apr 11 03:39:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 11 03:24:57 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	66941	20.00	ng	0.00
21) Naphthalene-d8	10.48	136	299271	20.00	ng	0.00
38) Acenaphthene-d10	14.33	164	180680	20.00	ng	0.00
63) Phenanthrene-d10	17.07	188	375546	20.00	ng	0.00
75) Chrysene-d12	21.25	240	325529	20.00	ng	0.00
86) Perylene-d12	23.49	264	296143	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	220293	51.94	ng	0.00
7) Phenol-d6	6.88	99	179120	28.13	ng	0.00
23) Nitrobenzene-d5	8.85	82	449268	86.96	ng	0.00
41) 2,4,6-Tribromophenol	15.83	330	182900	149.68	ng	0.00
44) 2-Fluorobiphenyl	12.95	172	967898	91.21	ng	0.00
78) Terphenyl-d14	19.70	244	1098909	79.01	ng	0.00
Target Compounds						
83) Bis(2-ethylhexyl)phthalate	21.17	149	89479	5.94	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041015\
Data File : BG016325.D
Acq On : 10 Apr 2015 18:55
Operator : TP/IZ
Sample : G1806-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GMW-02

Quant Time: Apr 11 03:39:51 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 11 03:24:57 2015
Response via : Initial Calibration

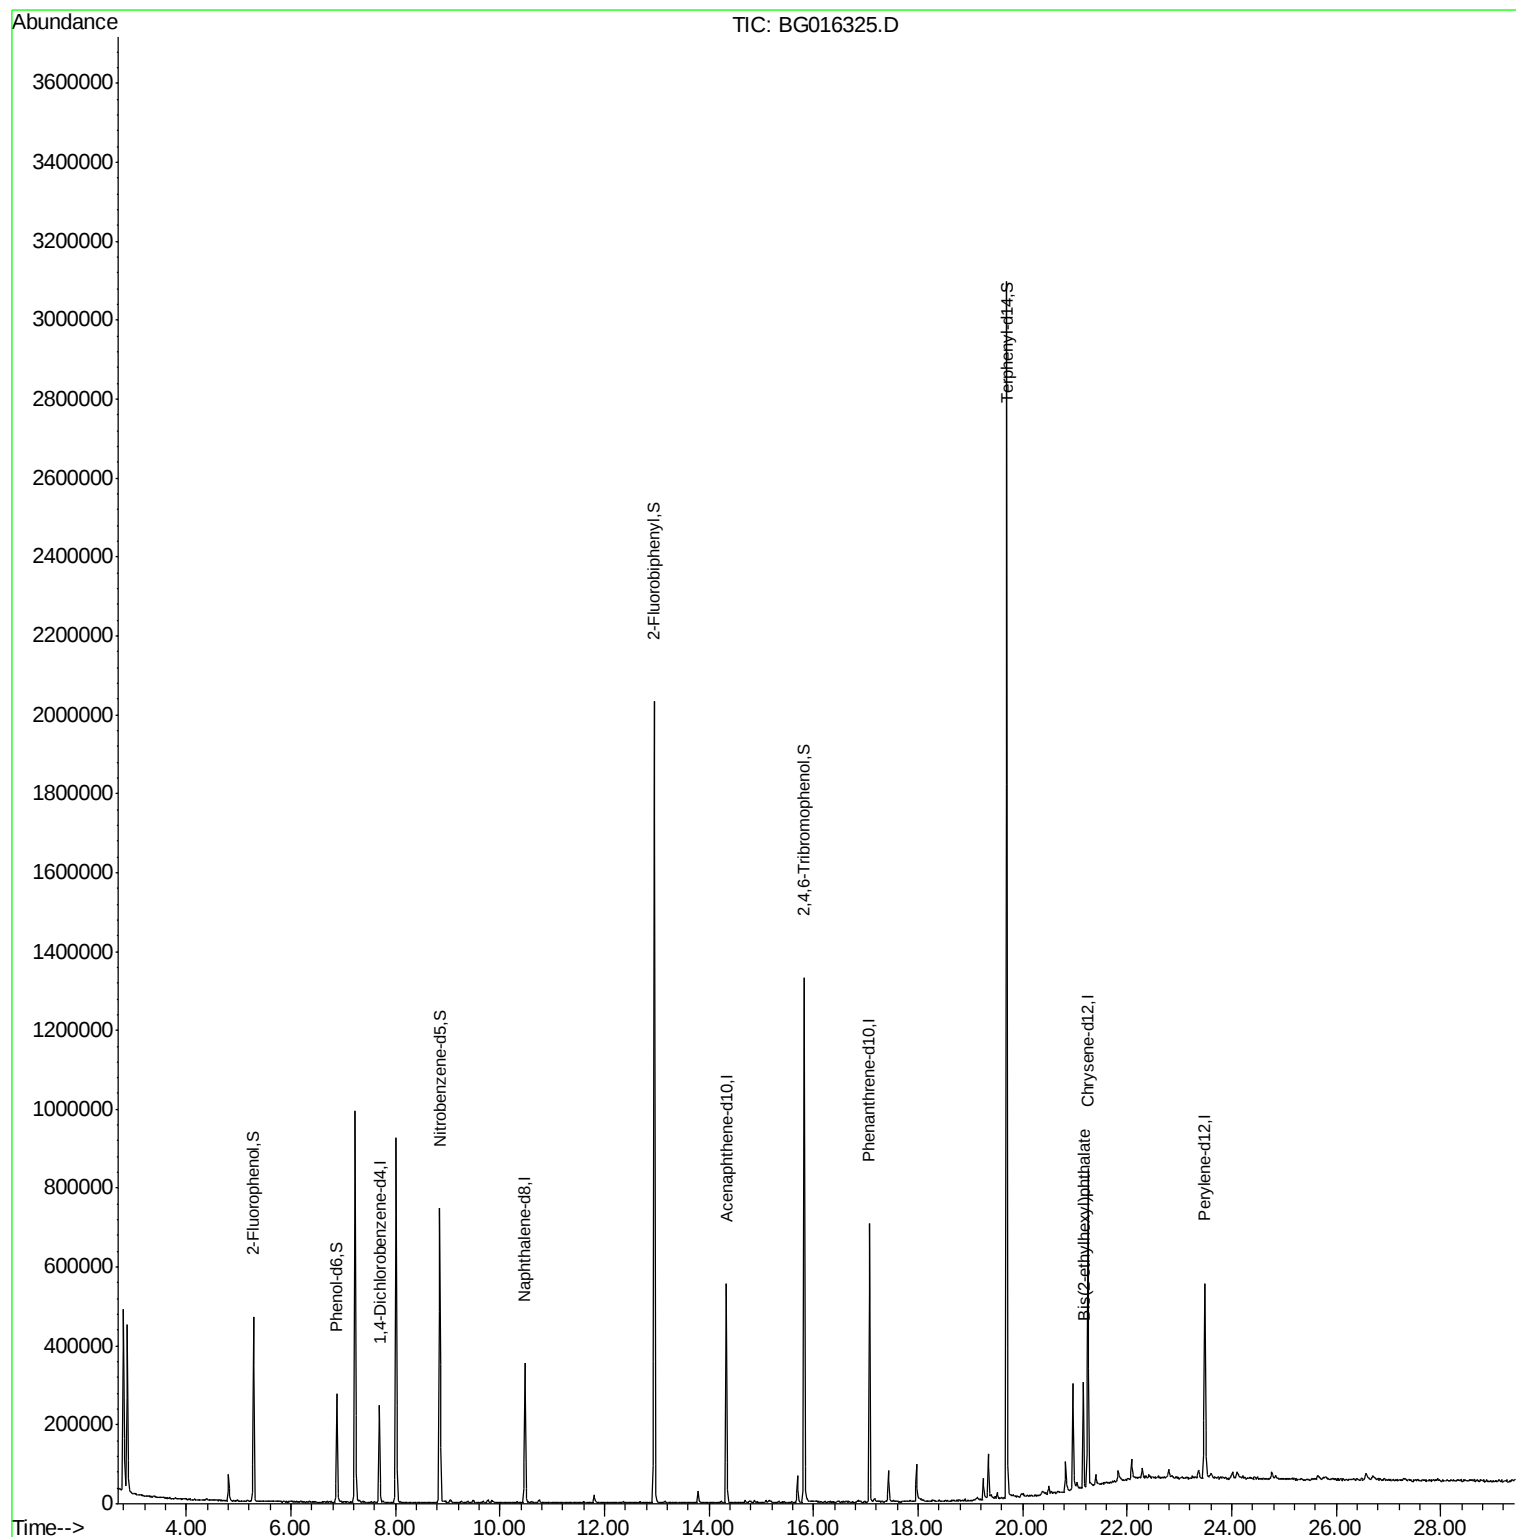




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.69 min Scan# 852
 Delta R.T. -0.00 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Instrument :
 BNA_G
 ClientSampleId :
 GMW-02

Tgt Ion:152 Resp: 66941
 Ion Ratio Lower Upper
 152 100
 150 160.9 130.1 195.1
 115 59.1 50.5 75.7

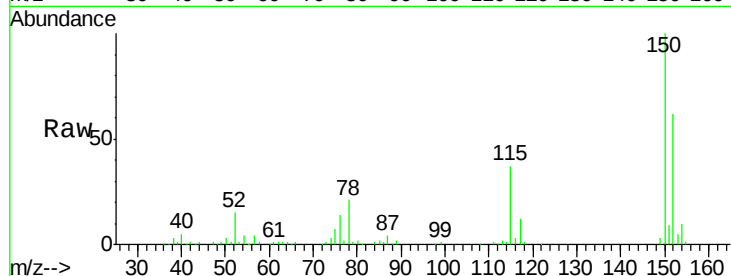


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

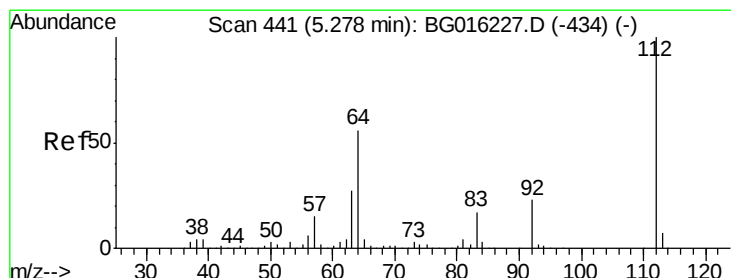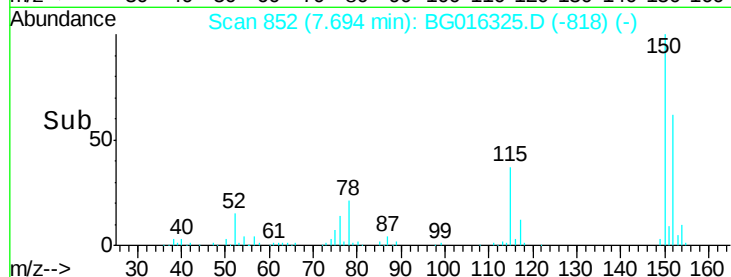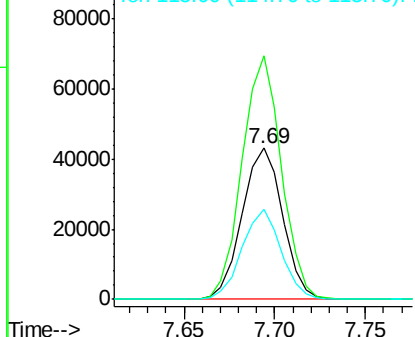



#5


2-Fluorophenol
 Concen: 51.94 ng
 RT: 5.28 min Scan# 442
 Delta R.T. 0.01 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Tgt Ion:112 Resp: 220293
 Ion Ratio Lower Upper
 112 100
 64 51.1 44.5 66.7
 63 24.5 21.4 32.0

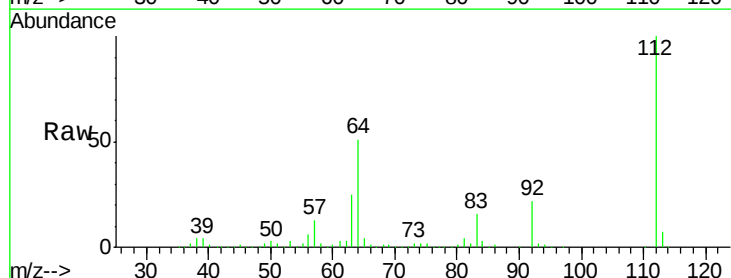

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

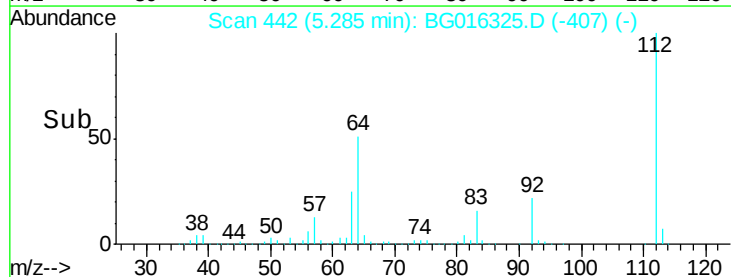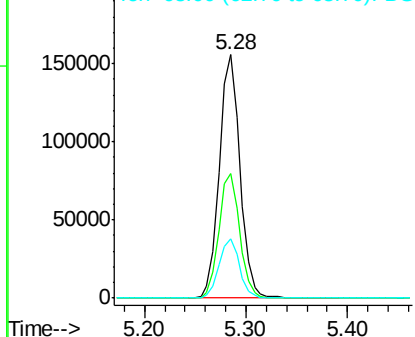

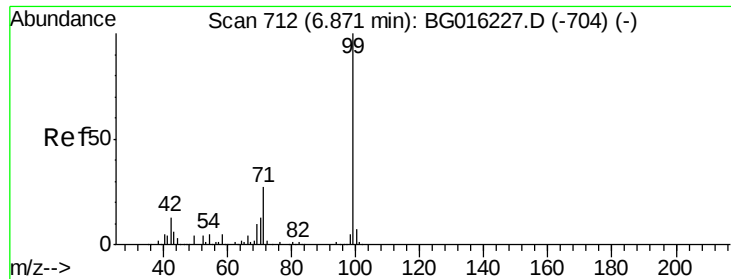

#7

Phenol-d6

Concen: 28.13 ng

RT: 6.88 min Scan# 713

Delta R.T. -0.00 min

Lab File: BG016325.D

Acq: 10 Apr 2015 18:55

Instrument :

BNA_G

ClientSampleId :

GMW-02


Tgt Ion: 99 Resp: 179120

Ion Ratio Lower Upper



99 100

42 11.6 10.0 15.0

71 25.0 21.5 32.3

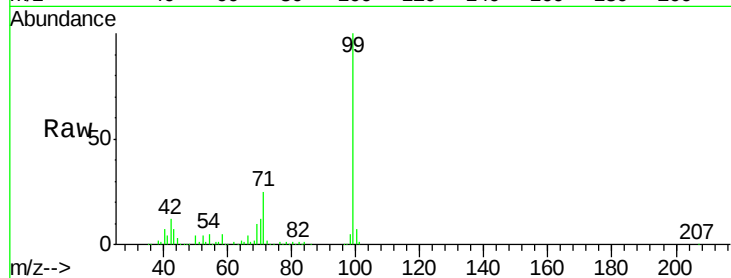

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

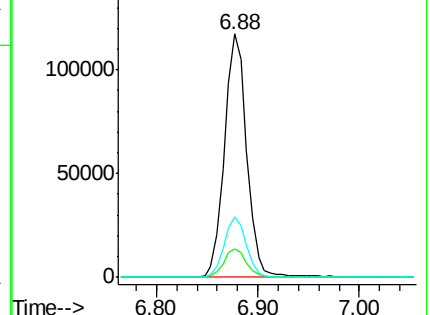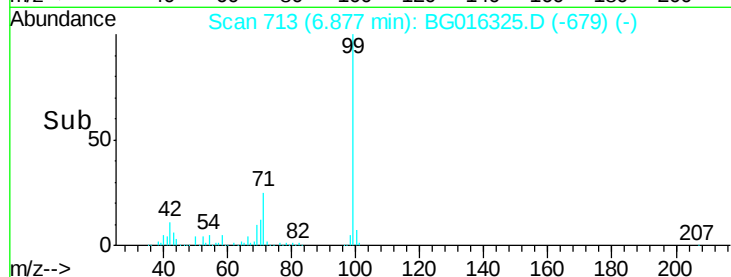

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.48 min Scan# 1326

Delta R.T. -0.00 min

Lab File: BG016325.D

Acq: 10 Apr 2015 18:55

Tgt Ion: 136 Resp: 299271


Ion Ratio Lower Upper

136 100



137 11.3 8.7 13.1

54 7.3 6.3 9.5

68 7.4 6.5 9.7

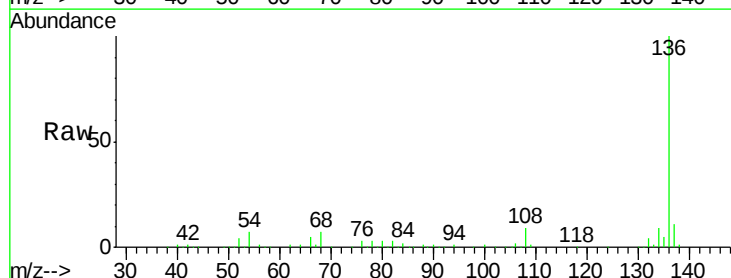

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

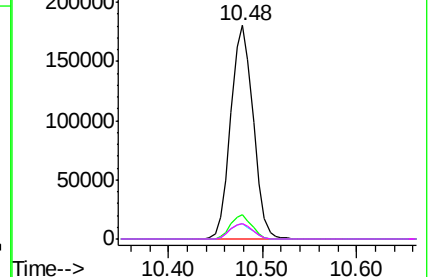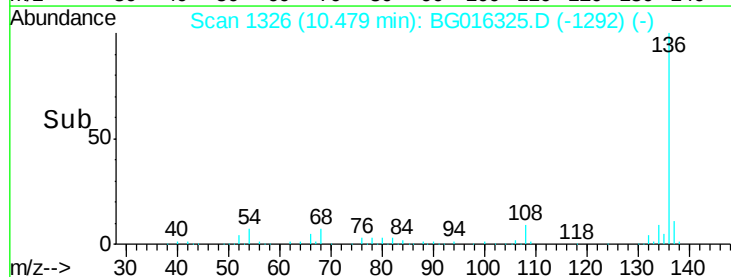






#23
 Nitrobenzene-d5
 Concen: 86.96 ng
 RT: 8.85 min Scan# 1049
 Delta R.T. -0.00 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Instrument :
 BNA_G
 ClientSampleId :
 GMW-02

Tgt Ion: 82 Resp: 449268
 Ion Ratio Lower Upper
 82 100
 128 50.9 37.8 56.8
 54 39.1 32.6 49.0

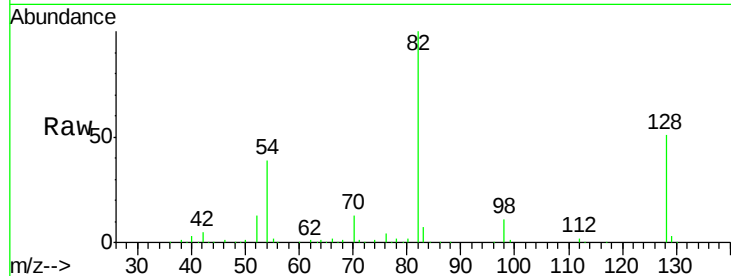


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

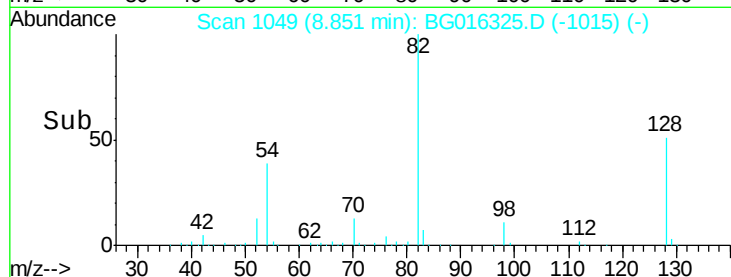
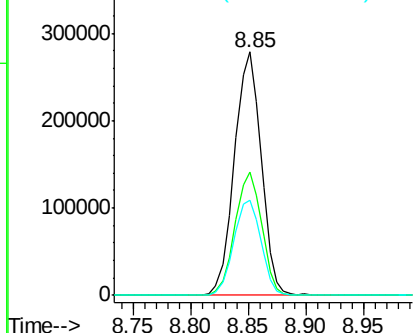



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.33 min Scan# 1982
 Delta R.T. -0.00 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Tgt Ion: 164 Resp: 180680
 Ion Ratio Lower Upper
 164 100
 162 97.7 77.3 115.9
 160 44.4 36.7 55.1

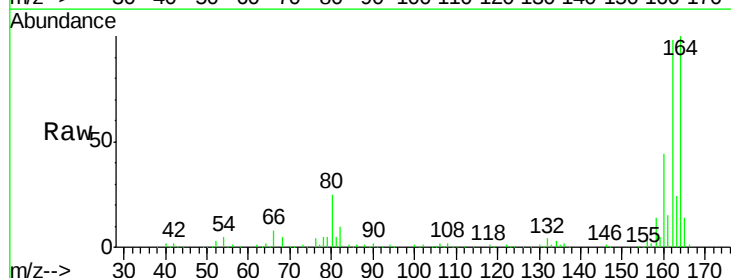

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

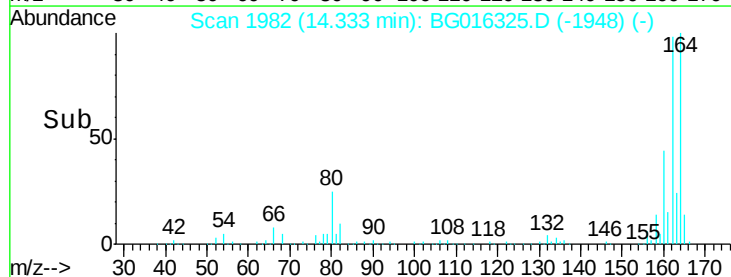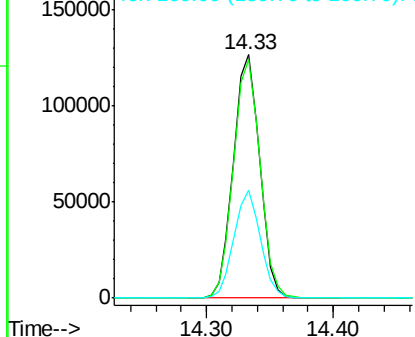


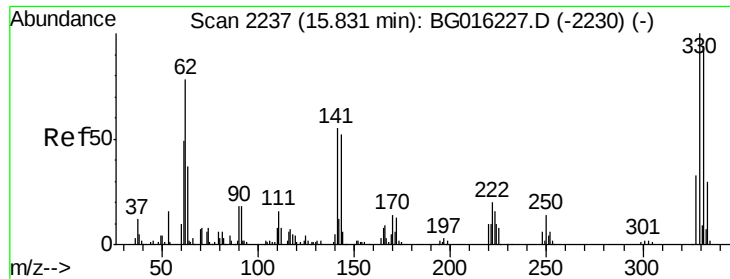




#41
 2,4,6-Tribromophenol
 Concen: 149.68 ng
 RT: 15.83 min Scan# 2236
 Delta R.T. -0.00 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Instrument :
 BNA_G
 ClientSampleId :
 GMW-02

Tgt Ion:330 Resp: 182900
 Ion Ratio Lower Upper
 330 100
 332 96.3 75.8 113.6
 141 55.5 46.6 69.8

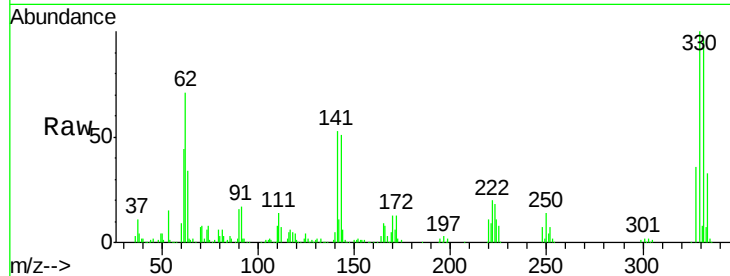


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

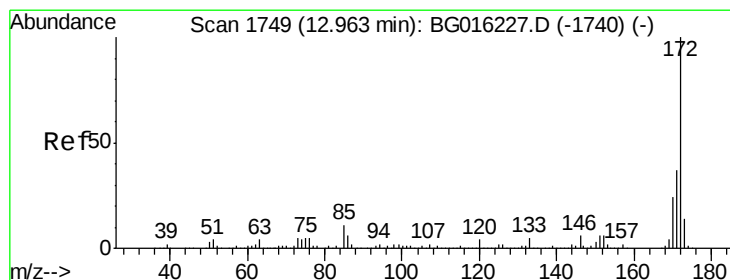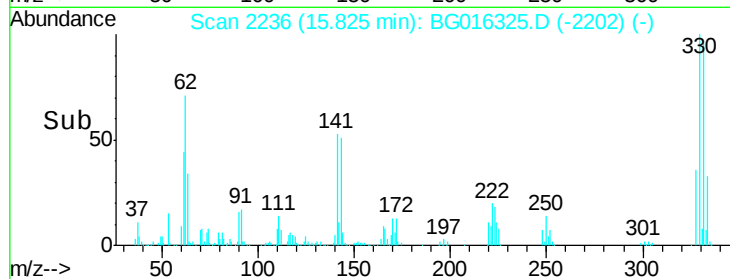
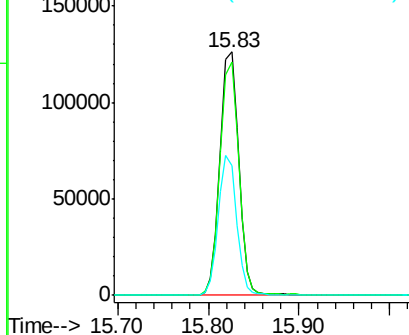



#44
 2-Fluorobiphenyl
 Concen: 91.21 ng
 RT: 12.95 min Scan# 1747
 Delta R.T. -0.00 min
 Lab File: BG016325.D
 Acq: 10 Apr 2015 18:55

Tgt Ion:172 Resp: 967898
 Ion Ratio Lower Upper
 172 100
 171 38.0 29.6 44.4
 170 24.3 19.4 29.2

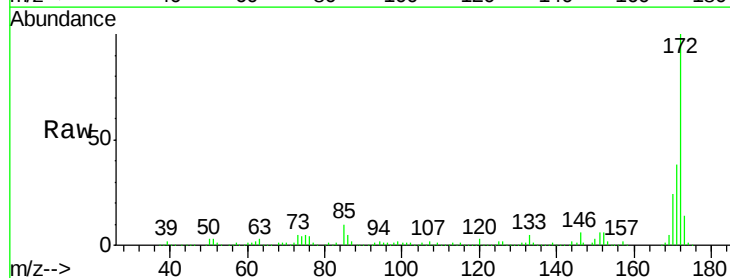

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

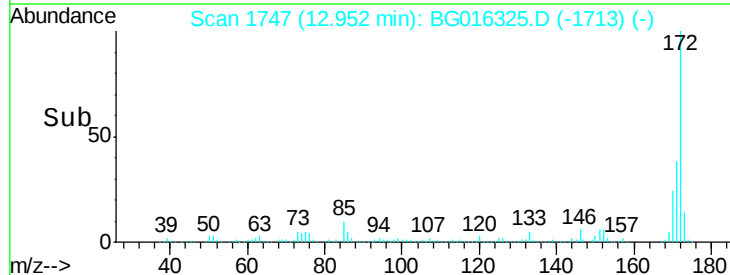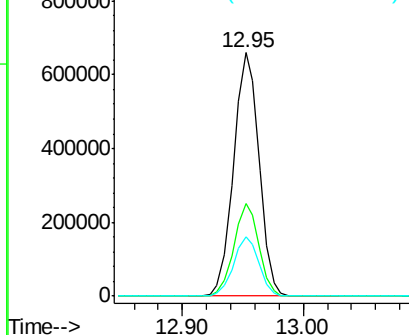


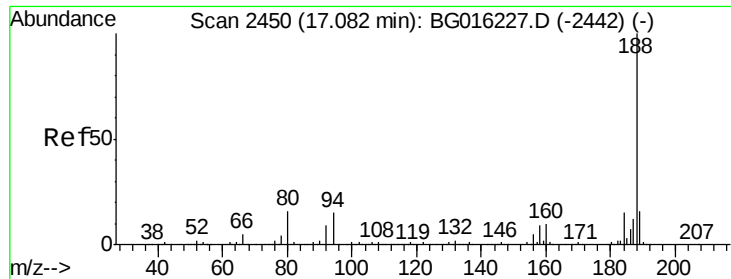




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.07 min Scan# 2448
Delta R.T. -0.00 min
Lab File: BG016325.D
Acq: 10 Apr 2015 18:55

Instrument :
BNA_G
ClientSampleId :
GMW-02

Tgt Ion:188 Resp: 375546
Ion Ratio Lower Upper
188 100
94 13.6 12.2 18.4
80 14.2 12.8 19.2

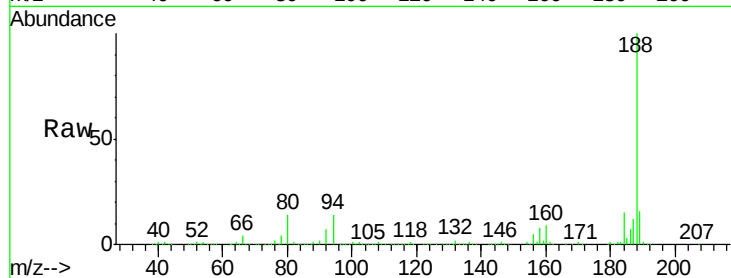


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGO
Ion 80.00 (79.70 to 80.70): BGO

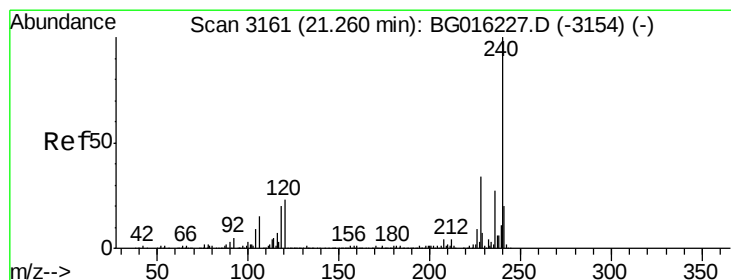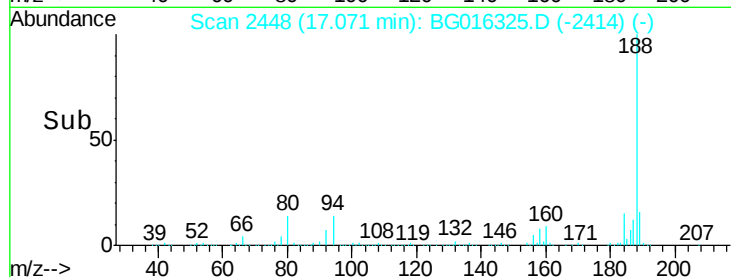
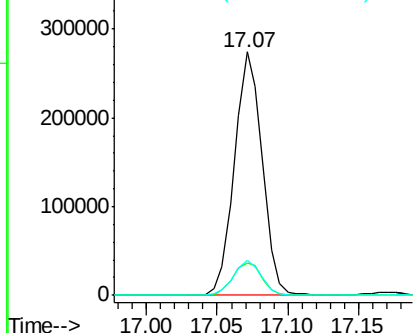



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.25 min Scan# 3159
Delta R.T. -0.01 min
Lab File: BG016325.D
Acq: 10 Apr 2015 18:55

Tgt Ion:240 Resp: 325529
Ion Ratio Lower Upper
240 100
120 20.9 18.6 28.0
236 26.2 21.7 32.5

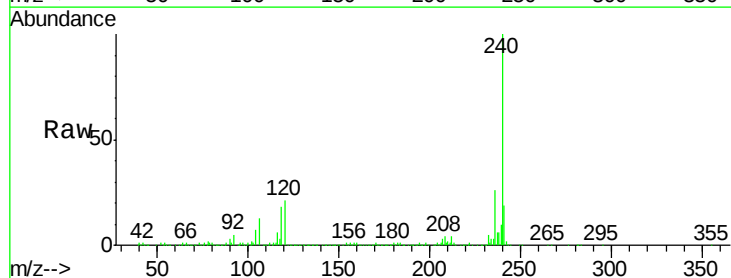

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

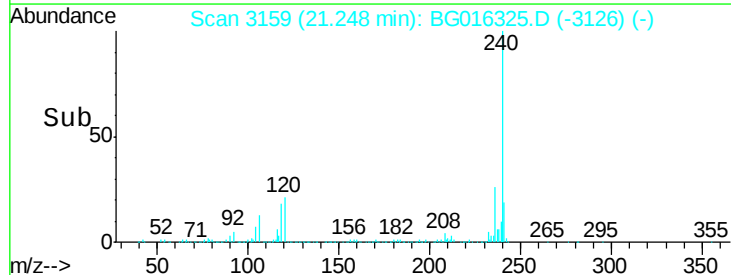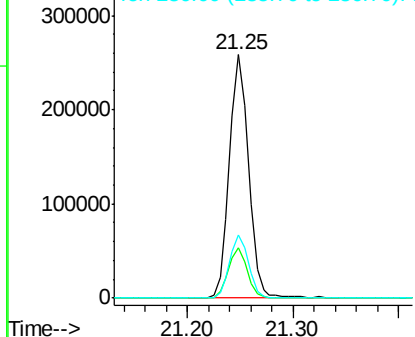

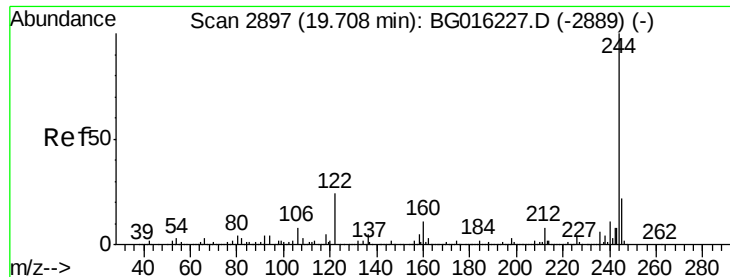

#78

Terphenyl-d14

Concen: 79.01 ng

RT: 19.70 min Scan# 2895

Delta R.T. -0.01 min

Lab File: BG016325.D

Acq: 10 Apr 2015 18:55

Instrument :

BNA_G

ClientSampleId :

GMW-02


Tgt Ion:244 Resp: 1098909

Ion Ratio Lower Upper

244 100

212 8.3 6.6 9.8




122 24.2 19.1 28.7

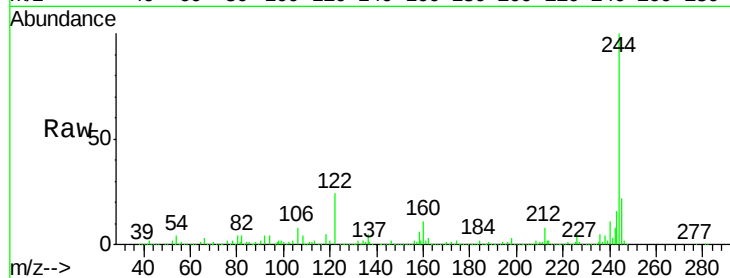

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

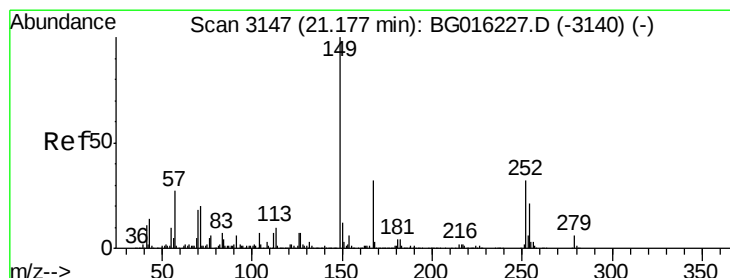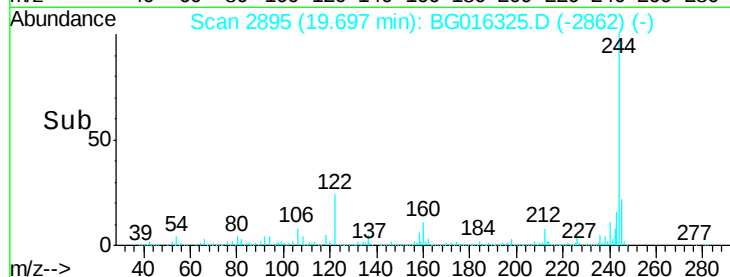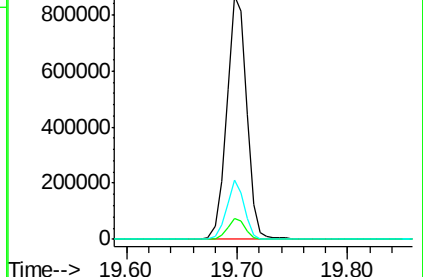

#83

Bis(2-ethylhexyl)phthalate

Concen: 5.94 ng

RT: 21.17 min Scan# 3145

Delta R.T. -0.00 min

Lab File: BG016325.D

Acq: 10 Apr 2015 18:55


Tgt Ion:149 Resp: 89479

Ion Ratio Lower Upper

149 100

167 31.1 25.8 38.6



279 6.3 4.7 7.1

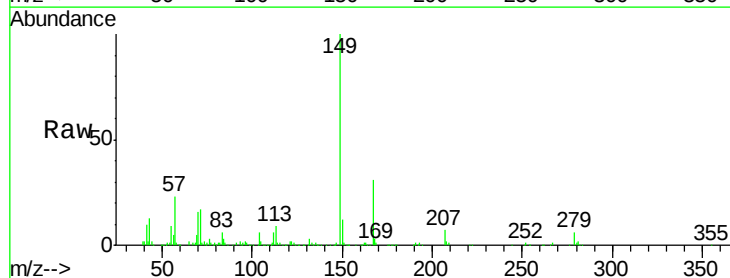


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

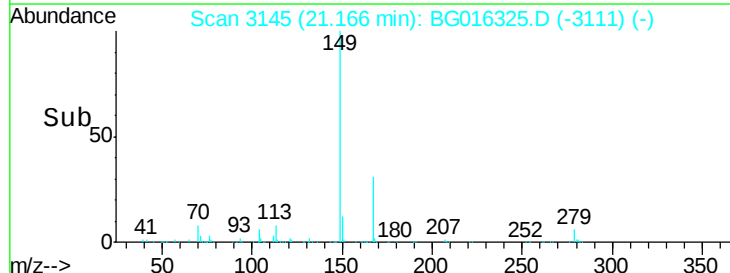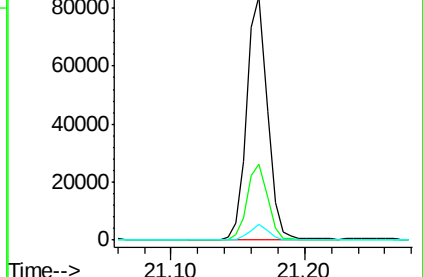


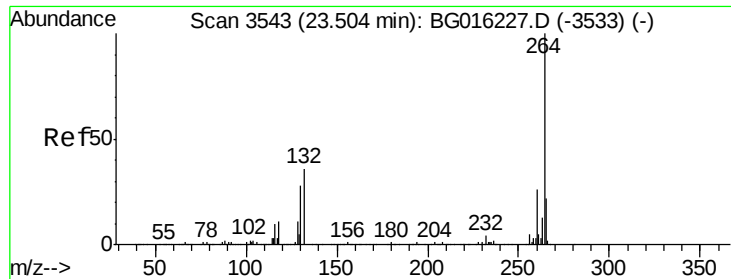

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.49 min Scan# 3541
Delta R.T. -0.00 min
Lab File: BG016325.D
Acq: 10 Apr 2015 18:55

Instrument :
BNA_G
ClientSampleId :
GMW-02

Tgt Ion: 264 Resp: 296143
Ion Ratio Lower Upper
264 100
260 24.5 20.4 30.6
265 21.7 17.2 25.8

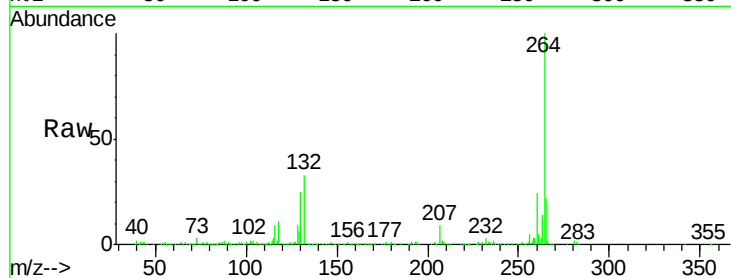

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

