
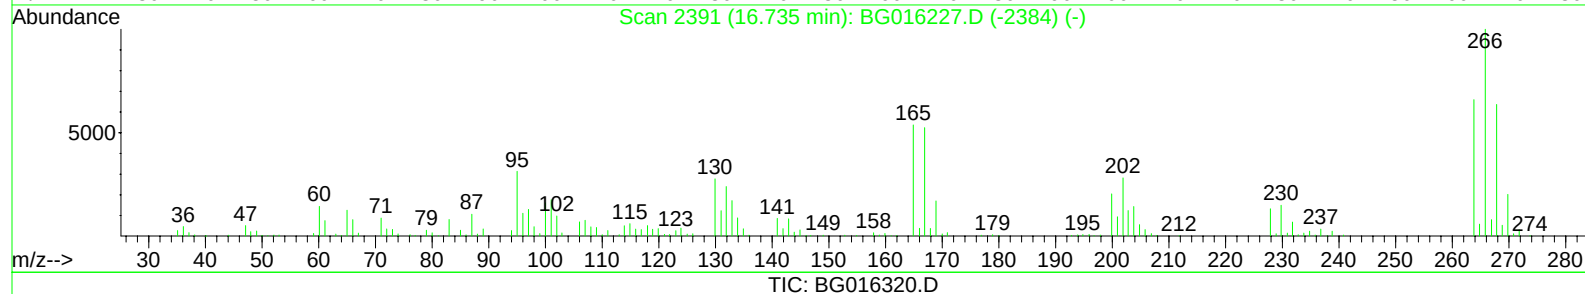
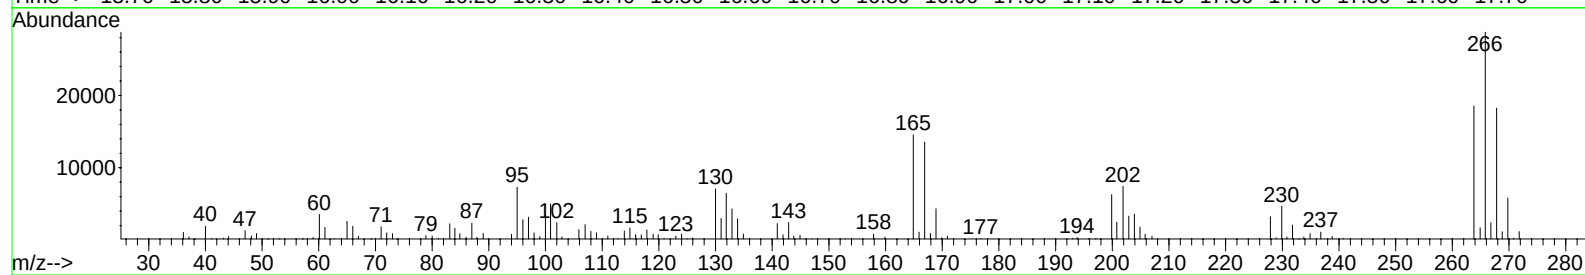


Data Path : Z:\HPCHEM1\BNA G\Data\BG041015\
Data File : BG016320.D
Acq On : 10 Apr 2015 15:47
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:20:11 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

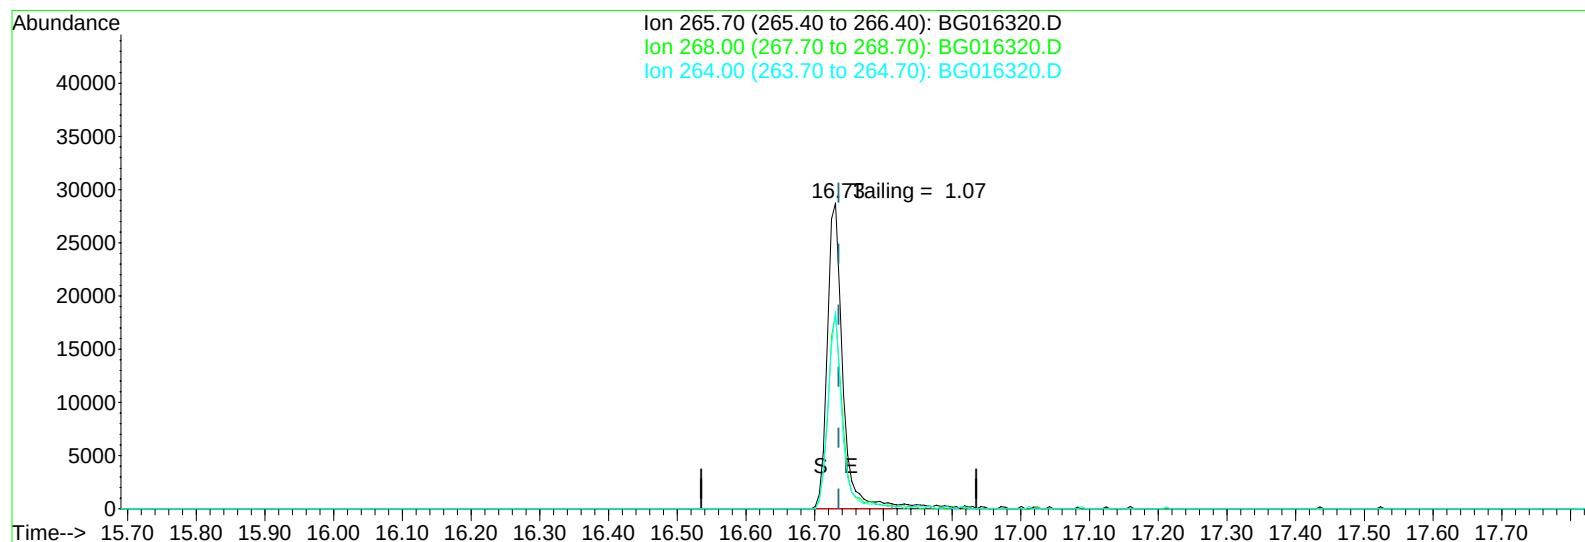

(69) Pentachlorophenol (C)




16.730min (-0.005) 14483.07ng

response 44767

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.51
264.00	66.00	64.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG041015\
Data File : BG016320.D
Acq On : 10 Apr 2015 15:47
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:20:11 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

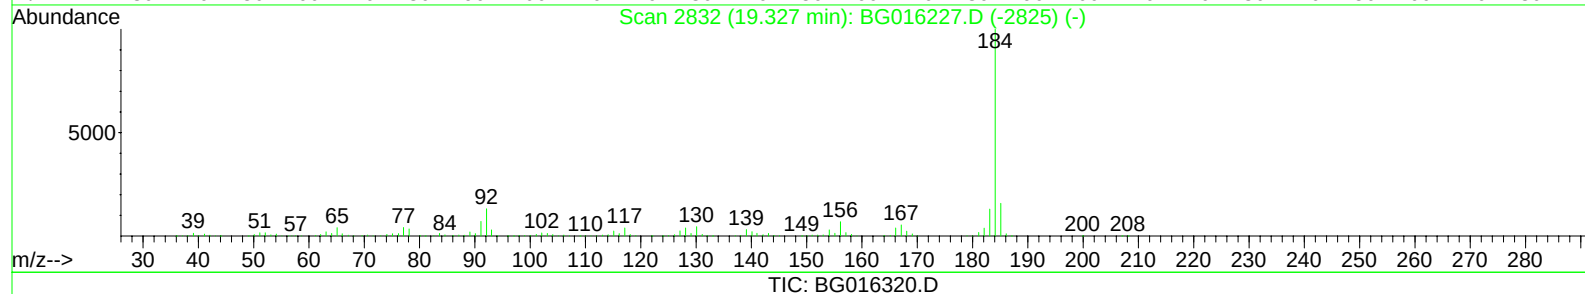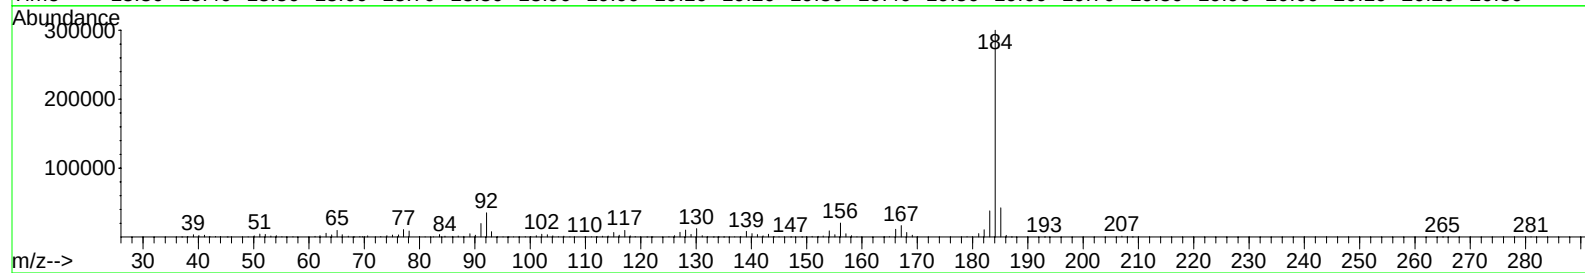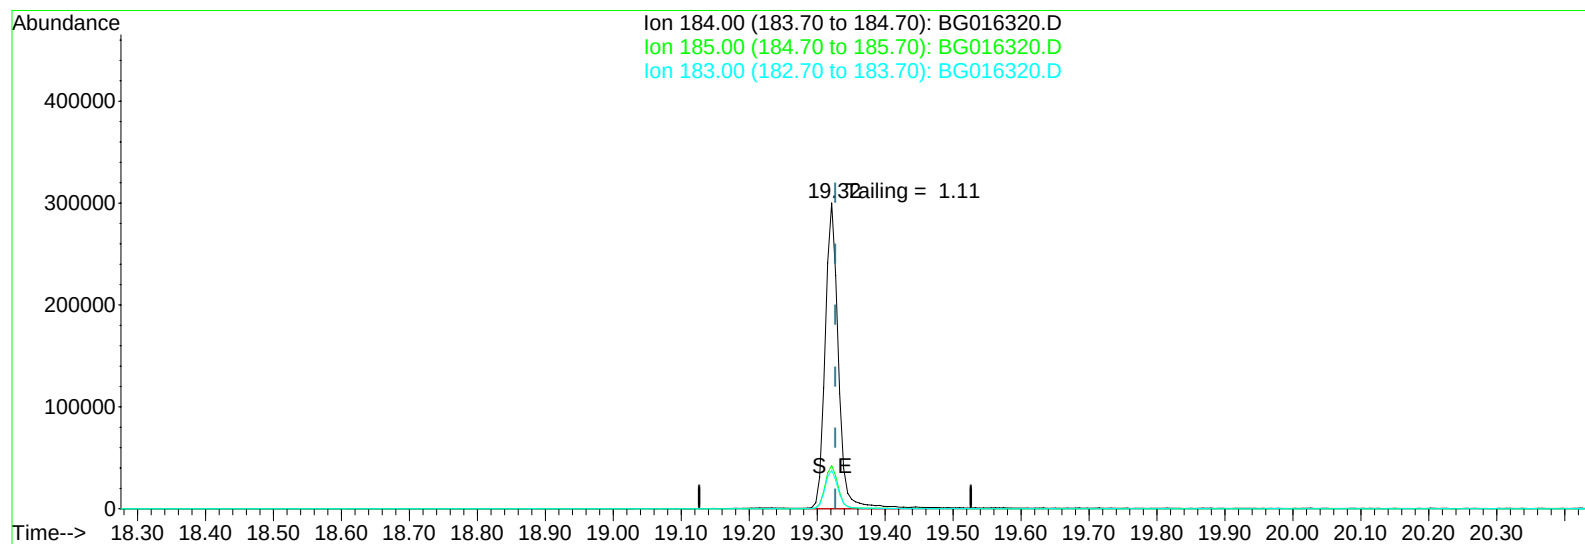

(76) Benzidine

19.321min (-0.005) 8832.32ng

response 401149

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.15
183.00	13.00	12.63
0.00	0.00	0.00