
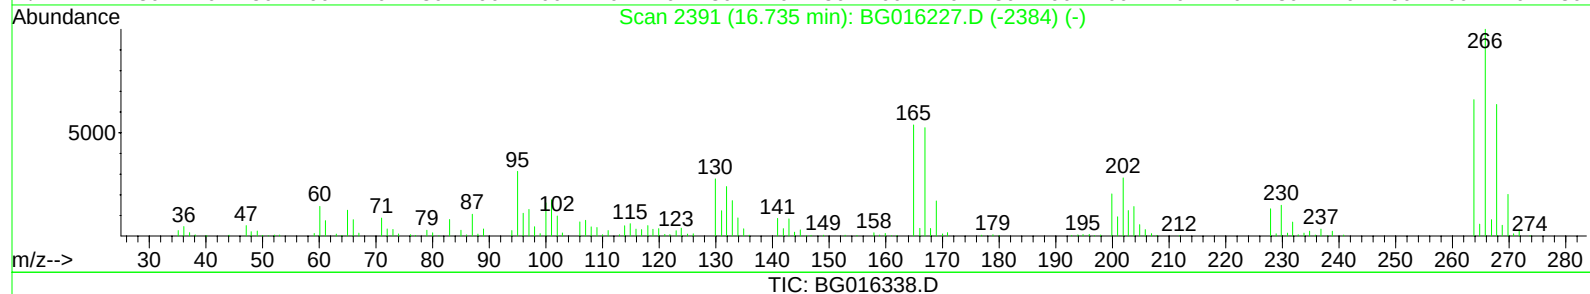
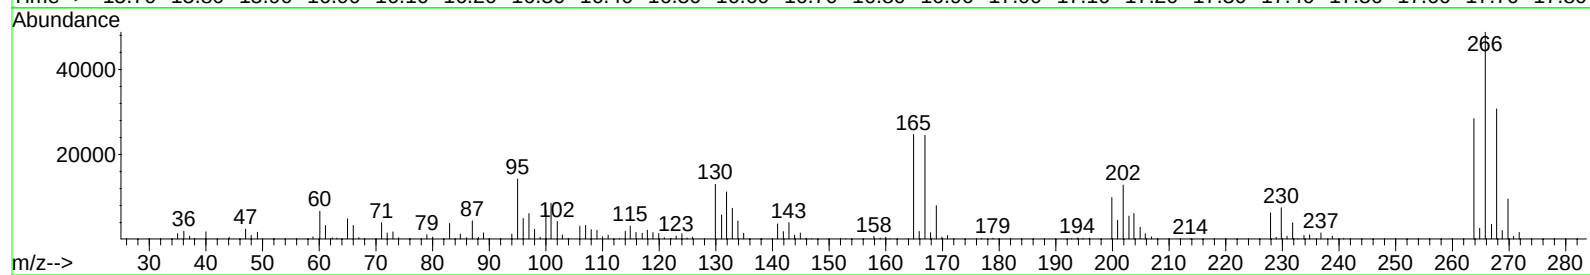


Data Path : Z:\HPCHEM1\BNA G\Data\BG041015\
Data File : BG016338.D
Acq On : 11 Apr 2015 4:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:21:08 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

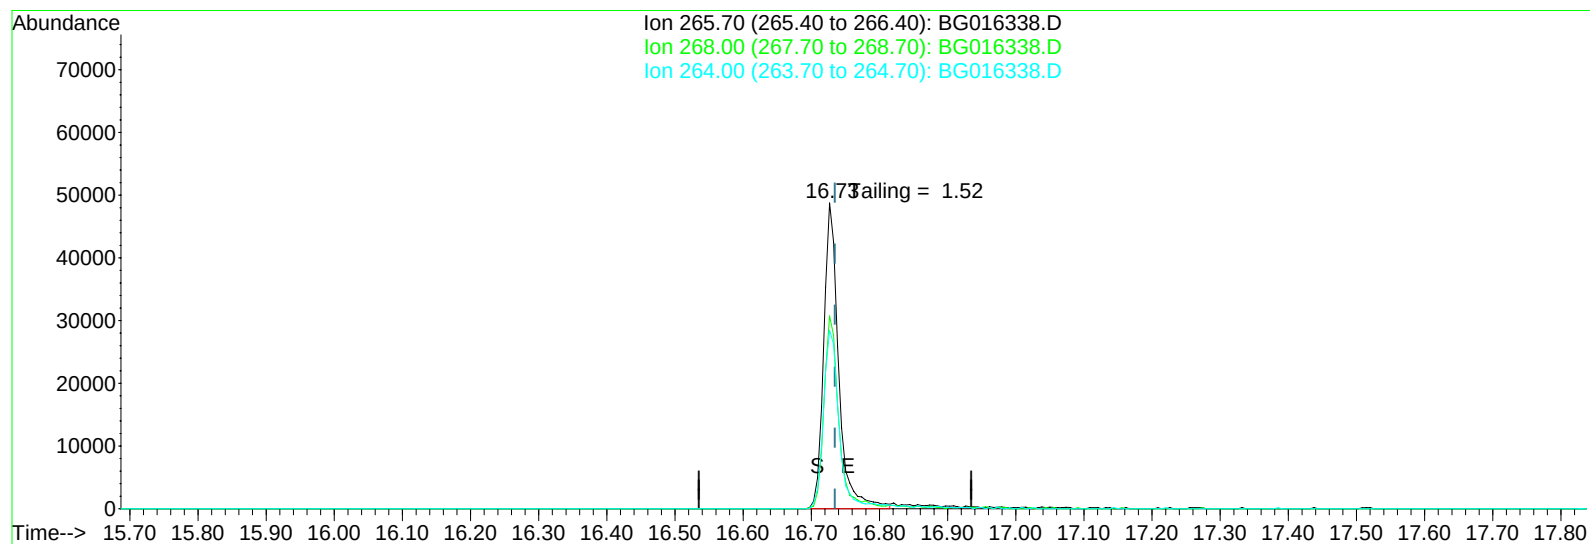

(69) Pentachlorophenol (C)




16.727min (-0.008) 0.00ng

response 75496

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.08
264.00	66.00	58.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG041015\
Data File : BG016338.D
Acq On : 11 Apr 2015 4:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:21:08 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:17:17 2015
Response via : Initial Calibration

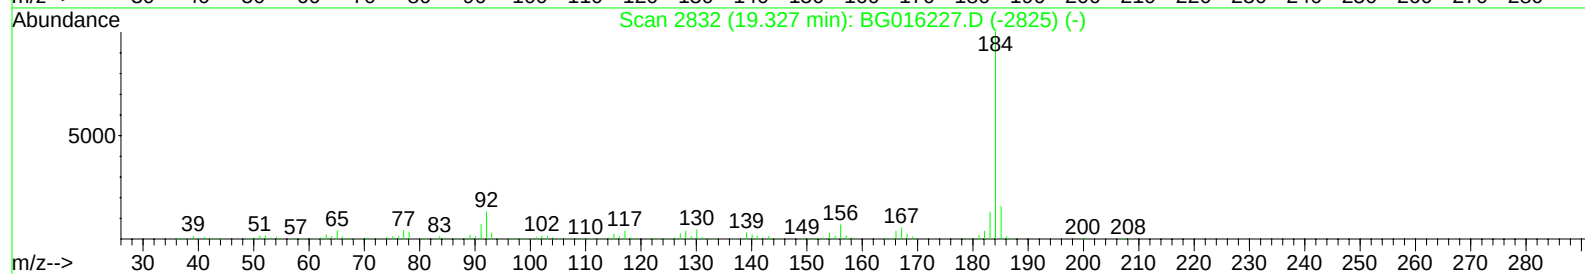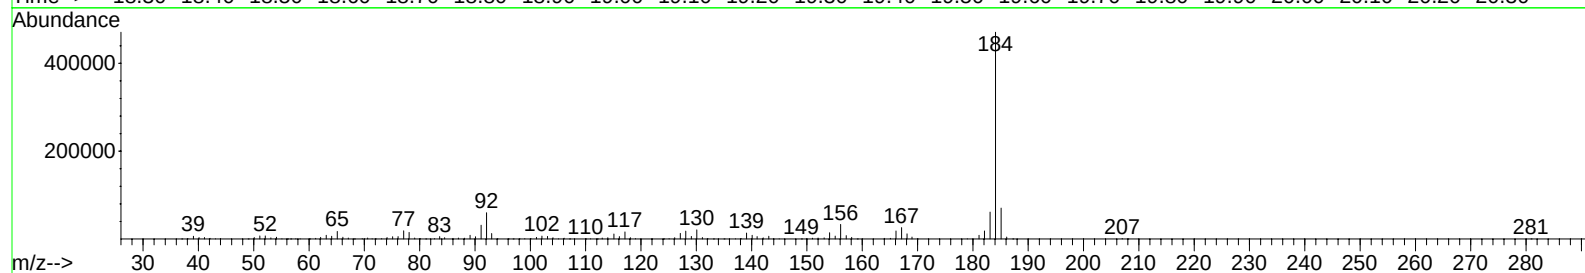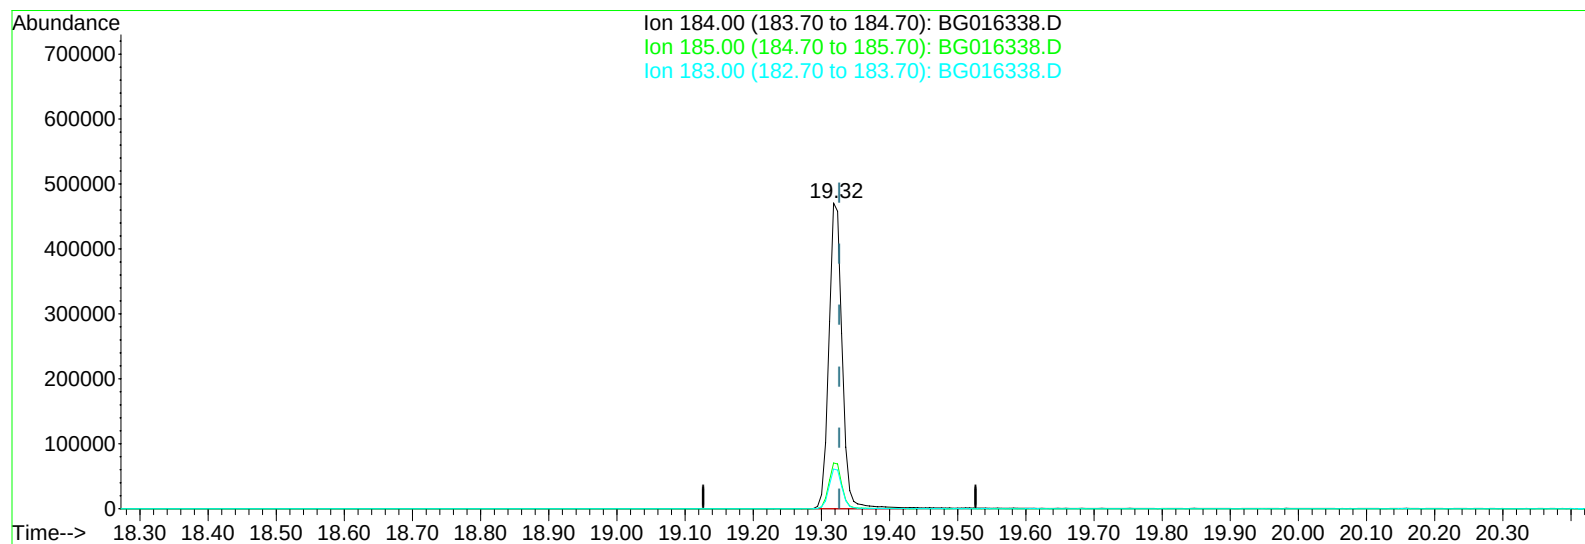

TIC: BG016338.D

(76) Benzidine

19.318min (-0.009) 40656.46ng

response 632757

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.95
183.00	13.00	13.01
0.00	0.00	0.00