


Data Path : Z:\HPCHEM1\BNA_G\Data\BG041015\
 Data File : BG016338.D
 Acq On : 11 Apr 2015 4:46
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 04:17:17 2015

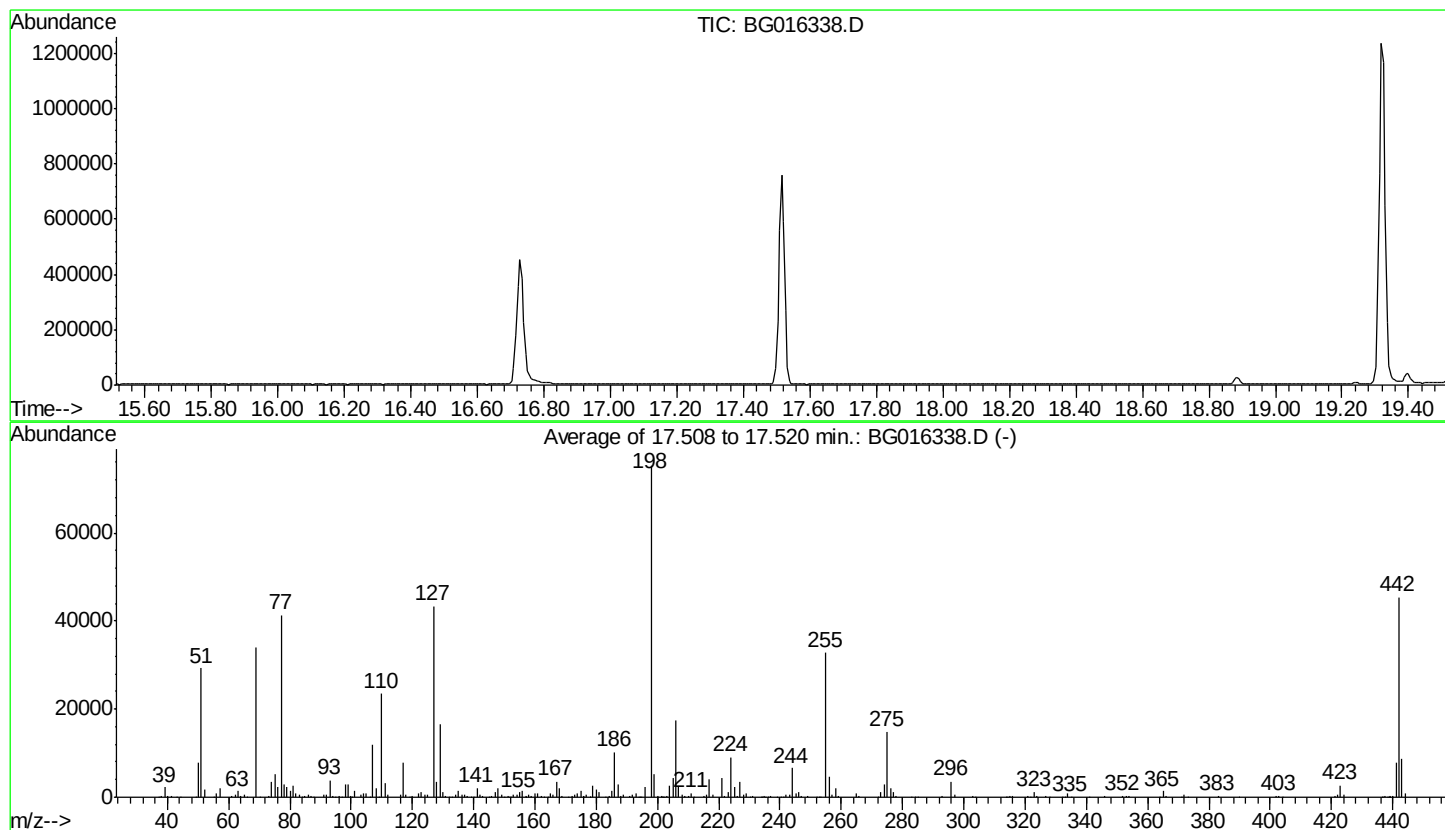

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	29330	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.3	34061	PASS
70	69	0.00	2	0.4	146	PASS
127	198	10	80	57.7	43410	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75258	PASS
199	198	5	9	7.1	5332	PASS
275	198	10	60	19.8	14915	PASS
365	198	1	100	1.8	1373	PASS
441	442	0.01	24	17.4	7926	PASS
442	198	50	100	60.4	45450	PASS
443	442	15	24	19.3	8763	PASS