
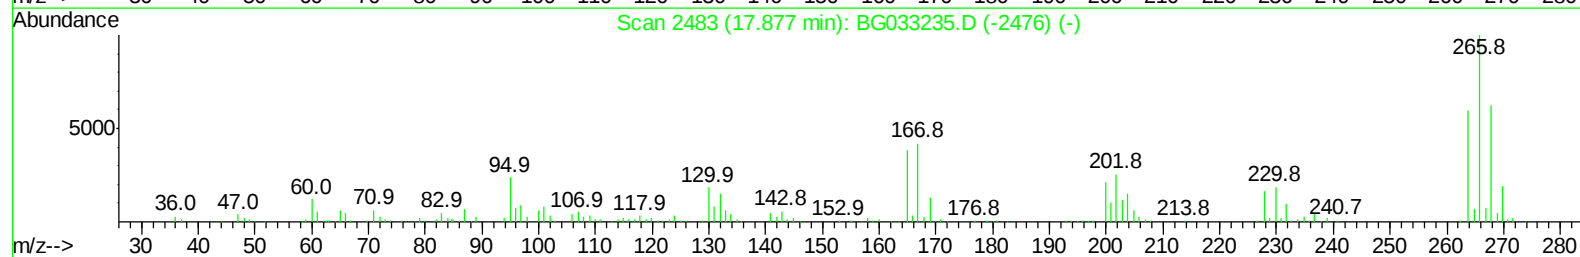
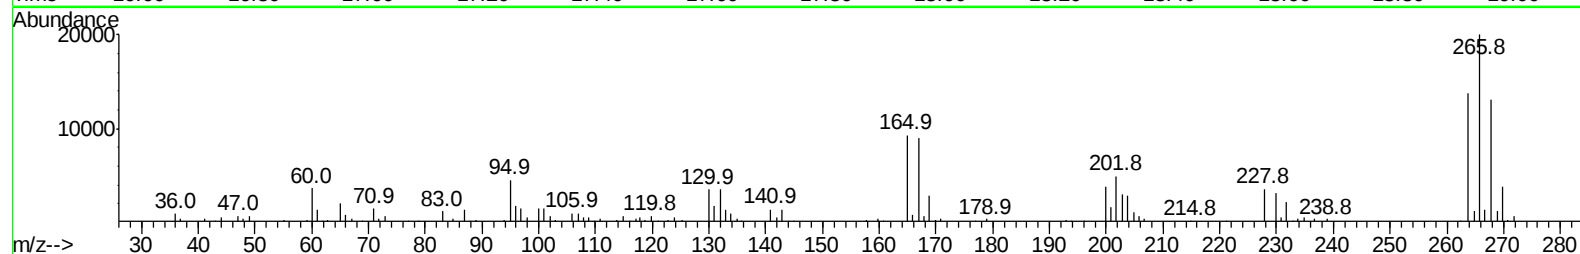


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041018\
Data File : BG033709.D
Acq On : 10 Apr 2018 12:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:11:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

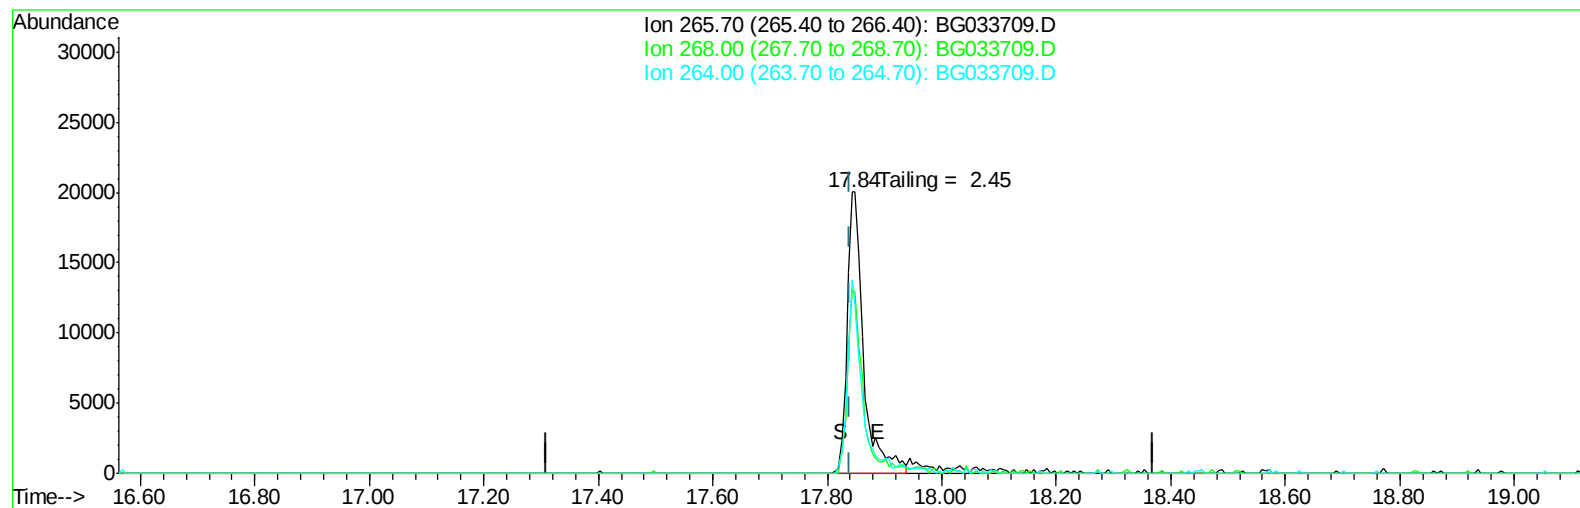

TIC: BG033709.D

(69) Pentachlorophenol (C)




17.843min (+0.002) 48169.72ng

response 39748

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.35
264.00	62.00	68.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041018\
 Data File : BG033709.D
 Acq On : 10 Apr 2018 12:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:11:05 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 16:51:36 2018
 Response via : Initial Calibration

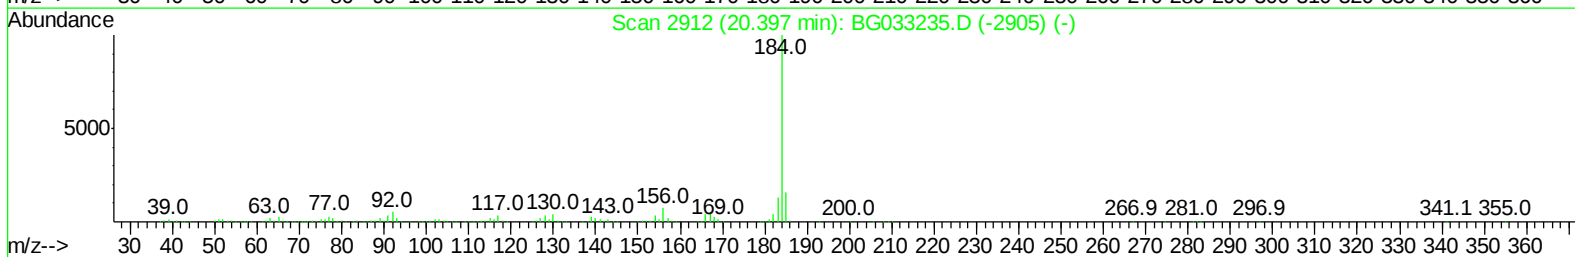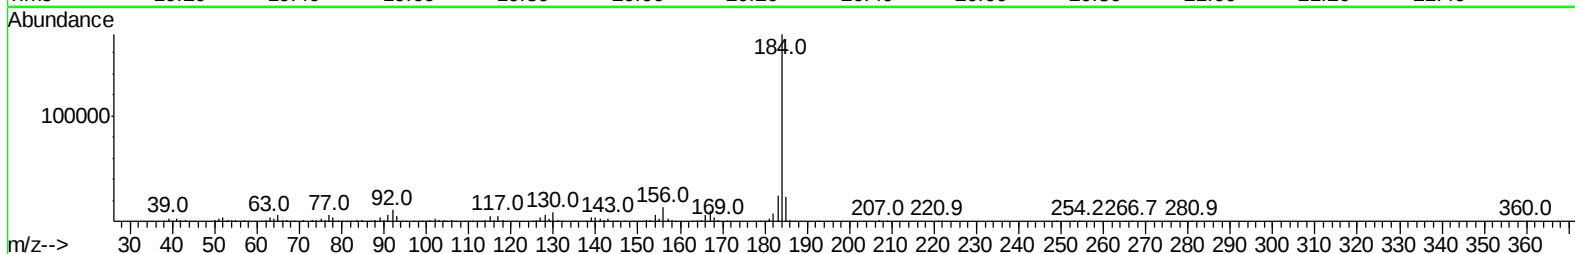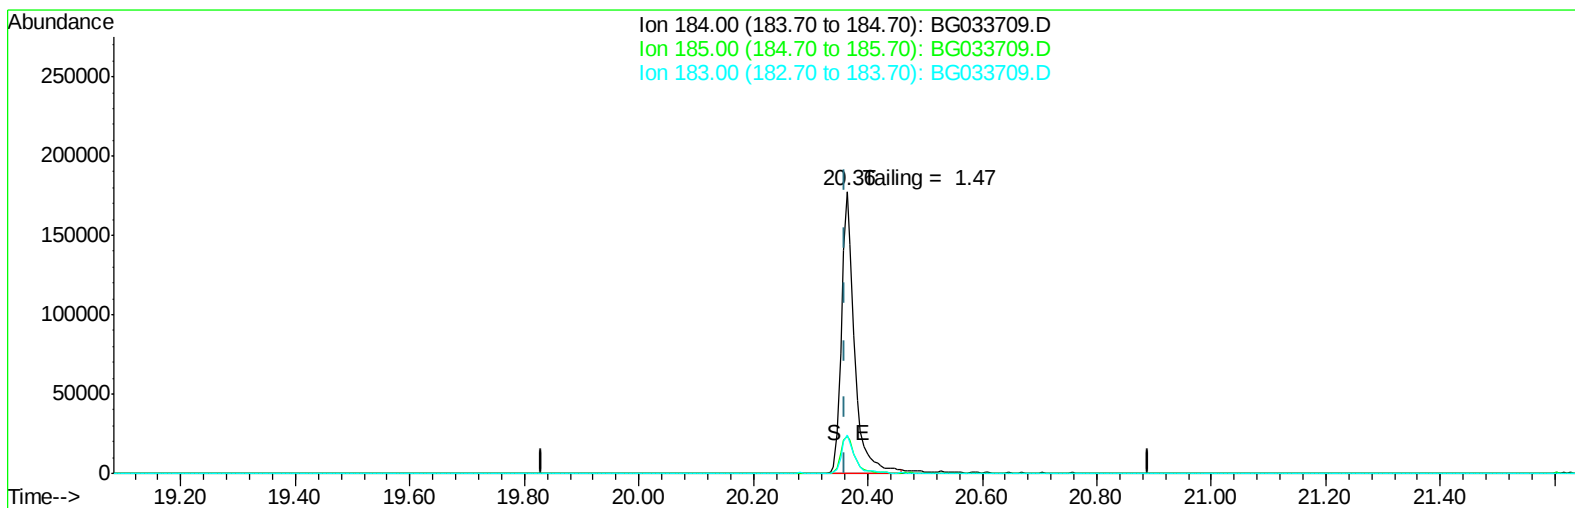

TIC: BG033709.D

(76) Benzidine

20.364min (+0.002) 0.00ng

response 288393

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.26
183.00	13.30	13.62
0.00	0.00	0.00