


Data Path : Z:\HPCHEM1\BNA G\Data\BG041018\
 Data File : BG033709.D
 Acq On : 10 Apr 2018 12:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 10 16:51:36 2018

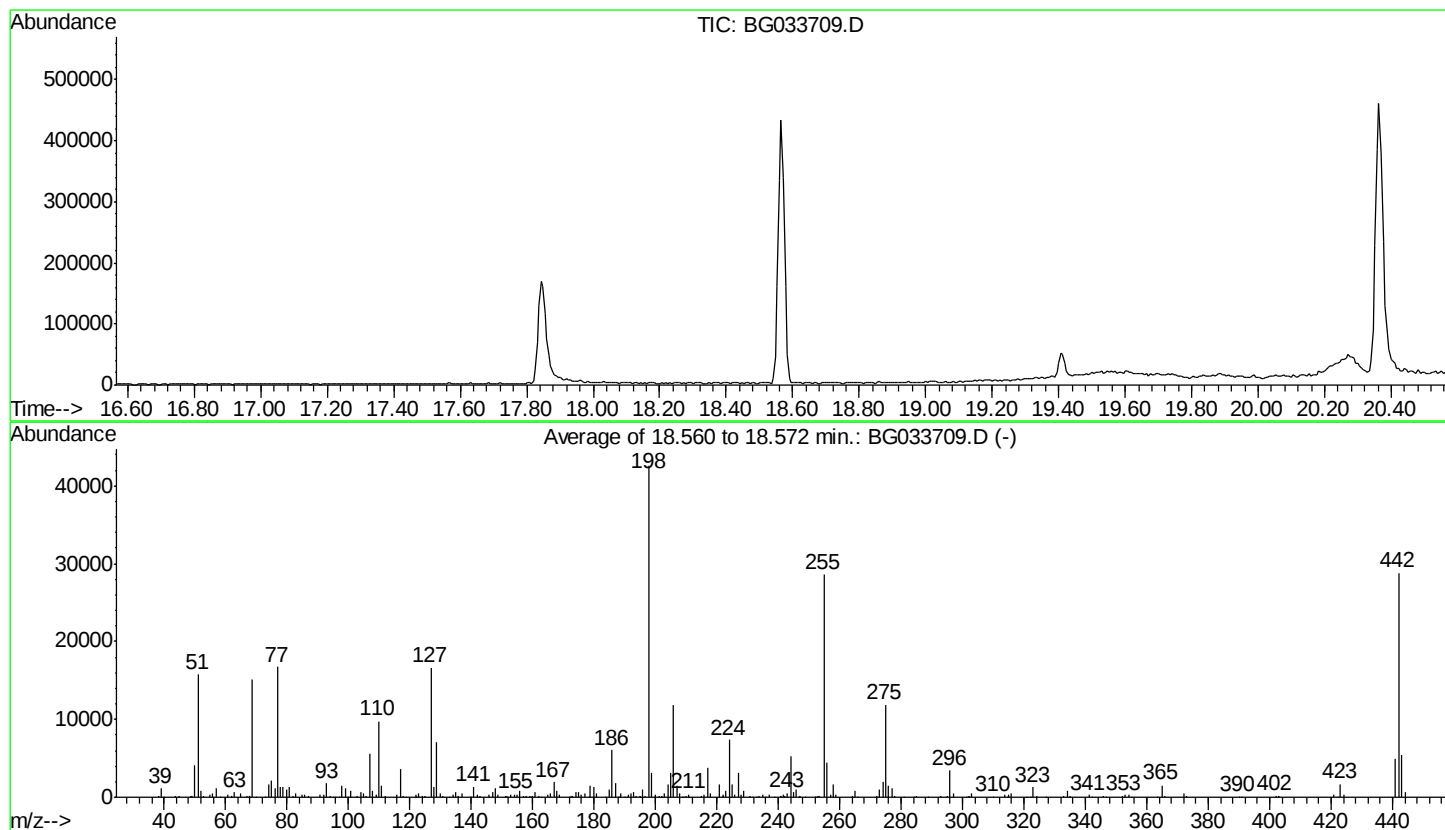

AutoFind: Scans 2599, 2600, 2601; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	15739	PASS
68	69	0.00	2	1.1	163	PASS
69	198	0.00	100	35.7	15191	PASS
70	69	0.00	2	0.4	62	PASS
127	198	10	80	39.2	16690	PASS
197	198	0.00	2	0.5	230	PASS
198	198	100	100	100.0	42602	PASS
199	198	5	9	7.3	3092	PASS
275	198	10	60	27.9	11878	PASS
365	198	1	100	3.7	1555	PASS
441	443	0.01	100	90.6	4982	PASS
442	198	50	100	67.7	28858	PASS
443	442	15	24	19.0	5497	PASS