

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057041.D
 Acq On : 10 Apr 2023 12:00
 Operator : CG/JU
 Sample : 02224-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-01

Quant Time: Apr 11 04:11:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 08 04:45:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.408	152	14277	20.000	ng	0.00
21) Naphthalene-d8	11.251	136	58076	20.000	ng	# 0.00
39) Acenaphthene-d10	15.023	164	42136	20.000	ng	0.00
64) Phenanthrene-d10	17.760	188	98302	20.000	ng	# 0.00
76) Chrysene-d12	22.072	240	84330	20.000	ng	-0.01
86) Perylene-d12	25.614	264	93883	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.917	112	84657	94.900	ng	0.00
7) Phenol-d6	7.539	99	121810	91.299	ng	0.00
23) Nitrobenzene-d5	9.583	82	81192	57.204	ng	0.00
42) 2,4,6-Tribromophenol	16.503	330	60637	90.081	ng	0.00
45) 2-Fluorobiphenyl	13.648	172	190812	61.407	ng	0.00
79) Terphenyl-d14	20.327	244	341845	68.594	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057041.D
Acq On : 10 Apr 2023 12:00
Operator : CG/JU
Sample : 02224-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01

Quant Time: Apr 11 04:11:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration




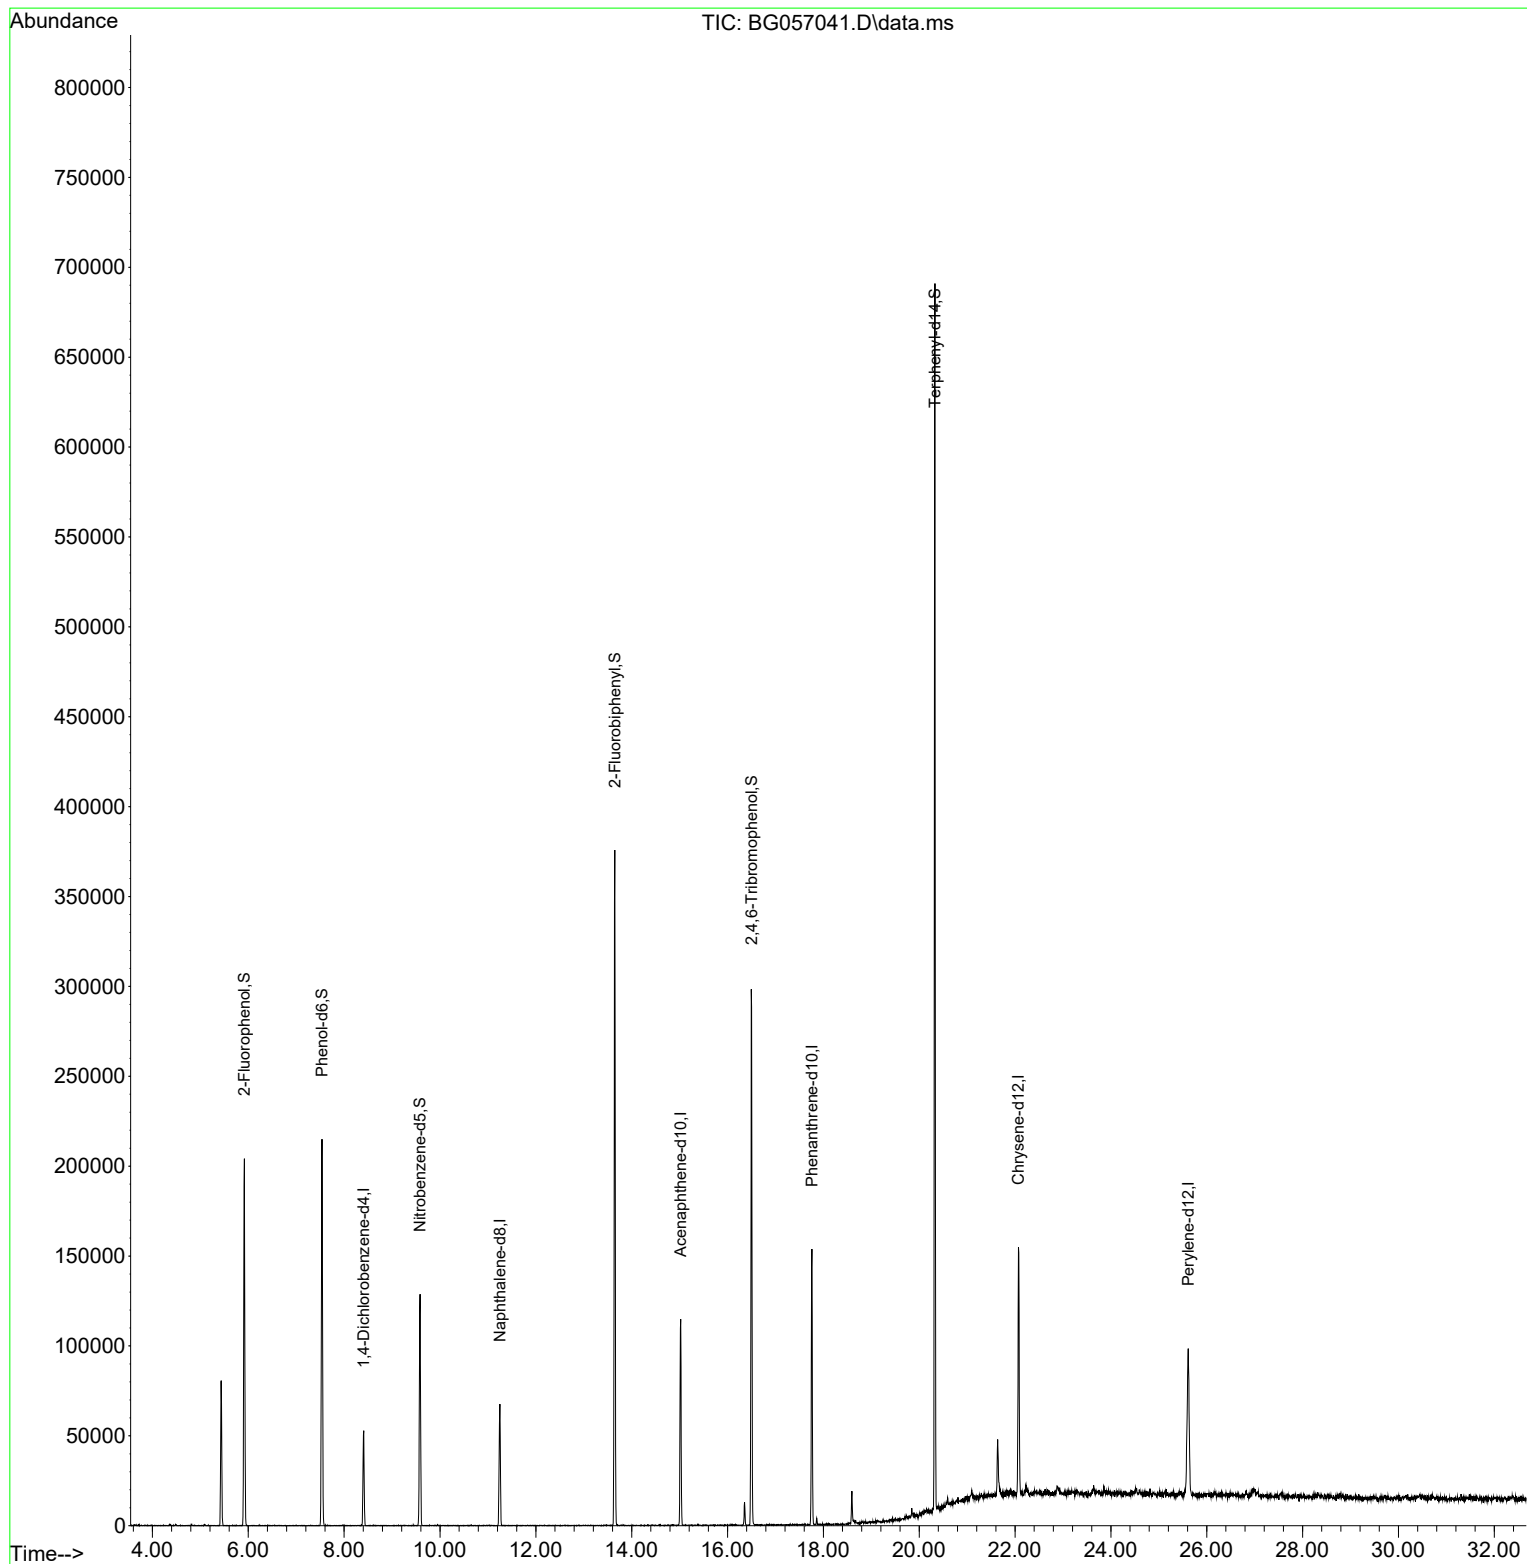




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.408 min Scan# 81
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00




Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01


Tgt Ion:152 Resp: 14277
Ion Ratio Lower Upper
152 100
150 164.2 124.1 186.1
115 62.5 49.1 73.7

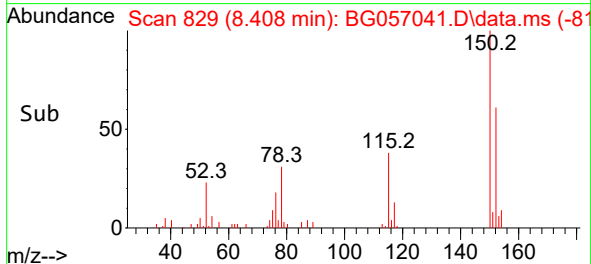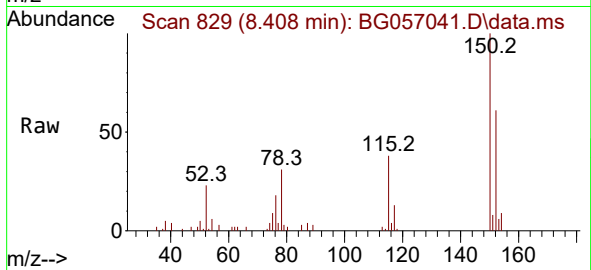

#5
2-Fluorophenol
Concen: 94.900 ng
RT: 5.917 min Scan# 405
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00

Tgt Ion:112 Resp: 84657
Ion Ratio Lower Upper
112 100
64 65.8 53.2 79.8
63 40.8 32.6 48.8


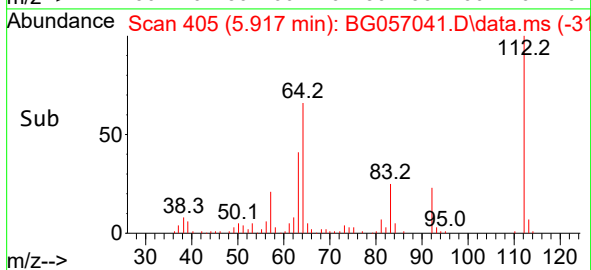

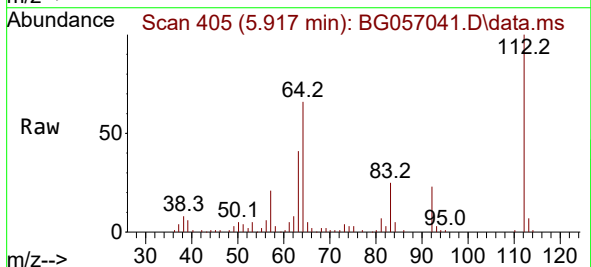


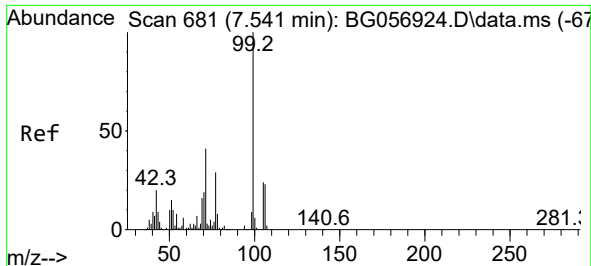

#7
Phenol-d6
Concen: 91.299 ng
RT: 7.539 min Scan# 681
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00




Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01


Tgt Ion: 99 Resp: 121810
Ion Ratio Lower Upper
99 100
42 19.9 15.7 23.5
71 42.5 32.5 48.7

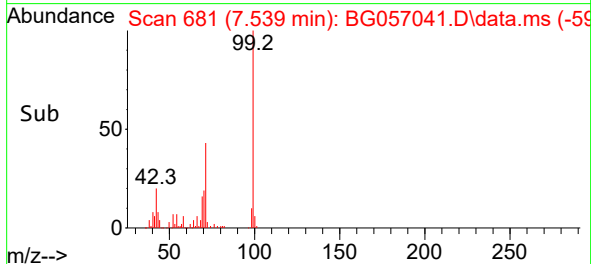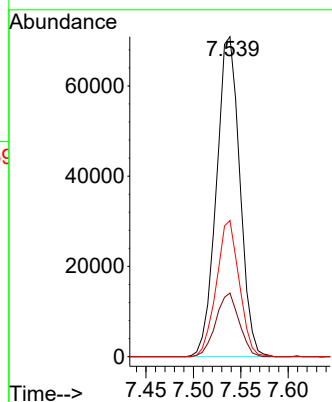

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.251 min Scan# 1313
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00

Tgt Ion:136 Resp: 58076
Ion Ratio Lower Upper
136 100
137 10.4 8.6 13.0
54 6.6 6.9 10.3#
68 5.4 3.8 5.6


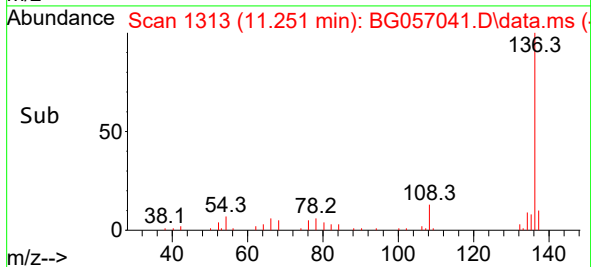

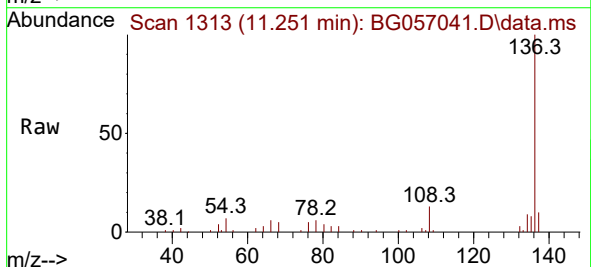


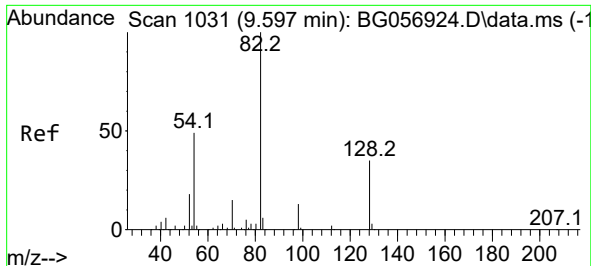

#23
Nitrobenzene-d5
Concen: 57.204 ng
RT: 9.583 min Scan# 1029
Delta R.T. -0.005 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00




Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01


Tgt Ion: 82 Resp: 81192
Ion Ratio Lower Upper
82 100
128 37.7 27.9 41.9
54 49.7 39.4 59.2

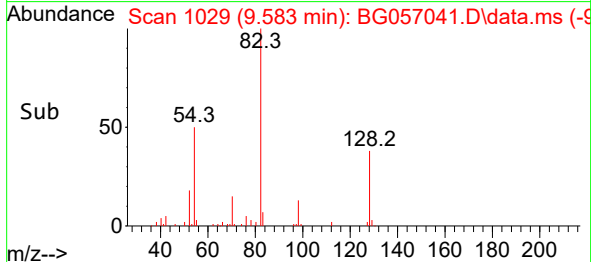

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.023 min Scan# 1955
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00

Tgt Ion: 164 Resp: 42136
Ion Ratio Lower Upper
164 100
162 100.4 77.8 116.8
160 44.5 33.5 50.3


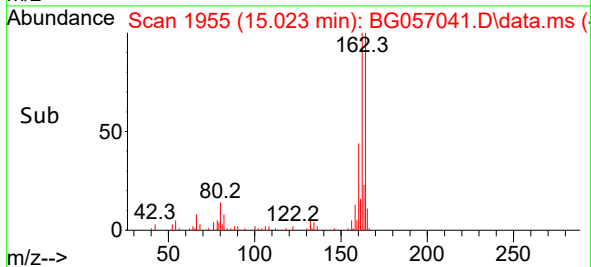

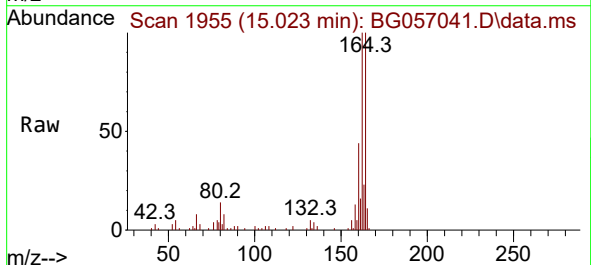


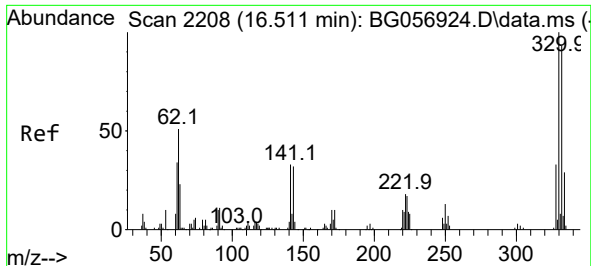

#42
2,4,6-Tribromophenol
Concen: 90.081 ng
RT: 16.503 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00




Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01


Tgt Ion:330 Resp: 60637
Ion Ratio Lower Upper
330 100
332 96.0 76.1 114.1
141 29.7 25.8 38.6

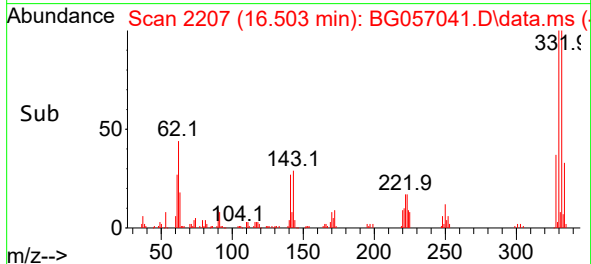

#45
2-Fluorobiphenyl
Concen: 61.407 ng
RT: 13.648 min Scan# 1721
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00

Tgt Ion:172 Resp: 190812
Ion Ratio Lower Upper
172 100
171 38.4 30.6 46.0
170 26.0 20.6 30.8


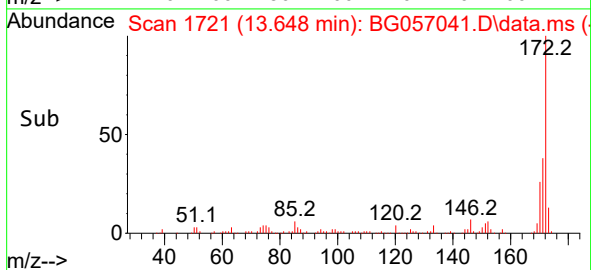

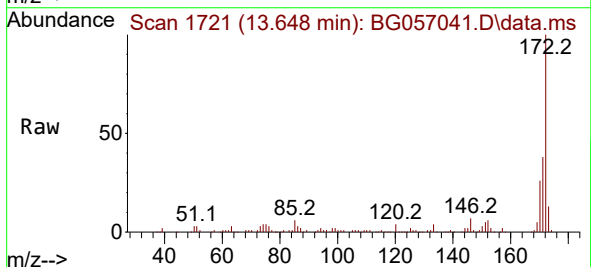


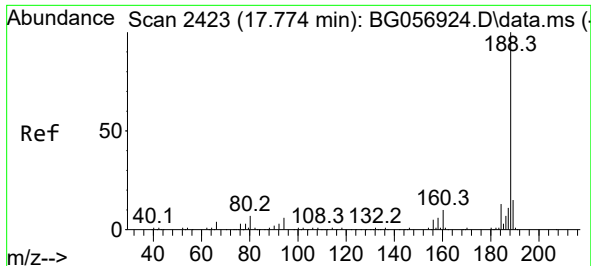

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.760 min Scan# 2423
Delta R.T. 0.000 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00




Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-01


Tgt Ion:188 Resp: 98302
Ion Ratio Lower Upper
188 100
94 5.0 4.6 6.8
80 8.3 5.5 8.3#

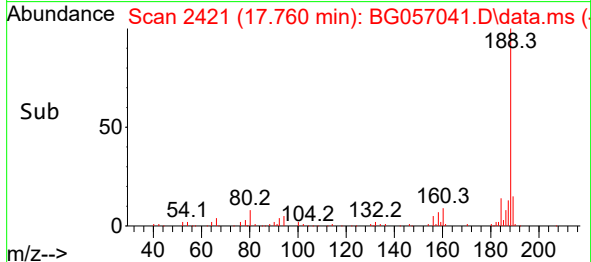

#76
Chrysene-d12
Concen: 20.000 ng
RT: 22.072 min Scan# 3155
Delta R.T. -0.011 min
Lab File: BG057041.D
Acq: 10 Apr 2023 12:00

Tgt Ion:240 Resp: 84330
Ion Ratio Lower Upper
240 100
120 4.2 3.8 5.6
236 26.2 21.0 31.6


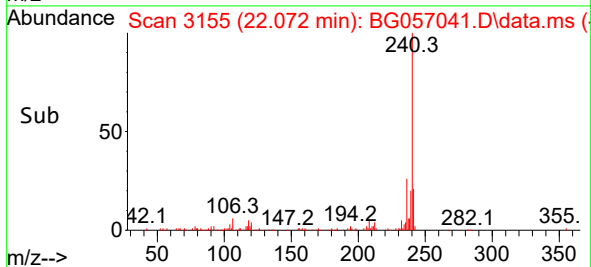

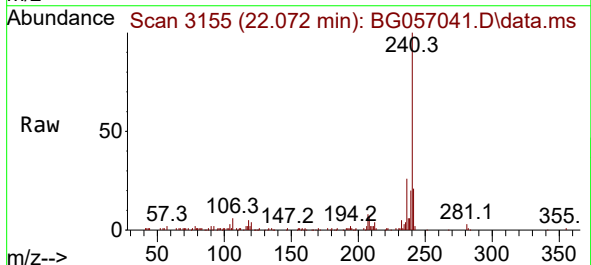


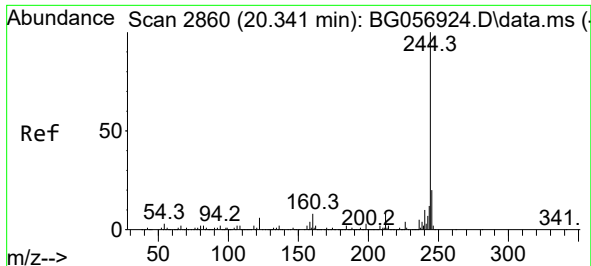

#79
 Terphenyl-d14
 Concen: 68.594 ng
 RT: 20.327 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BG057041.D
 Acq: 10 Apr 2023 12:00

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-01

Tgt Ion:244 Resp: 341845
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.1 9.1
 122 5.9 5.0 7.4

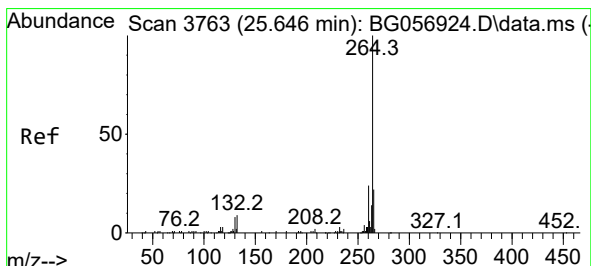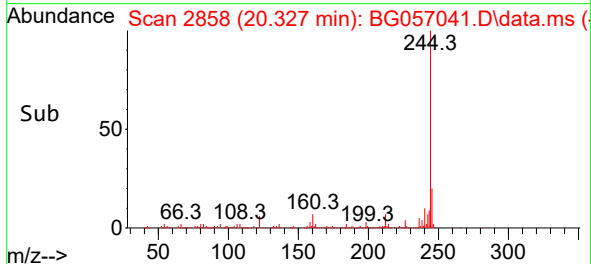

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.614 min Scan# 3758
 Delta R.T. -0.017 min
 Lab File: BG057041.D
 Acq: 10 Apr 2023 12:00

Tgt Ion:264 Resp: 93883
 Ion Ratio Lower Upper
 264 100
 260 26.6 19.0 28.4
 265 20.4 17.8 26.6

