

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057040.D
 Acq On : 10 Apr 2023 11:19
 Operator : CG/JU
 Sample : 02224-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.432	316	322	333	rBB	81701	131889	16.90%	3.815%
2	5.913	398	404	412	rBB	126569	210638	26.99%	6.093%
3	7.535	673	680	688	rBV	179746	308229	39.49%	8.916%
4	8.404	822	828	836	rBV	52133	86489	11.08%	2.502%
5	9.579	1021	1028	1036	rBB	109386	198028	25.37%	5.728%
6	11.247	1304	1312	1319	rBB	64891	119434	15.30%	3.455%
7	13.644	1710	1720	1727	rBV	311851	489464	62.71%	14.158%
8	15.019	1948	1954	1962	rBV	112362	178873	22.92%	5.174%
9	16.358	2175	2182	2187	rBV	12481	16871	2.16%	0.488%
10	16.499	2200	2206	2212	rBV	107428	158743	20.34%	4.592%
11	17.762	2414	2421	2428	rBV	148711	224559	28.77%	6.496%
12	18.596	2557	2563	2567	rBV5	4881	8257	1.06%	0.239%
13	19.959	2788	2795	2803	rVB7	4437	11915	1.53%	0.345%
14	20.329	2852	2858	2863	rBV	610780	780572	100.00%	22.579%
15	20.664	2911	2915	2919	rBV7	6573	11093	1.42%	0.321%
16	21.639	3077	3081	3088	rVB5	29330	49026	6.28%	1.418%
17	22.074	3149	3155	3163	rVB	135158	233566	29.92%	6.756%
18	25.616	3748	3758	3768	rVB2	78312	239411	30.67%	6.925%




Sum of corrected areas: 3457057

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057040.D
Acq On : 10 Apr 2023 11:19
Operator : CG/JU
Sample : 02224-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

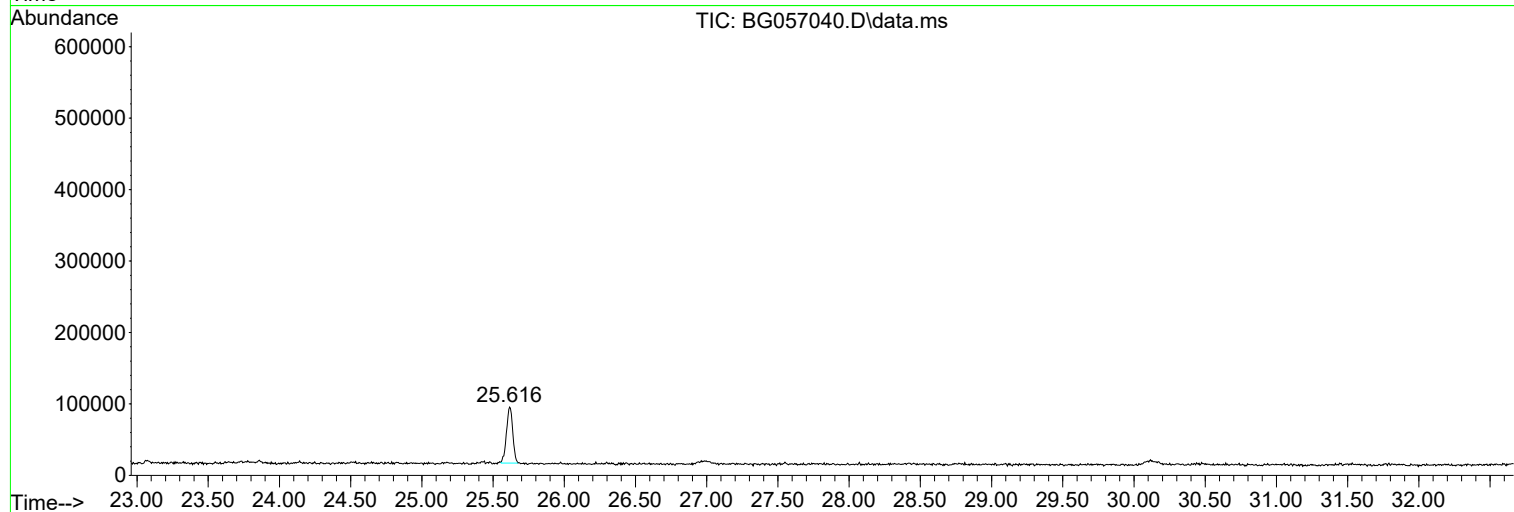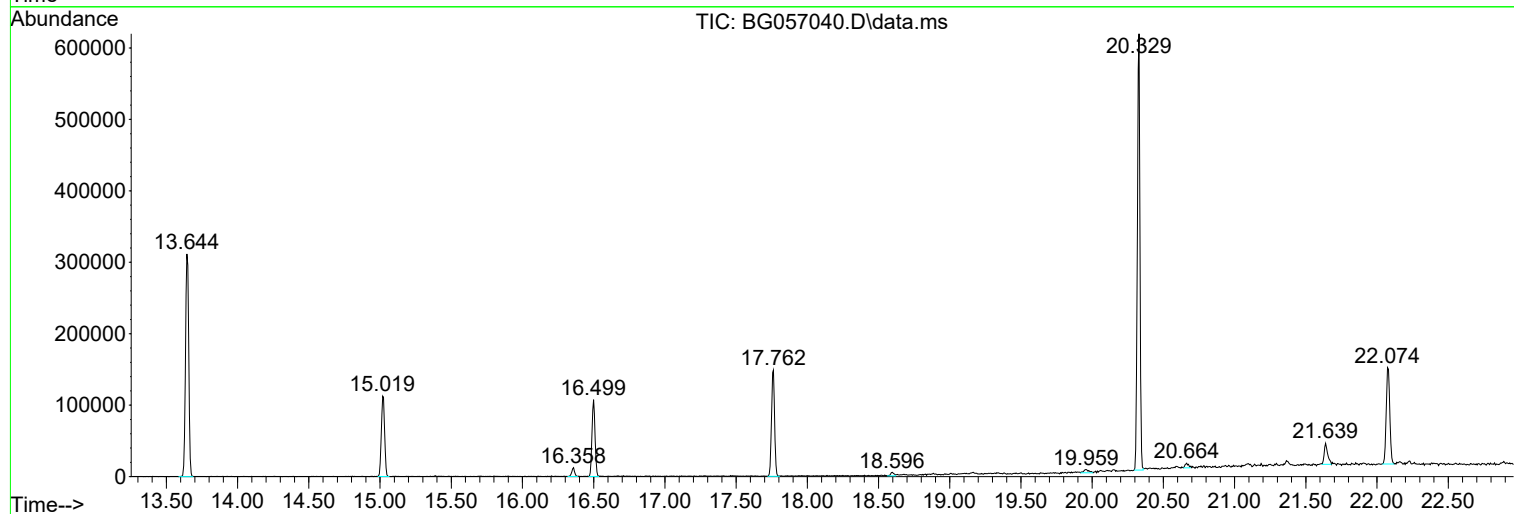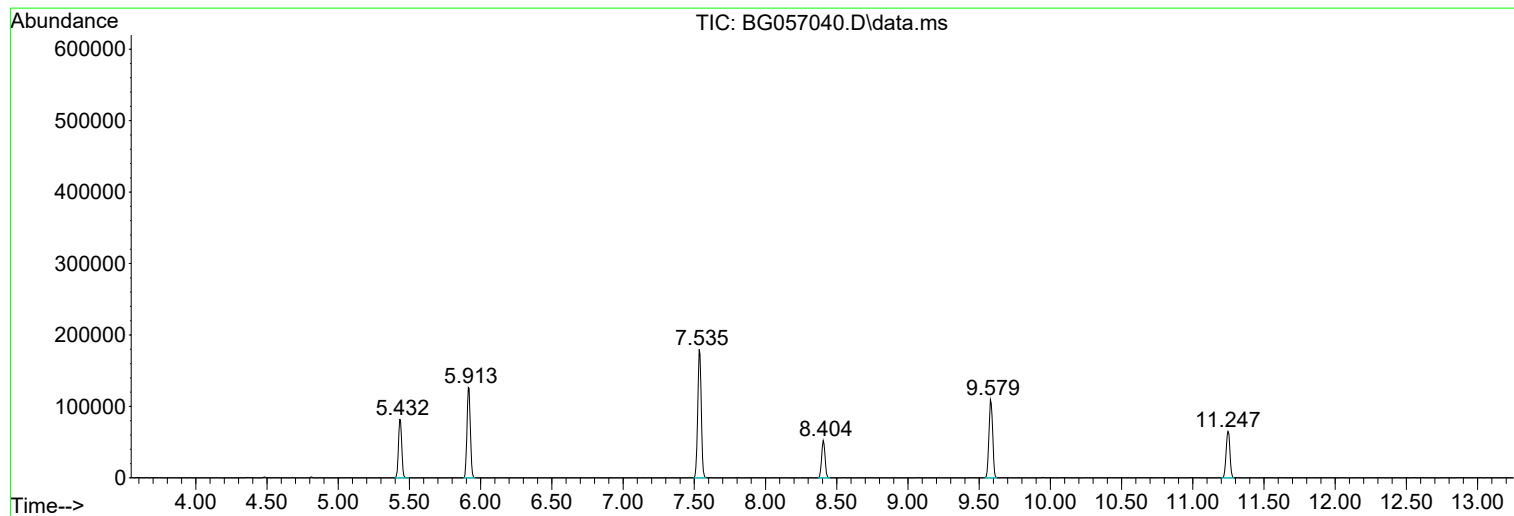

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057040.D
Acq On : 10 Apr 2023 11:19
Operator : CG/JU
Sample : 02224-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057040.D
Acq On : 10 Apr 2023 11:19
Operator : CG/JU
Sample : 02224-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------