

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041023\  
 Data File : BG057041.D  
 Acq On : 10 Apr 2023 12:00  
 Operator : CG/JU  
 Sample : 02224-01  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 OU3-FC-BACKFILL-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057041.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.436       | 317           | 323         | 330          | rBB      | 80794          | 131052        | 14.88%          | 3.176%        |
| 2         | 5.917       | 398           | 405         | 414          | rBB      | 204206         | 326889        | 37.11%          | 7.921%        |
| 3         | 7.539       | 673           | 681         | 691          | rBB      | 215058         | 368181        | 41.80%          | 8.921%        |
| 4         | 8.408       | 822           | 829         | 836          | rBB      | 52922          | 87516         | 9.93%           | 2.121%        |
| 5         | 9.583       | 1021          | 1029        | 1037         | rBV      | 128591         | 224987        | 25.54%          | 5.452%        |
| 6         | 11.251      | 1305          | 1313        | 1320         | rBB      | 67658          | 122506        | 13.91%          | 2.968%        |
| 7         | 13.648      | 1713          | 1721        | 1730         | rVB      | 375726         | 562685        | 63.88%          | 13.634%       |
| 8         | 15.023      | 1947          | 1955        | 1961         | rBV      | 114745         | 179886        | 20.42%          | 4.359%        |
| 9         | 16.356      | 2176          | 2182        | 2189         | rVB2     | 12808          | 16890         | 1.92%           | 0.409%        |
| 10        | 16.497      | 2200          | 2206        | 2218         | rVB      | 298186         | 438920        | 49.83%          | 10.635%       |
| 11        | 17.760      | 2414          | 2421        | 2433         | rBV      | 153406         | 229020        | 26.00%          | 5.549%        |
| 12        | 18.594      | 2558          | 2563        | 2571         | rBV3     | 18302          | 26889         | 3.05%           | 0.652%        |
| 13        | 20.327      | 2852          | 2858        | 2863         | rBV      | 681921         | 880888        | 100.00%         | 21.345%       |
| 14        | 21.637      | 3076          | 3081        | 3088         | rBV4     | 31267          | 55761         | 6.33%           | 1.351%        |
| 15        | 22.072      | 3150          | 3155        | 3163         | rVB      | 137206         | 234342        | 26.60%          | 5.678%        |
| 16        | 25.614      | 3748          | 3758        | 3772         | rVB      | 81992          | 240523        | 27.30%          | 5.828%        |




Sum of corrected areas: 4126935

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041023\  
Data File : BG057041.D  
Acq On : 10 Apr 2023 12:00  
Operator : CG/JU  
Sample : 02224-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
OU3-FC-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG033023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

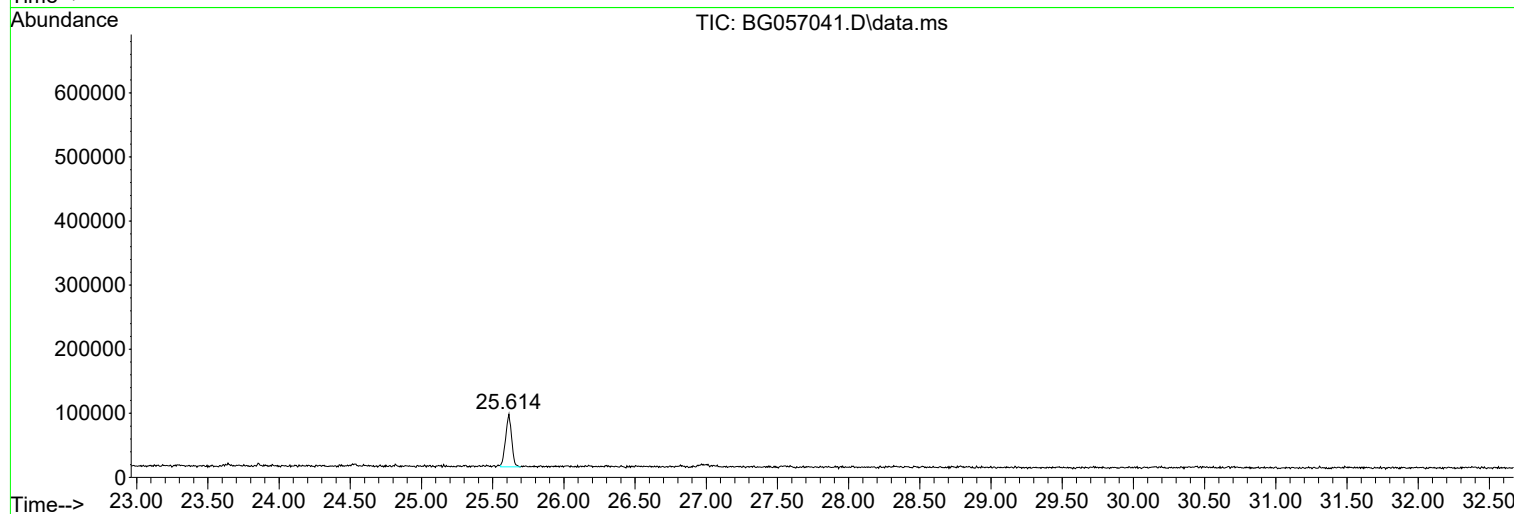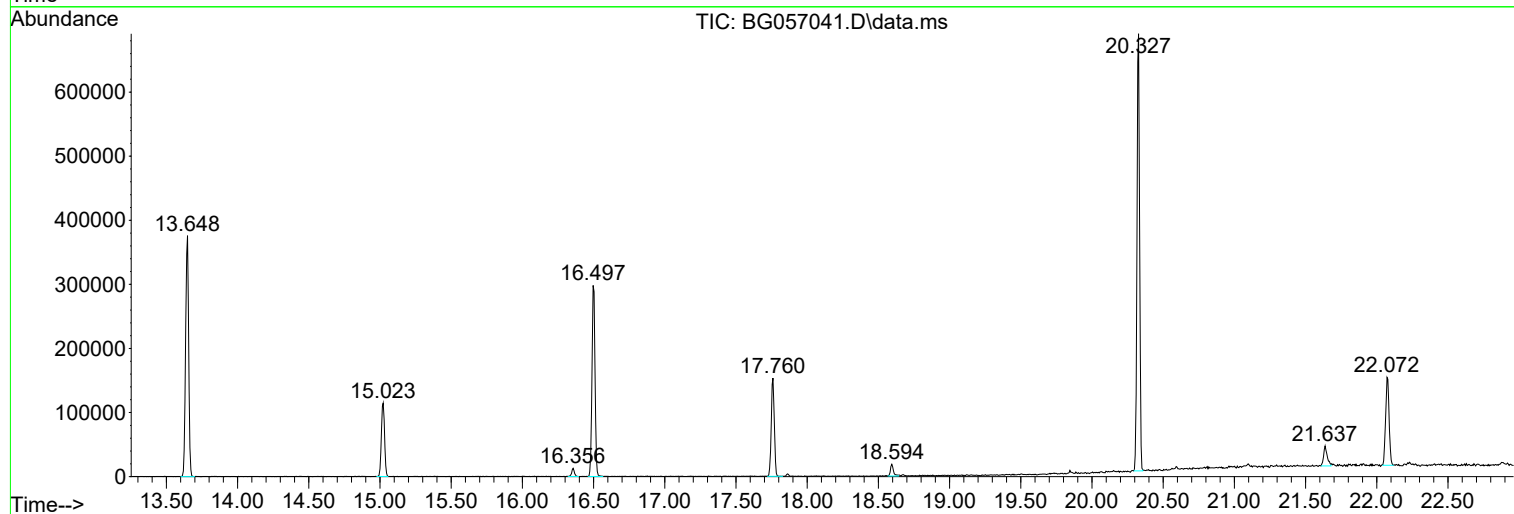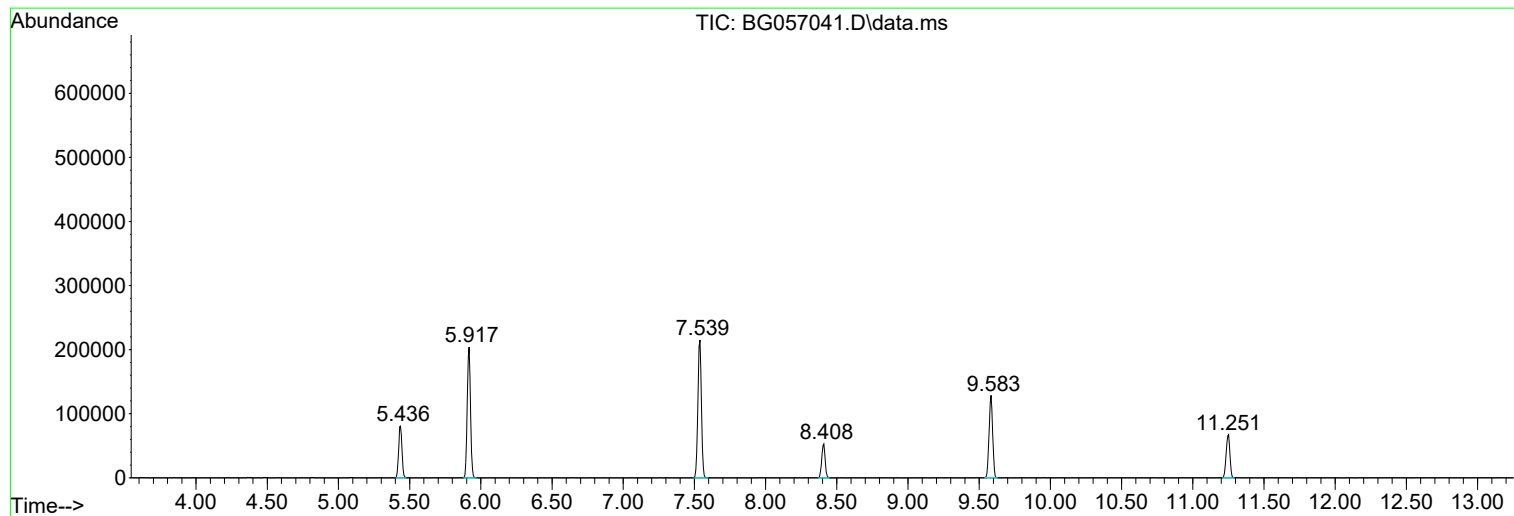

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041023\  
Data File : BG057041.D  
Acq On : 10 Apr 2023 12:00  
Operator : CG/JU  
Sample : 02224-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
OU3-FC-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG033023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041023\  
Data File : BG057041.D  
Acq On : 10 Apr 2023 12:00  
Operator : CG/JU  
Sample : 02224-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
OU3-FC-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG033023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|