

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057042.D
 Acq On : 10 Apr 2023 12:42
 Operator : CG/JU
 Sample : 02224-23
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-12

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.436	316	323	331	rBB	103552	155071	14.87%	3.258%
2	5.917	397	405	415	rBB	244158	391034	37.50%	8.216%
3	7.539	673	681	689	rBV	247989	435768	41.79%	9.156%
4	8.402	822	828	835	rBB	56553	94756	9.09%	1.991%
5	9.583	1021	1029	1038	rBB	149688	265149	25.43%	5.571%
6	11.245	1305	1312	1320	rVB	73756	129719	12.44%	2.725%
7	13.642	1713	1720	1728	rVB	448173	662821	63.56%	13.926%
8	15.017	1948	1954	1961	rBV	125269	189307	18.15%	3.977%
9	16.356	2175	2182	2187	rVB	20890	31609	3.03%	0.664%
10	16.497	2199	2206	2214	rBV	356808	525951	50.44%	11.050%
11	17.754	2414	2420	2427	rBV	160992	242937	23.30%	5.104%
12	18.588	2555	2562	2569	rBV3	22596	33888	3.25%	0.712%
13	20.327	2852	2858	2864	rBV	816471	1042795	100.00%	21.909%
14	21.637	3076	3081	3088	rBV3	37515	60963	5.85%	1.281%
15	22.072	3149	3155	3162	rBV	143189	243792	23.38%	5.122%
16	25.614	3748	3758	3768	rVB2	81632	254015	24.36%	5.337%




Sum of corrected areas: 4759575

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057042.D
Acq On : 10 Apr 2023 12:42
Operator : CG/JU
Sample : 02224-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

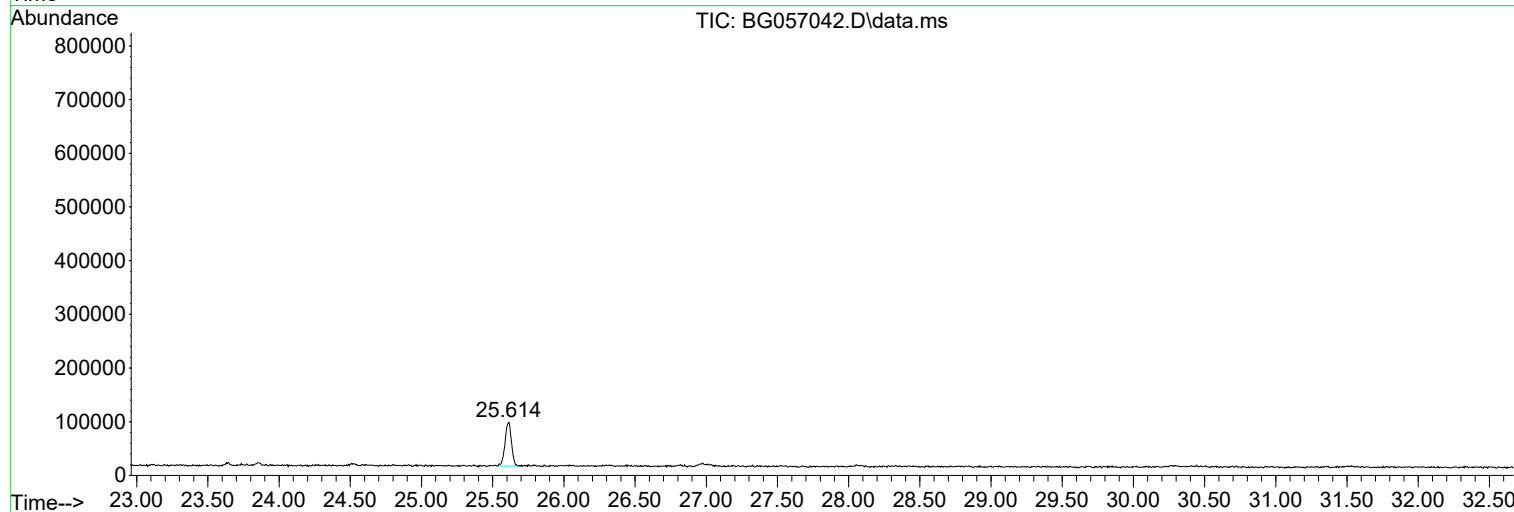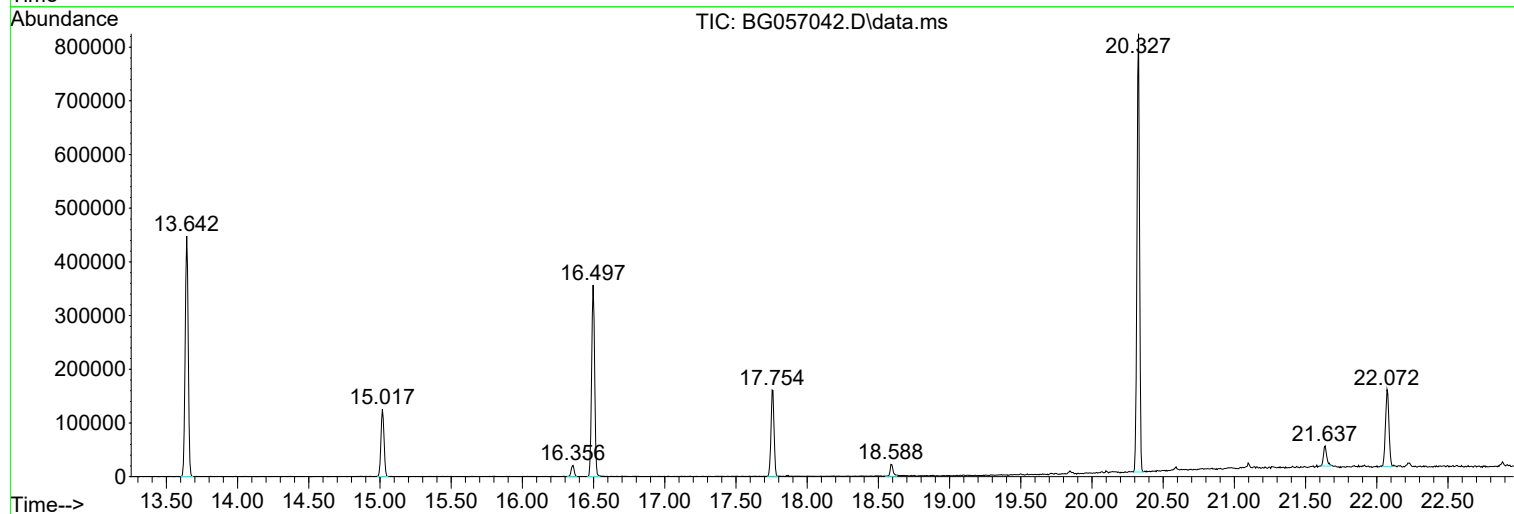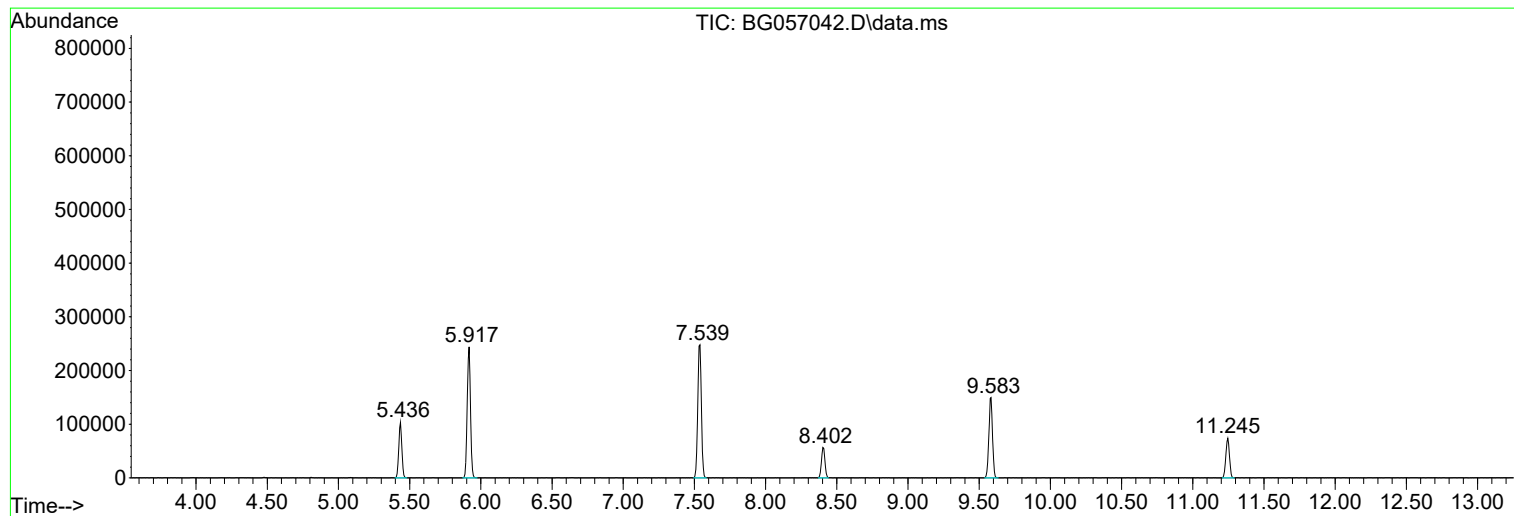

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057042.D
Acq On : 10 Apr 2023 12:42
Operator : CG/JU
Sample : 02224-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057042.D
Acq On : 10 Apr 2023 12:42
Operator : CG/JU
Sample : 02224-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------