

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057043.D
 Acq On : 10 Apr 2023 13:24
 Operator : CG/JU
 Sample : 02224-25
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.432	314	322	332	rBB	89183	140584	15.35%	3.161%
2	5.913	398	404	413	rBB	213429	353900	38.65%	7.957%
3	7.535	673	680	689	rBB	229495	393551	42.98%	8.848%
4	8.404	822	828	834	rBV2	58015	96244	10.51%	2.164%
5	9.579	1021	1028	1037	rBB	133645	235857	25.76%	5.303%
6	11.241	1304	1311	1320	rBV	73225	133207	14.55%	2.995%
7	13.644	1713	1720	1726	rBV	404364	594583	64.93%	13.368%
8	15.019	1947	1954	1960	rVB	130887	192661	21.04%	4.332%
9	16.352	2175	2181	2188	rBV	17779	26157	2.86%	0.588%
10	16.499	2199	2206	2214	rBV	307065	465530	50.84%	10.467%
11	17.756	2414	2420	2427	rVB	163872	243250	26.56%	5.469%
12	18.590	2557	2562	2566	rBV2	24353	32833	3.59%	0.738%
13	20.323	2852	2857	2862	rBV	739325	915726	100.00%	20.588%
14	21.099	2986	2989	2995	rVB7	7973	9604	1.05%	0.216%
15	21.633	3076	3080	3090	rVB3	30567	48936	5.34%	1.100%
16	22.074	3148	3155	3162	rBV	145059	255564	27.91%	5.746%
17	23.854	3453	3458	3465	rVB2	26571	53752	5.87%	1.209%
18	25.616	3748	3758	3768	rVB2	84480	255822	27.94%	5.752%




Sum of corrected areas: 4447761

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057043.D
Acq On : 10 Apr 2023 13:24
Operator : CG/JU
Sample : 02224-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

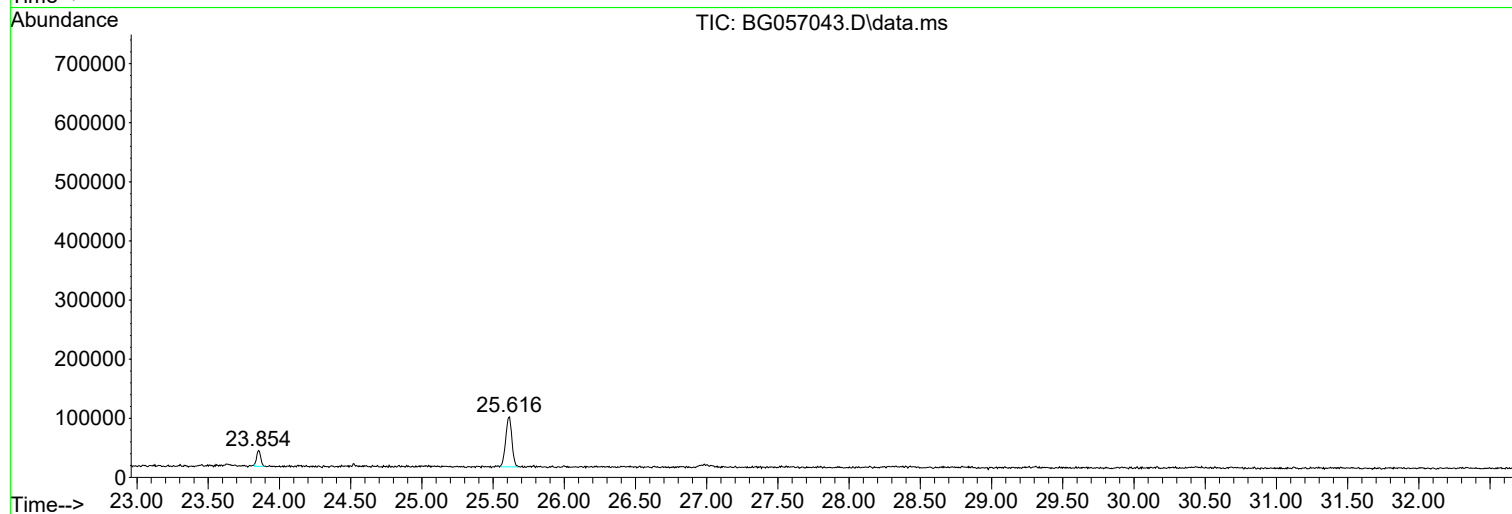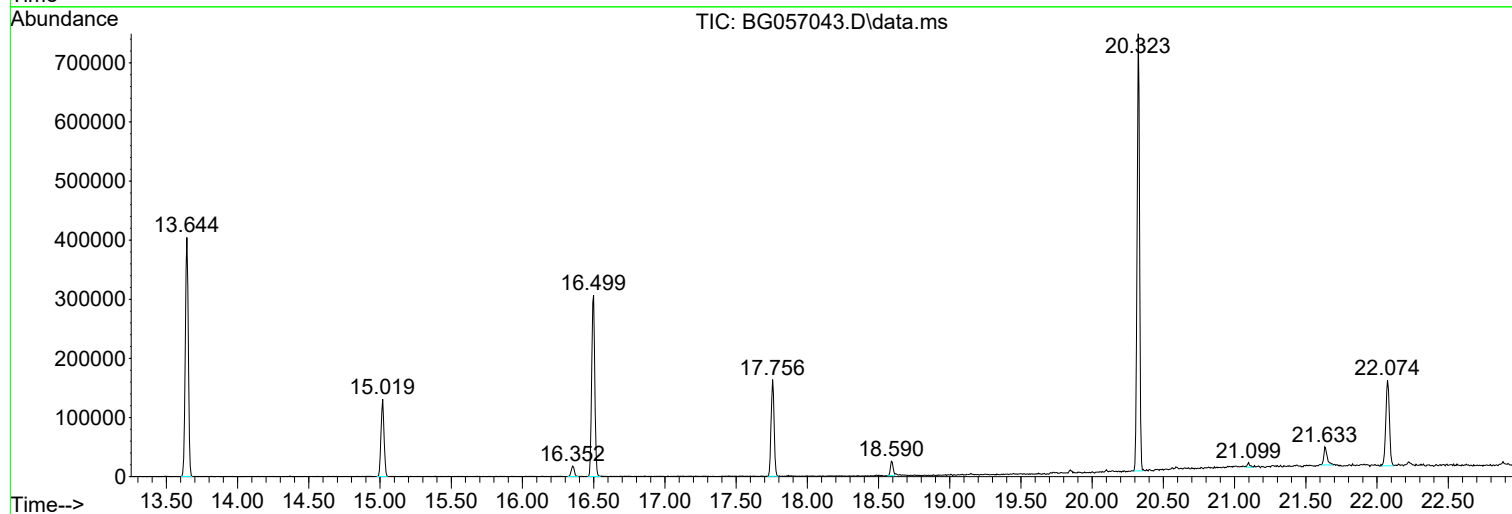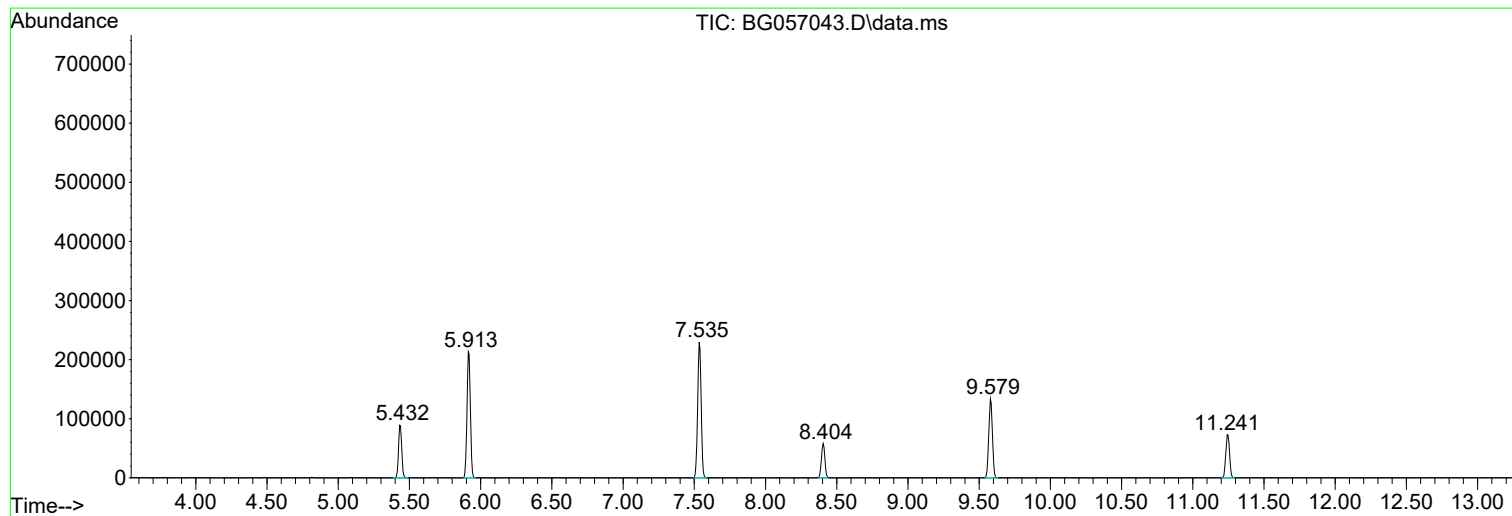

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057043.D
Acq On : 10 Apr 2023 13:24
Operator : CG/JU
Sample : 02224-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057043.D
Acq On : 10 Apr 2023 13:24
Operator : CG/JU
Sample : 02224-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------