

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057045.D
 Acq On : 10 Apr 2023 14:48
 Operator : CG/JU
 Sample : 02224-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.435	317	323	331	rBV	103799	163061	15.88%	3.280%
2	5.916	398	405	415	rVB	253069	411937	40.12%	8.286%
3	7.538	673	681	688	rBV	262988	457388	44.55%	9.200%
4	8.407	822	829	835	rBB2	61123	102277	9.96%	2.057%
5	9.582	1021	1029	1038	rBB	155947	276328	26.91%	5.558%
6	11.244	1305	1312	1319	rVB	83186	142811	13.91%	2.873%
7	13.641	1714	1720	1728	rBV	449181	678635	66.10%	13.651%
8	15.016	1948	1954	1961	rBV	131434	208327	20.29%	4.190%
9	16.355	2175	2182	2186	rVB2	14851	21186	2.06%	0.426%
10	16.496	2199	2206	2215	rBV	350793	526246	51.26%	10.585%
11	17.753	2414	2420	2428	rBV	169936	258783	25.21%	5.205%
12	18.593	2558	2563	2571	rBV2	23557	32562	3.17%	0.655%
13	19.845	2772	2776	2782	rBV6	6371	11435	1.11%	0.230%
14	20.326	2852	2858	2863	rBV	822689	1026709	100.00%	20.652%
15	21.636	3076	3081	3091	rVB3	39903	70179	6.84%	1.412%
16	22.071	3148	3155	3162	rBV	152285	272402	26.53%	5.479%
17	22.224	3176	3181	3187	rBV8	8425	15805	1.54%	0.318%
18	22.888	3289	3294	3297	rBV7	5986	10831	1.05%	0.218%
19	25.613	3748	3758	3771	rVB2	92577	284541	27.71%	5.724%




Sum of corrected areas: 4971443

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057045.D
Acq On : 10 Apr 2023 14:48
Operator : CG/JU
Sample : 02224-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

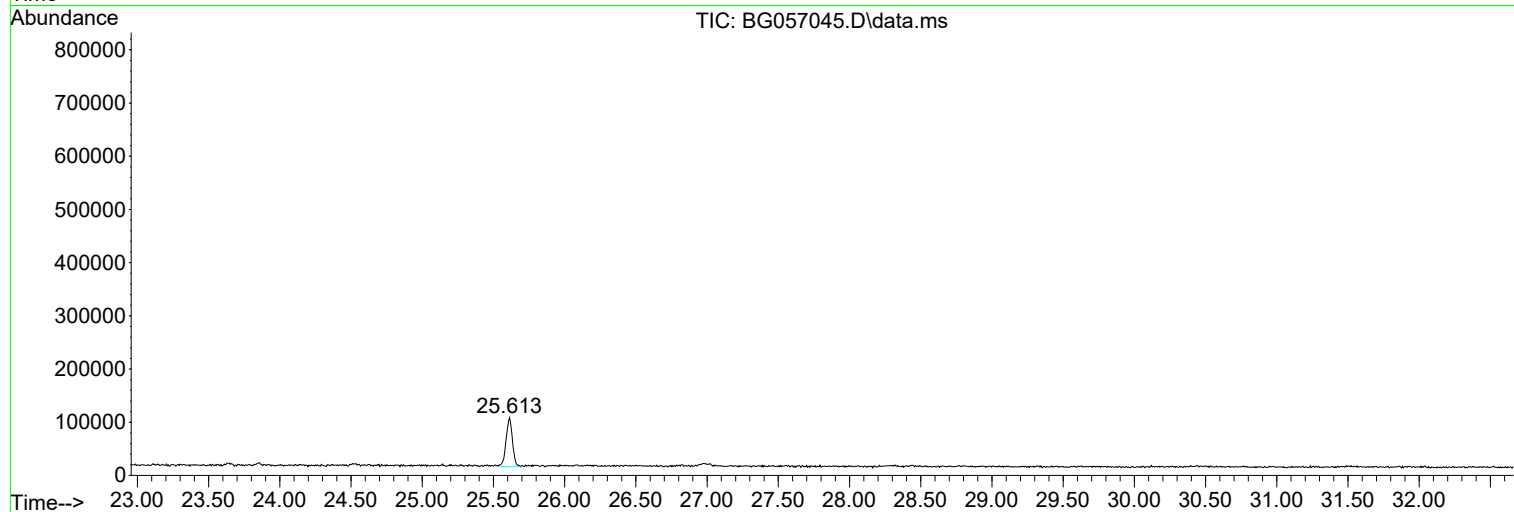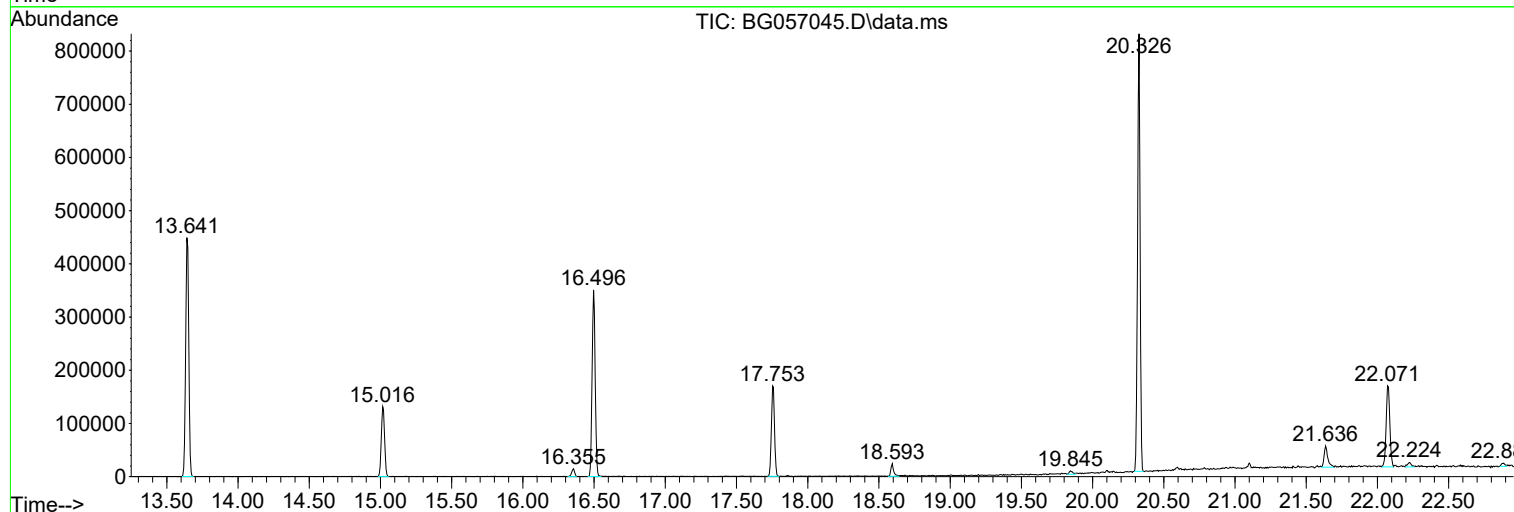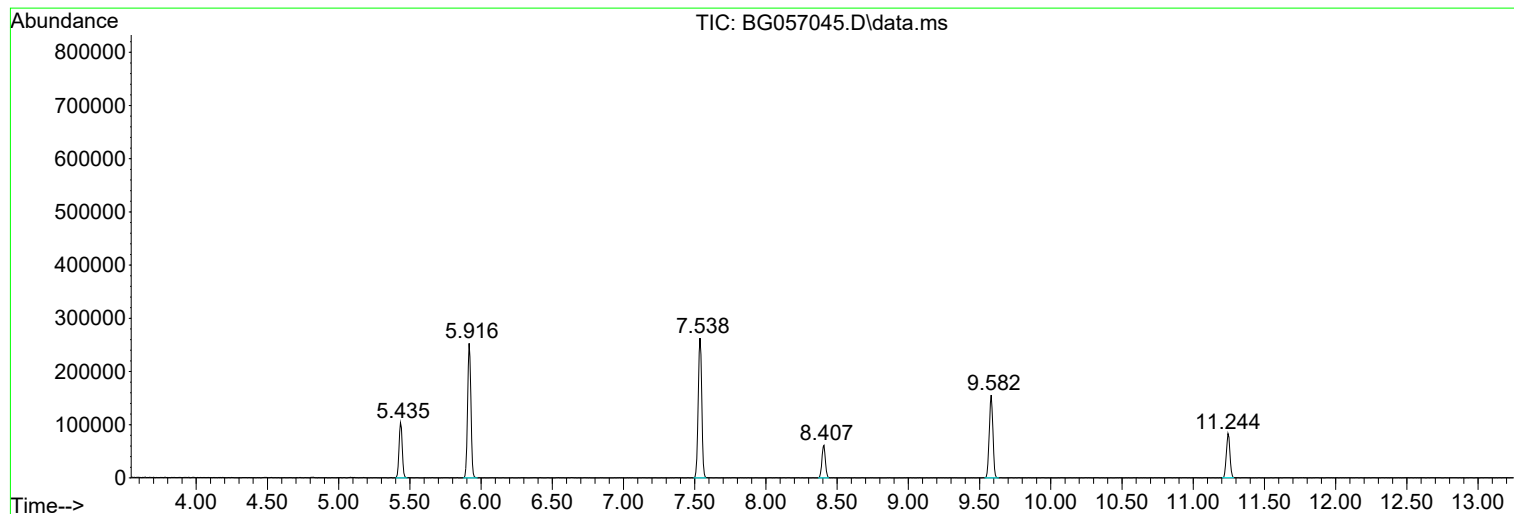

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057045.D
Acq On : 10 Apr 2023 14:48
Operator : CG/JU
Sample : 02224-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057045.D
Acq On : 10 Apr 2023 14:48
Operator : CG/JU
Sample : 02224-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------