
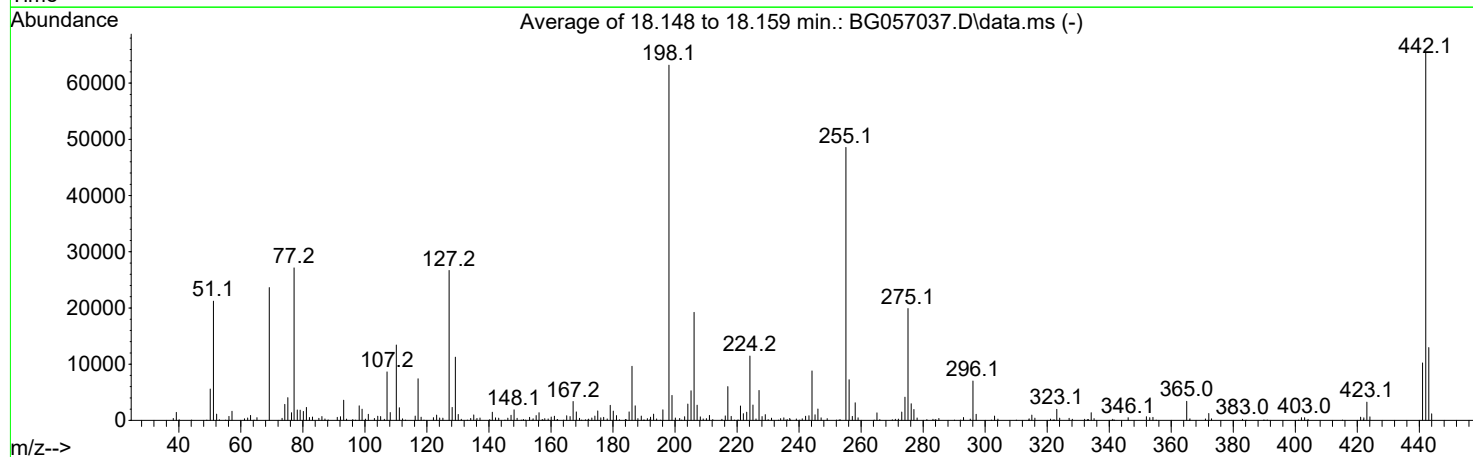


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057037.D
 Acq On : 10 Apr 2023 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 08 04:45:47 2023

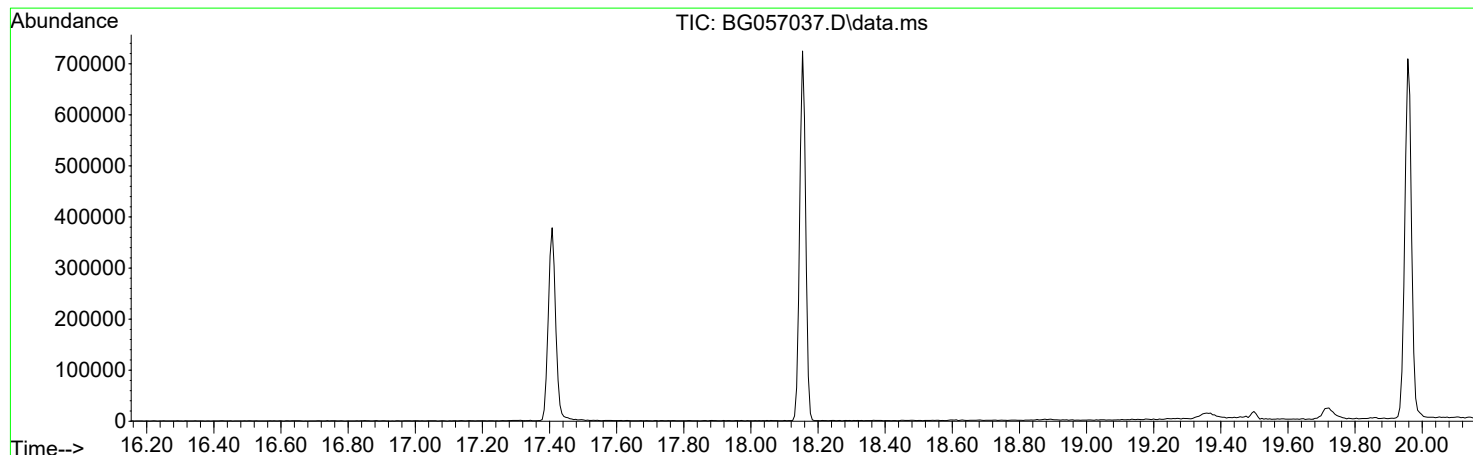




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	21219	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.4	23645	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	26667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63219	PASS
199	198	5	9	7.0	4447	PASS
275	198	10	60	31.5	19909	PASS
365	198	1	100	5.4	3399	PASS
441	198	0.01	100	16.2	10231	PASS
442	442	50	100	100.0	65451	PASS
443	442	15	24	19.8	12969	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
 Data File : BG057037.D
 Acq On : 10 Apr 2023 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 11 05:31:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 08 04:45:47 2023
 Response via : Initial Calibration

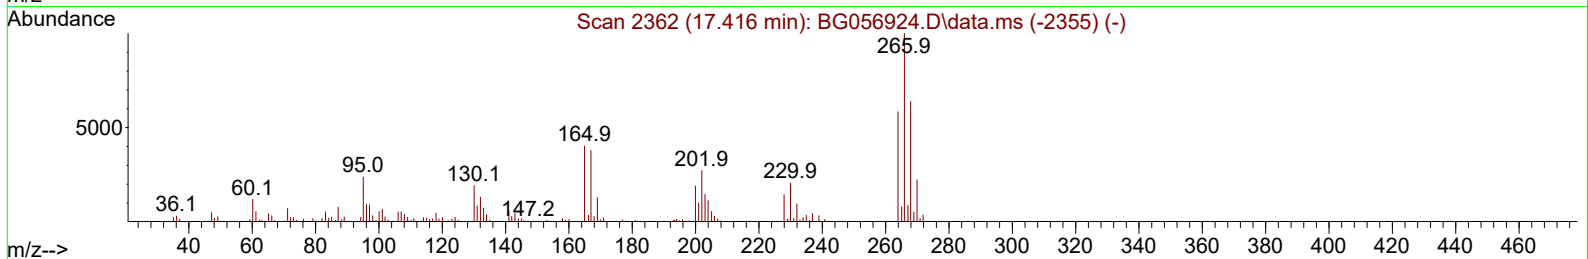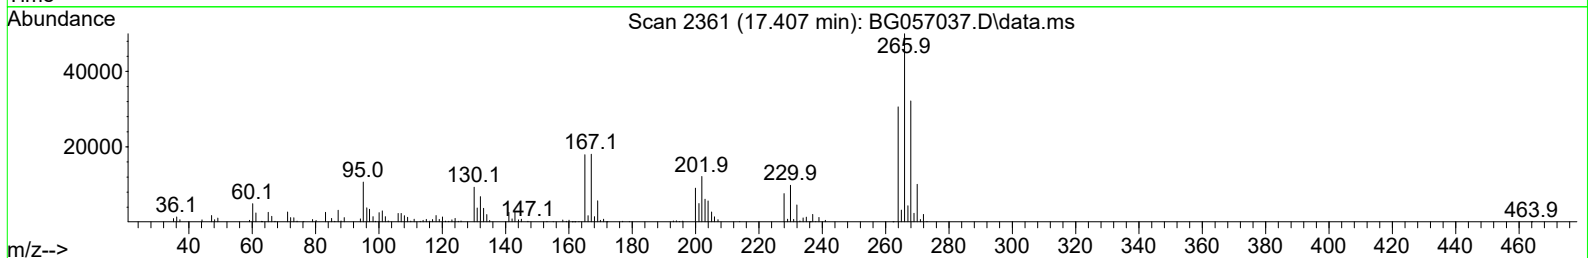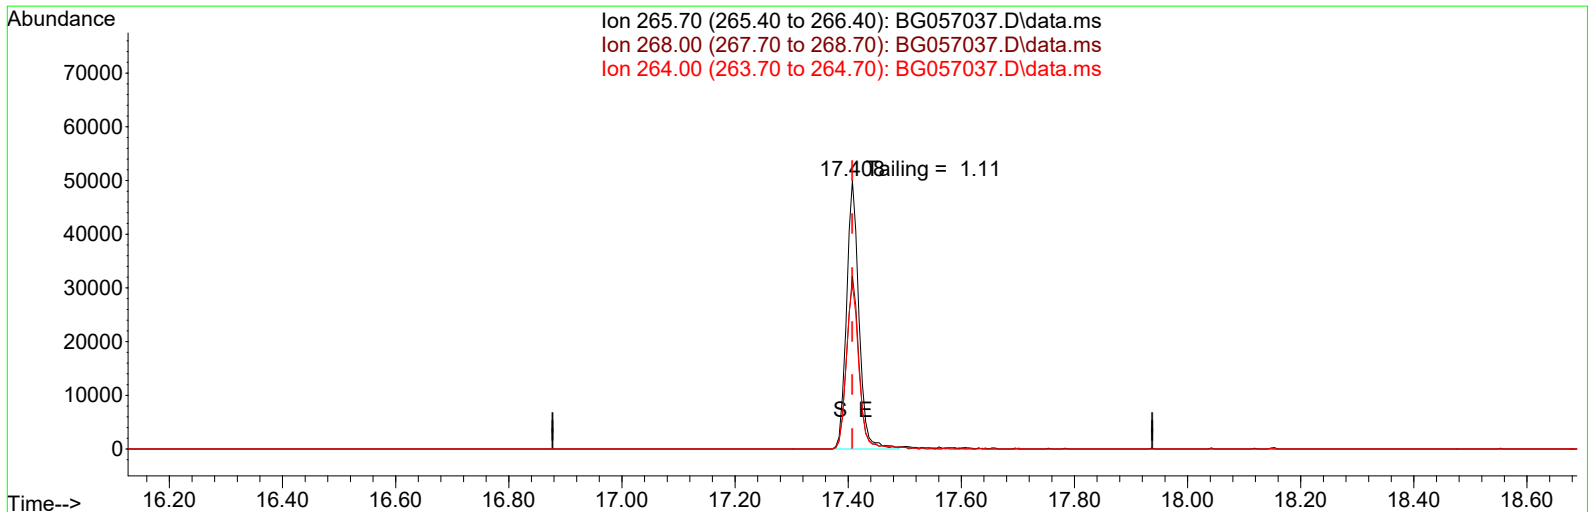

TIC: BG057037.D\data.ms

(70) Pentachlorophenol (C)

17.407min (+ 0.000) 20793.16 ng




response 76277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.35
264.00	58.50	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041023\
Data File : BG057037.D
Acq On : 10 Apr 2023 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 11 05:31:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

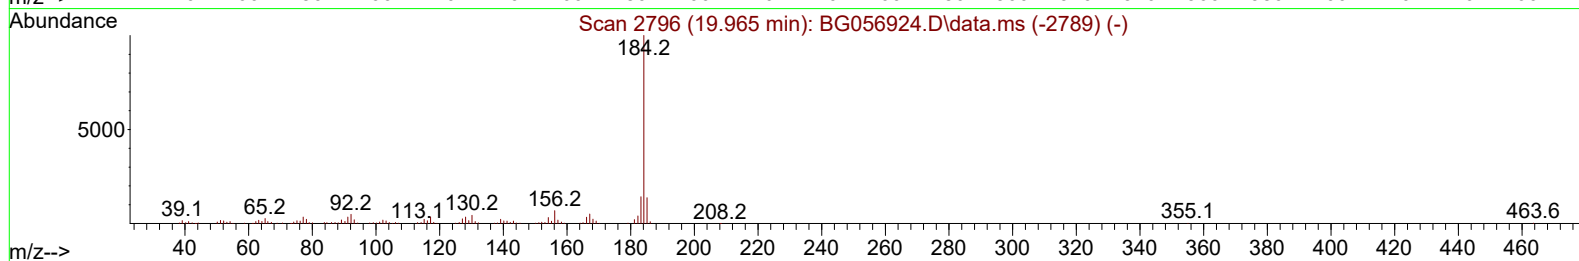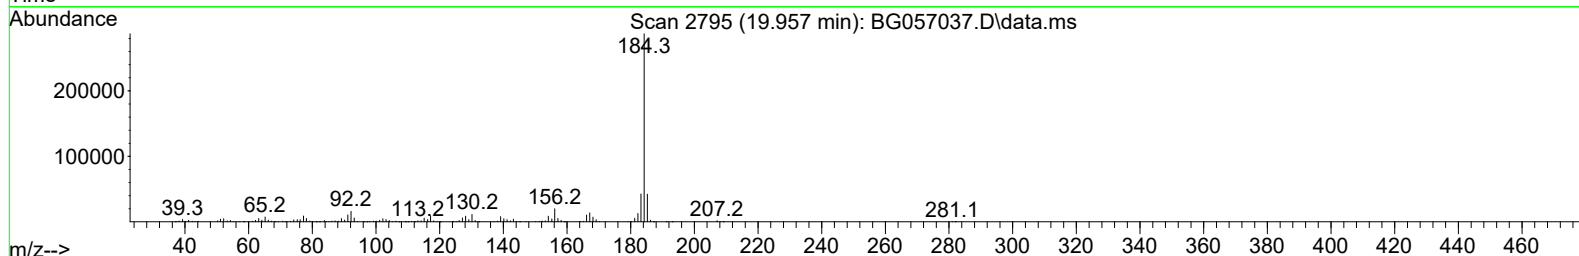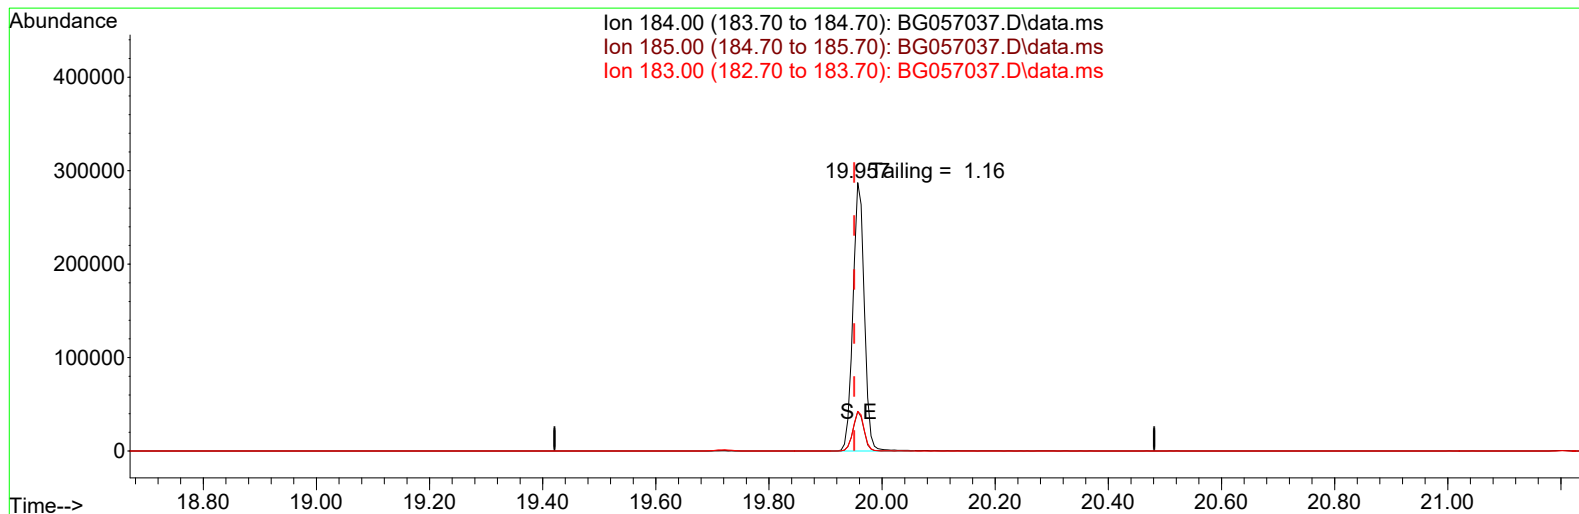

TIC: BG057037.D\data.ms

(77) Benzidine

19.957min (+ 0.006) 0.00 ng

response 401633

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.72
183.00	14.20	14.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/10/2023	BNA_G	BG057037.D
Compound Name	Response	Retention Time
DDT	203600	21.202
DDD	3173	20.791
DDE	120	20.239
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3293	206893	1.59

Instrument :
BNA_G
ClientSampleId :
DFTPP